

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052121\
 Data File : BF124018.D
 Acq On : 21 May 2021 15:00
 Operator : JU/CG
 Sample : PB136585BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB136585BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051421.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF124018.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.263	22	30	37	rVB	63968	88926	3.44%	0.552%
2	5.522	578	584	587	rBV	2208731	2189384	84.67%	13.602%
3	6.516	747	753	756	rBV	1928703	2180072	84.31%	13.545%
4	6.886	813	816	820	rVB	547345	474322	18.34%	2.947%
5	7.451	906	912	915	rBV	1392425	1450093	56.08%	9.009%
6	8.175	1030	1035	1038	rBV	650377	619471	23.96%	3.849%
7	9.251	1212	1218	1221	rBV	3099090	2585903	100.00%	16.066%
8	9.927	1328	1333	1336	rBV	906242	708478	27.40%	4.402%
9	10.716	1462	1467	1470	rBV	1795327	1579341	61.08%	9.812%
10	11.416	1582	1586	1589	rBV	876104	703036	27.19%	4.368%
11	13.004	1851	1856	1859	rBV	2818010	2571312	99.44%	15.975%
12	14.057	2031	2035	2038	rVB	624373	516941	19.99%	3.212%
13	15.545	2282	2288	2292	rBV2	362463	428320	16.56%	2.661%




Sum of corrected areas: 16095599

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052121\
Data File : BF124018.D
Acq On : 21 May 2021 15:00
Operator : JU/CG
Sample : PB136585BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB136585BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

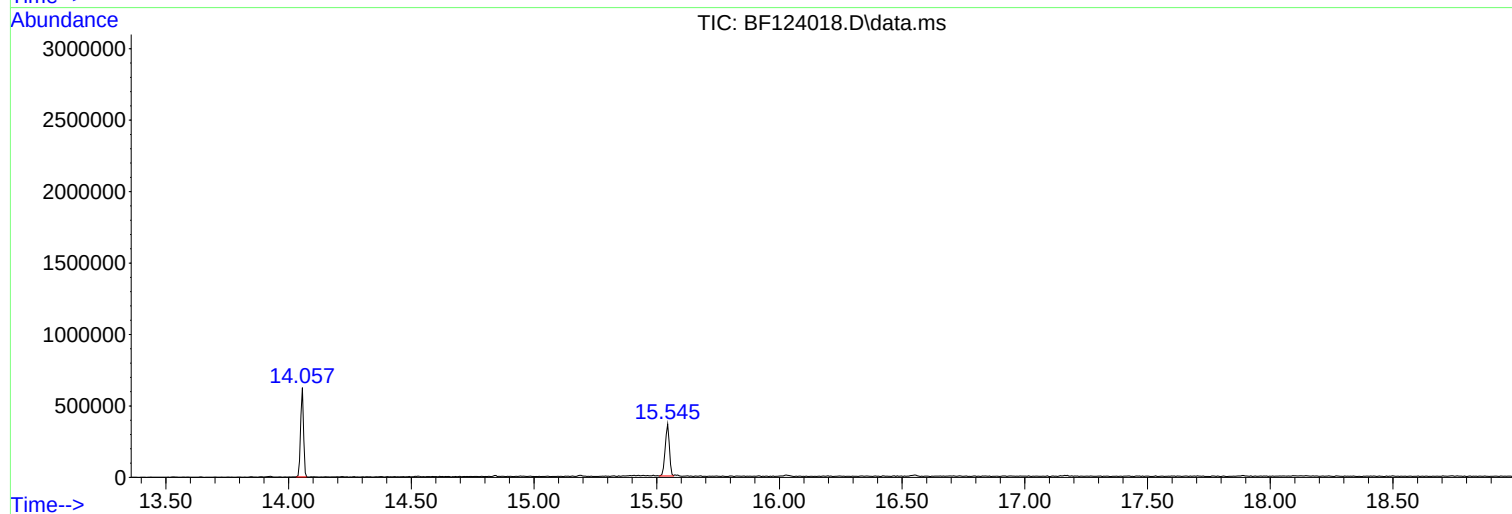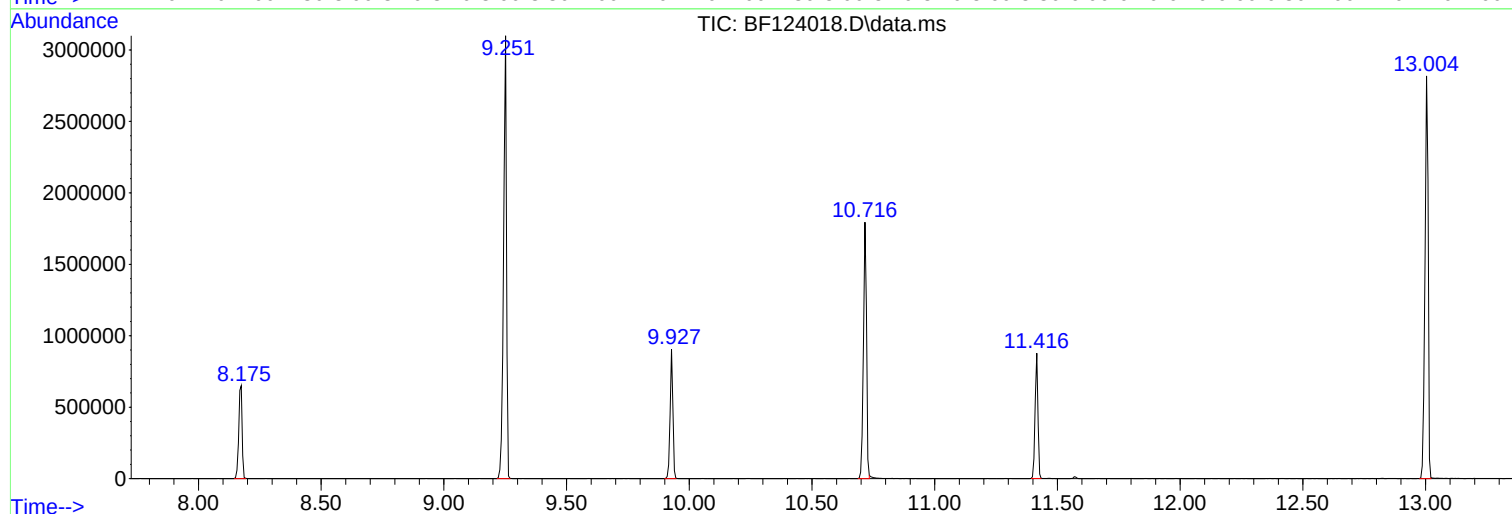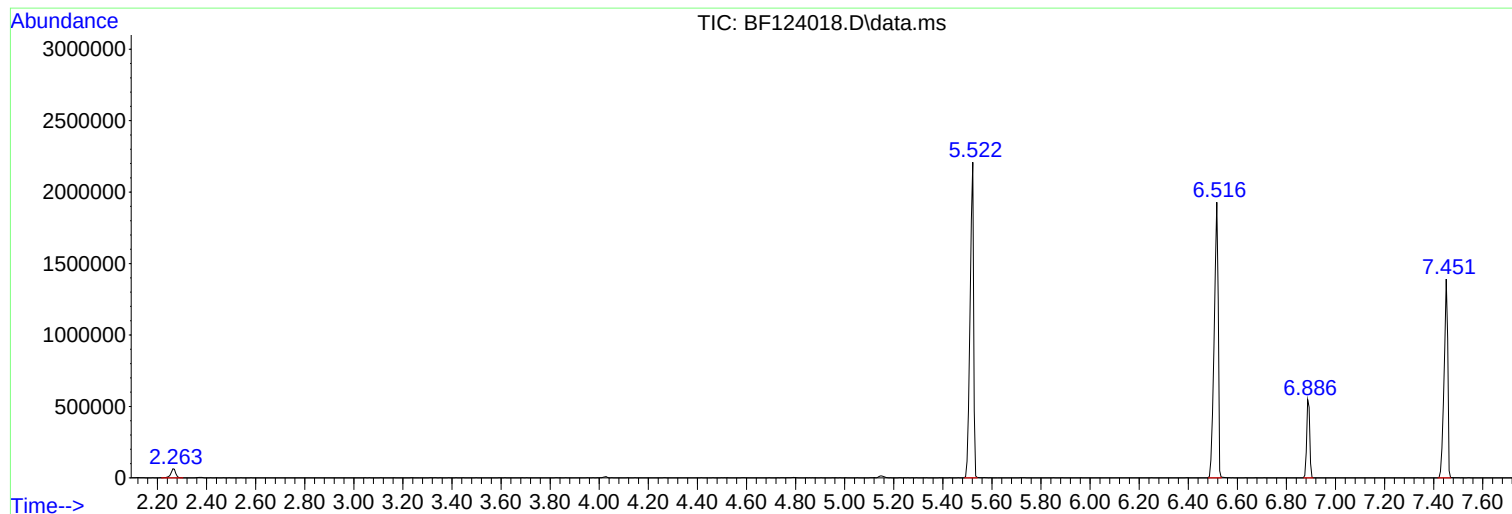

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052121\
Data File : BF124018.D
Acq On : 21 May 2021 15:00
Operator : JU/CG
Sample : PB136585BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB136585BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.263	3.75 ng	88926	1,4-Dichlorobenzene-d4	6.886

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	72
2			2-Methyl-5-hexen-3-ol	114	C7H14O	032815-70-6	25
3			(Aminomethyl)cyclopropane	71	C4H9N	002516-47-4	9
4			3-Pentanol, 2,4-dimethyl-	116	C7H16O	000600-36-2	9
5			Silane, tetramethyl-	88	C4H12Si	000075-76-3	9

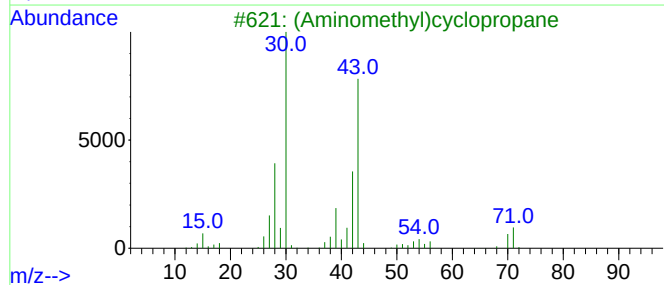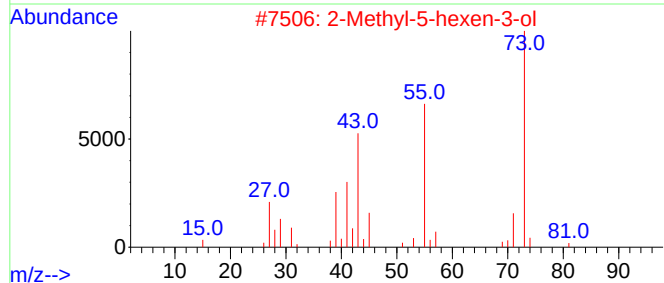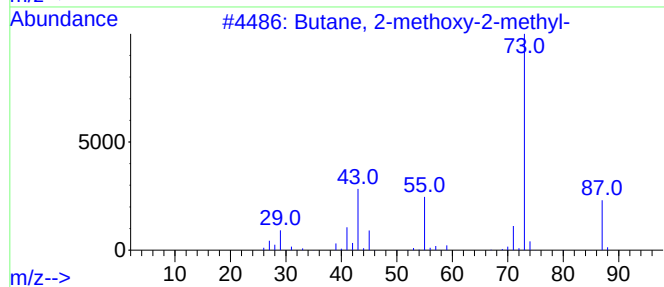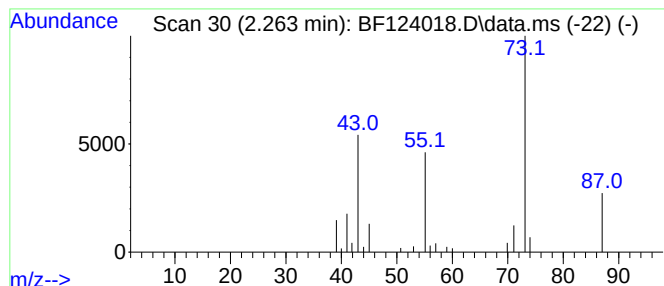

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052121\
Data File : BF124018.D
Acq On : 21 May 2021 15:00
Operator : JU/CG
Sample : PB136585BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB136585BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	2.263	3.8	ng	88926	1	6.886	474322	20.0