
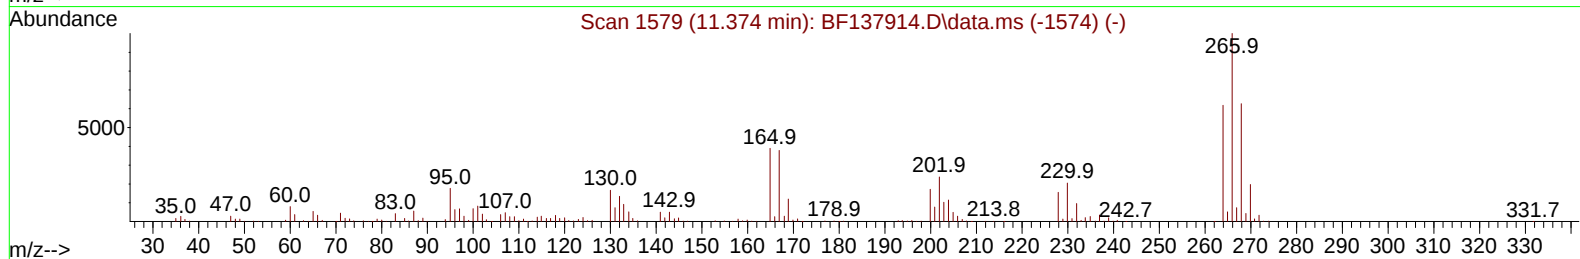
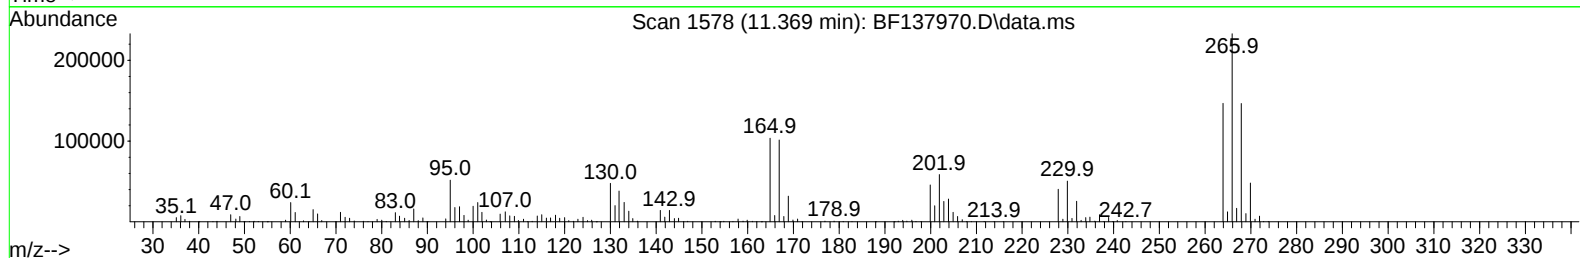


```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052124\  
Data File : BF137970.D  
Acq On    : 21 May 2024  10:52  
Operator  : CG\JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: May 21 11:39:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF051424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 15 04:12:16 2024
Response via : Initial Calibration

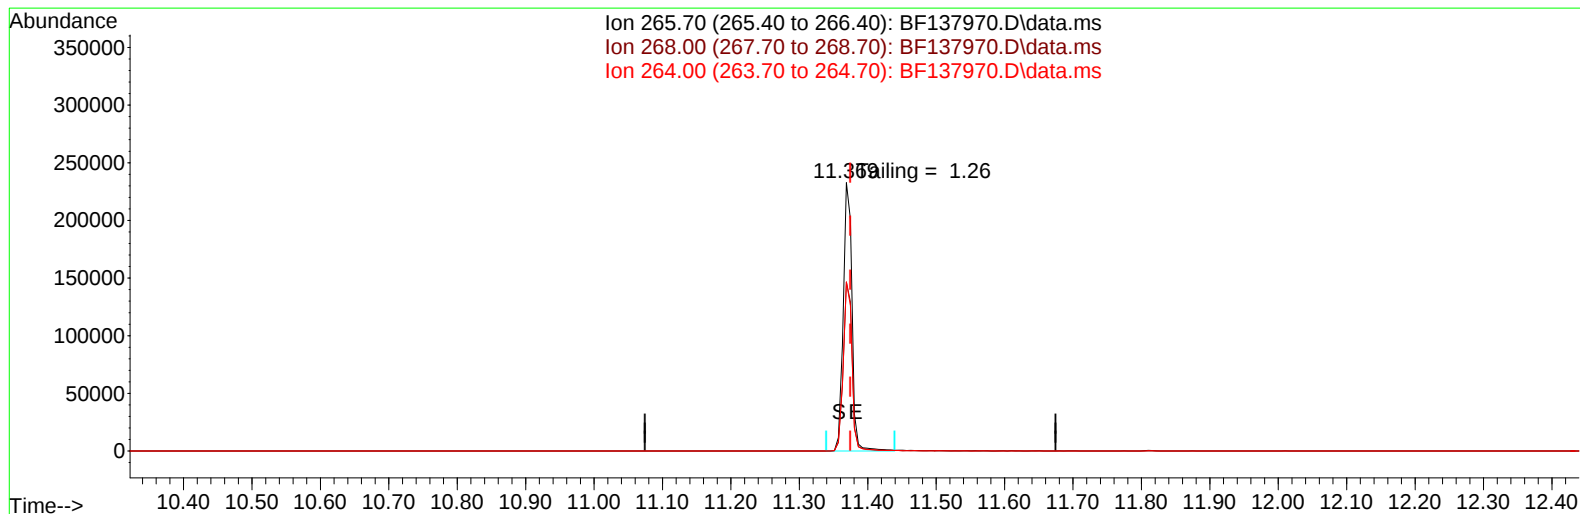

TIC: BF137970.D\data.ms

(70) **Pentachlorophenol (C)**




11.369min (-0.006) 344749.28 ng

response **208010**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	62.96
264.00	61.80	63.05
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052124\
Data File : BF137970.D
Acq On : 21 May 2024 10:52
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 21 11:39:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF051424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 15 04:12:16 2024
Response via : Initial Calibration

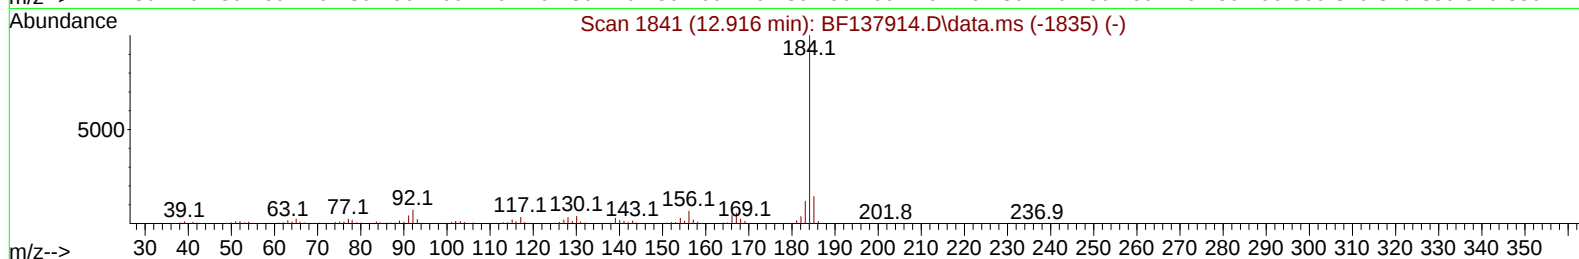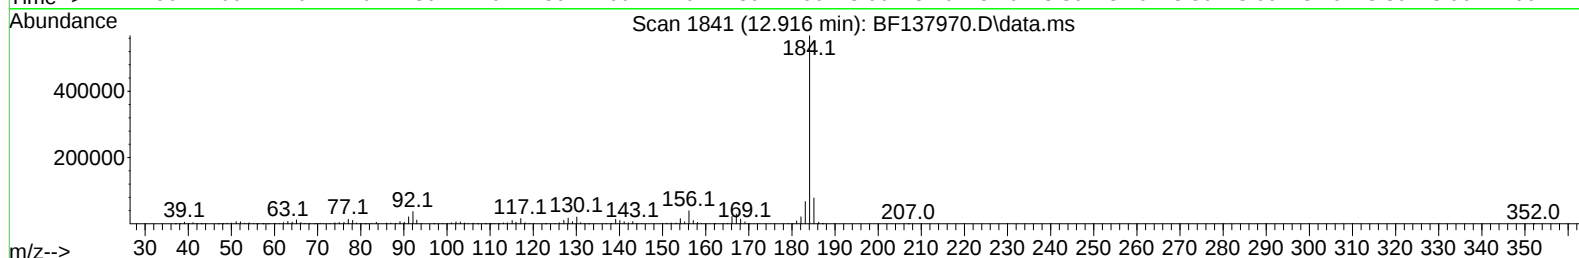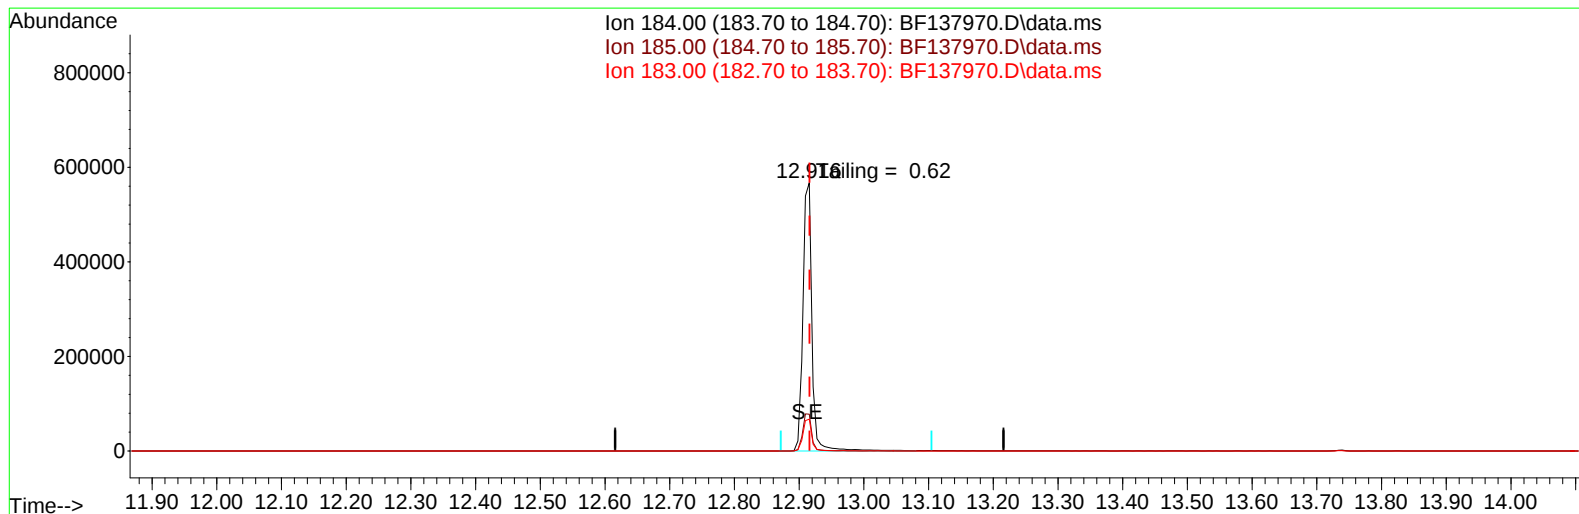

TIC: BF137970.D\data.ms

(77) Benzidine

12.916min (-0.000) 6617.67 ng m

response **553941**

Ion	Exp%	Act%
-----	------	------

184.00	100.00	100.00
--------	--------	--------

185.00	14.30	13.76
--------	-------	-------

183.00	11.90	11.90
--------	-------	-------

0.00 0.00 0.00