

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052124\
Data File : BF137974.D
Acq On : 21 May 2024 12:52
Operator : CG\JU
Sample : PB160998BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB160998BL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF051424.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF137974.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.463	52	64	69	rVB	105659	156139	2.80%	0.509%
2	5.669	603	609	612	rBV	3636872	3608797	64.72%	11.755%
3	6.651	770	776	779	rBV	3212091	3559726	63.84%	11.596%
4	7.034	837	841	844	rBV	1105887	900230	16.14%	2.932%
5	7.593	930	936	939	rBV	2198419	2392849	42.91%	7.795%
6	8.316	1054	1059	1062	rBV	1443226	1221067	21.90%	3.978%
7	9.392	1236	1242	1245	rBV	5400148	5065365	90.84%	16.500%
8	10.081	1353	1359	1362	rBV	1708607	1467838	26.32%	4.781%
9	10.875	1488	1494	1497	rBV	3325115	3167000	56.79%	10.316%
10	11.575	1609	1613	1616	rBV	1900350	1513442	27.14%	4.930%
11	13.163	1878	1883	1886	rBV	5728100	5576361	100.00%	18.165%
12	14.221	2059	2063	2067	rBV	1369686	1155425	20.72%	3.764%
13	15.786	2323	2329	2338	rBV	697273	914717	16.40%	2.980%




Sum of corrected areas: 30698956

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052124\
Data File : BF137974.D
Acq On : 21 May 2024 12:52
Operator : CG\JU
Sample : PB160998BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB160998BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF051424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

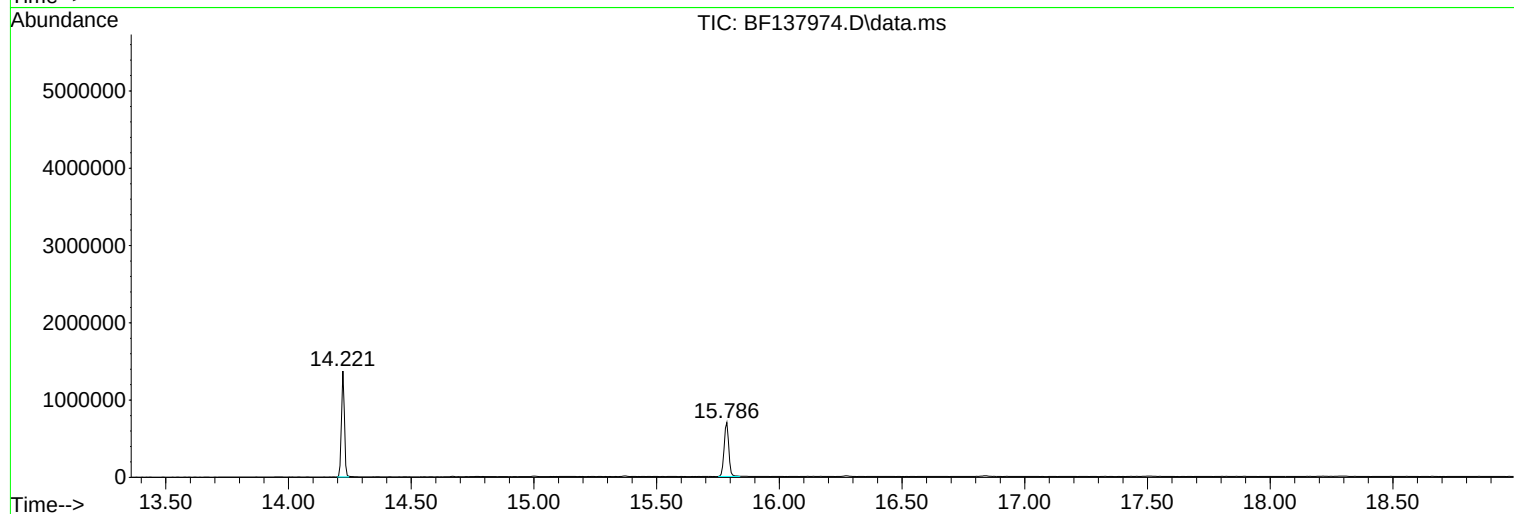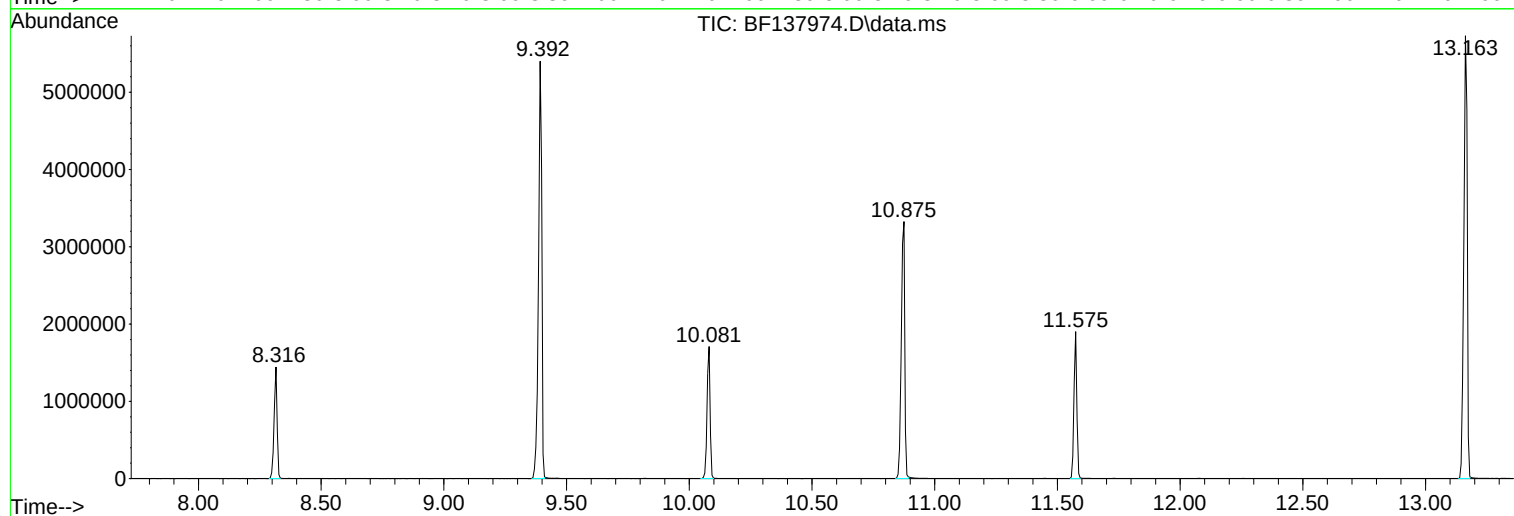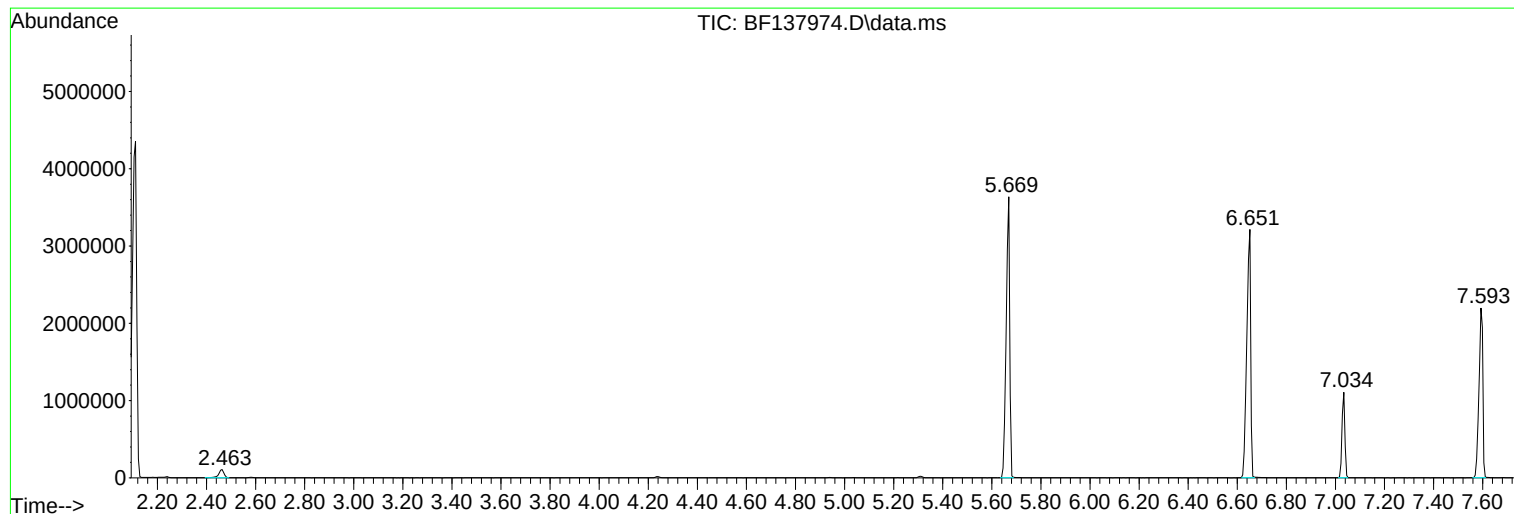

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052124\
Data File : BF137974.D
Acq On : 21 May 2024 12:52
Operator : CG\JU
Sample : PB160998BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB160998BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF051424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.463	3.47 ng	156139	1,4-Dichlorobenzene-d4	7.034

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	83
2			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	40
3			Silane, ethyltrimethyl-	102	C5H14Si	003439-38-1	36
4			Octanal, 7-methoxy-3,7-dimethyl-	186	C11H22O2	003613-30-7	23
5			Pentane, 3-methoxy-	102	C6H14O	036839-67-5	17

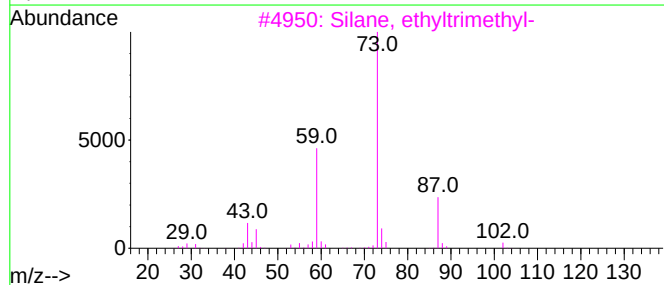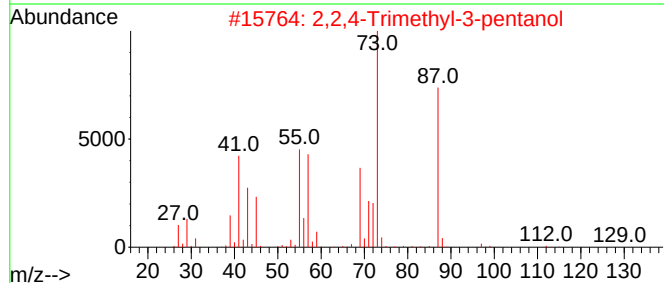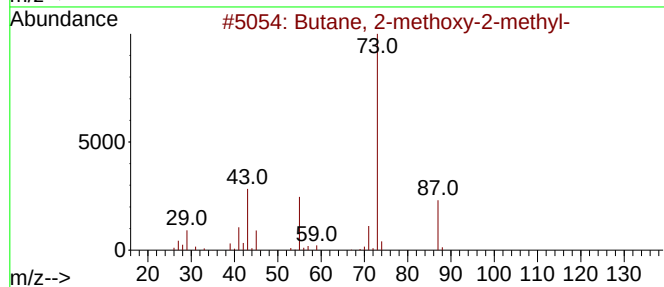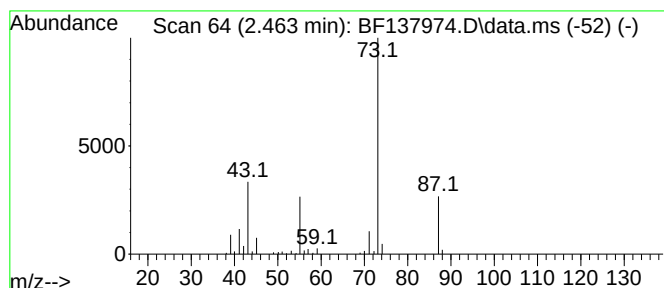

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052124\
Data File : BF137974.D
Acq On : 21 May 2024 12:52
Operator : CG\JU
Sample : PB160998BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB160998BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF051424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	2.463	3.5	ng	156139	1	7.034	900230	20.0