


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052124\
Data File : BF137970.D
Acq On : 21 May 2024 10:52
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF051424.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed May 15 04:12:16 2024

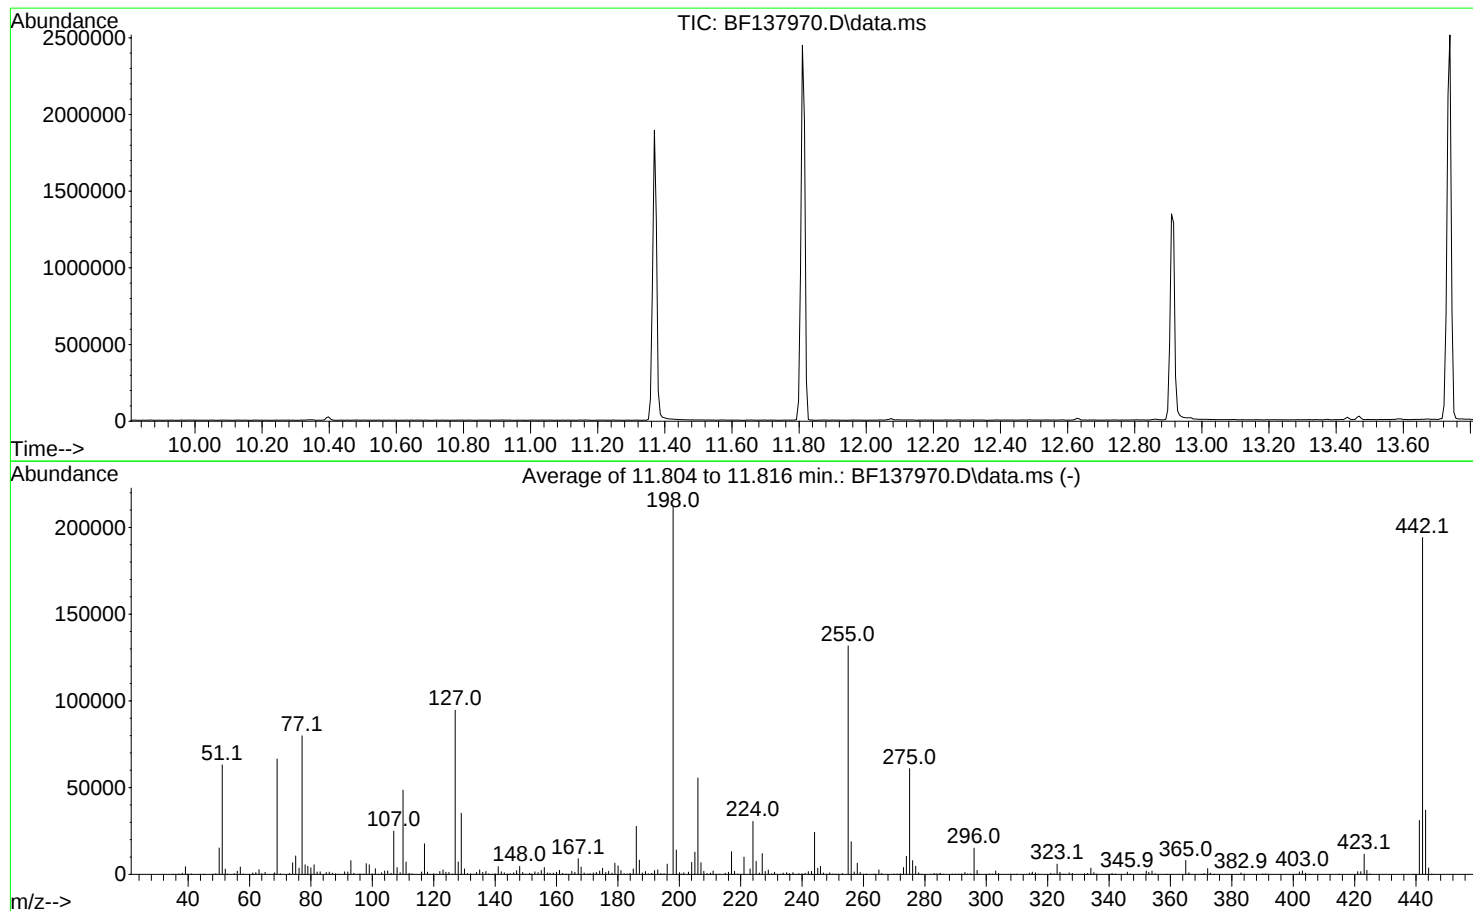

AutoFind: Scans 1652, 1653, 1654; Background Corrected with Scan 1647

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.7	63055	PASS
68	69	0.00	2	1.3	885	PASS
69	198	0.00	100	31.3	66475	PASS
70	69	0.00	2	0.5	363	PASS
127	198	10	80	44.6	94667	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	212051	PASS
199	198	5	9	6.6	14020	PASS
275	198	10	60	28.8	60976	PASS
365	198	1	100	3.8	7999	PASS
441	198	0.01	100	14.7	31102	PASS
442	442	50	100	100.0	194173	PASS
443	442	15	24	19.1	37038	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/21/2024	BNA_F	<u>BF137970.D</u>
Compound Name	Response	Retention Time
DDT	449939	13.739
DDD	6882	13.469
DDE	483	13.098
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7365	457304	1.61

Instrument :
BNA_F
ClientSampleId :
DFTPP

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052124\  
Data File : BF137970.D  
Acq On    : 21 May 2024  10:52  
Operator  : CG\JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 21 11:39:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF051424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 15 04:12:16 2024
Response via : Initial Calibration

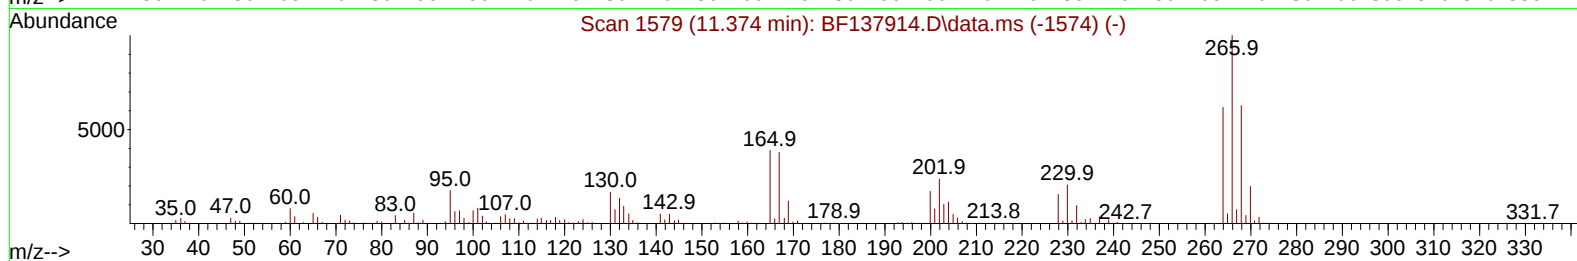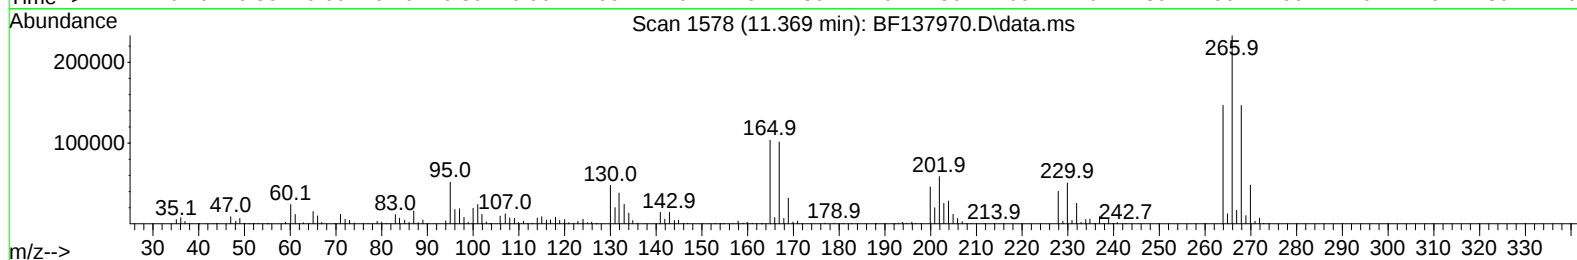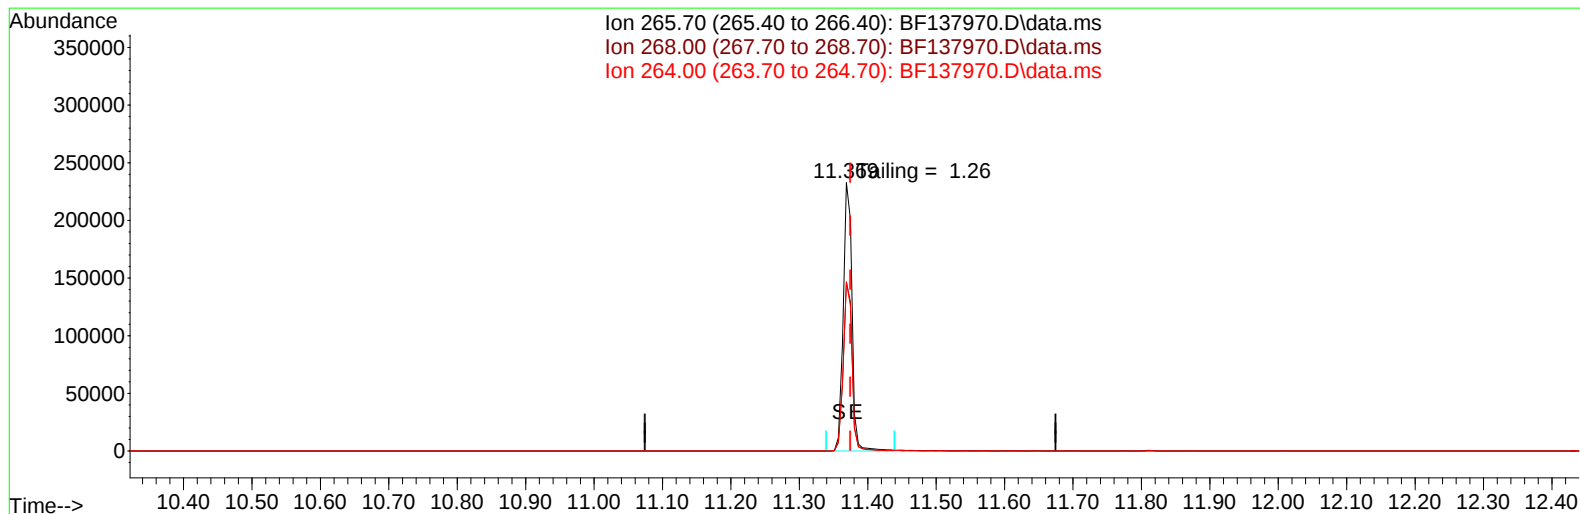

TIC: BF137970.D\data.ms

(70) Pentachlorophenol (C)

11.369min (-0.006) 344749.28 ng

response **208010**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	62.96
264.00	61.80	63.05
0.00	0.00	0.00

