
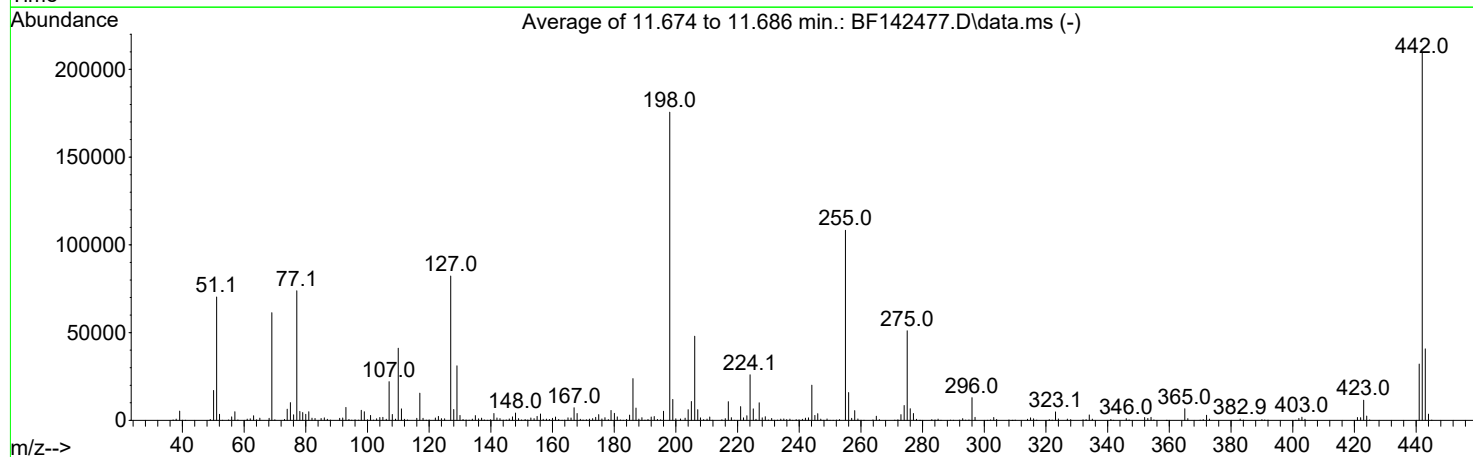


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052125\
Data File : BF142477.D
Acq On : 21 May 2025 09:41
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052025.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue May 20 16:26:47 2025

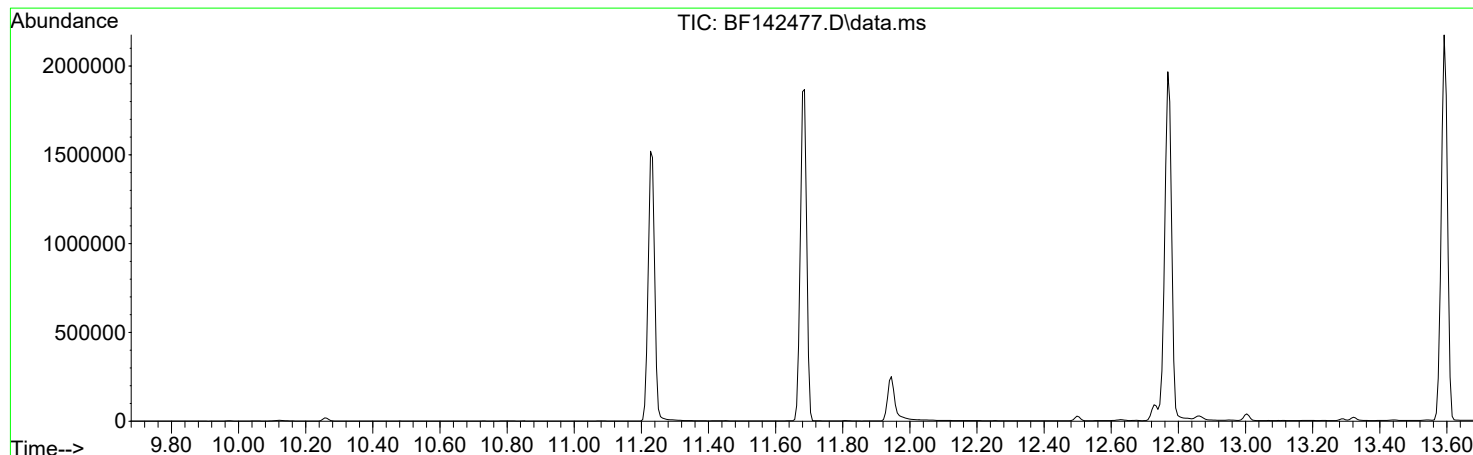

AutoFind: Scans 1612, 1613, 1614; Background Corrected with Scan 1606

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.0	70269	PASS
68	69	0.00	2	2.0	1206	PASS
69	198	0.00	100	34.9	61363	PASS
70	69	0.00	2	0.7	407	PASS
127	198	10	80	46.9	82288	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	175605	PASS
199	198	5	9	6.8	11940	PASS
275	198	10	60	29.1	51059	PASS
365	198	1	100	3.8	6708	PASS
441	198	0.01	100	18.3	32112	PASS
442	442	50	100	100.0	209616	PASS
443	442	15	24	19.4	40765	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/21/2025	BNA_F	<u>BF142477.D</u>
Compound Name	Response	Retention Time
DDT	567831	13.592
DDD	8926	13.321
DDE	878	12.957
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9804	577635	1.70

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052125\
Data File : BF142477.D
Acq On : 21 May 2025 09:41
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 21 11:31:19 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 20 16:26:47 2025
Response via : Initial Calibration

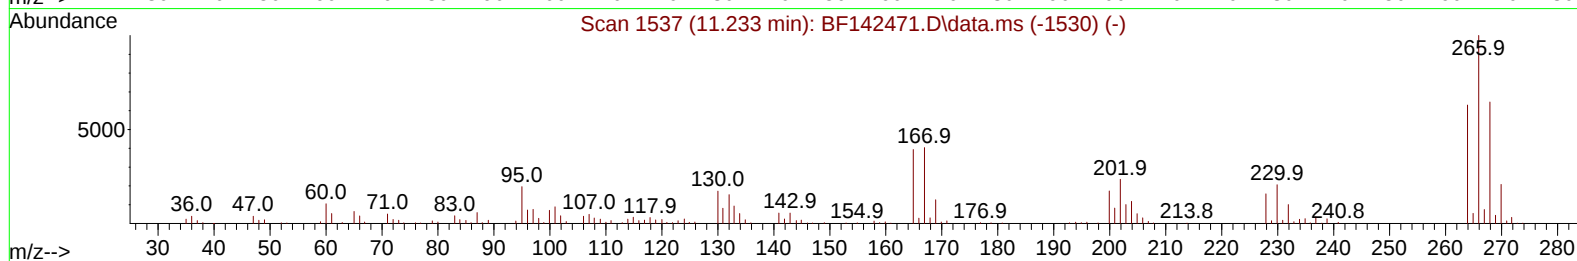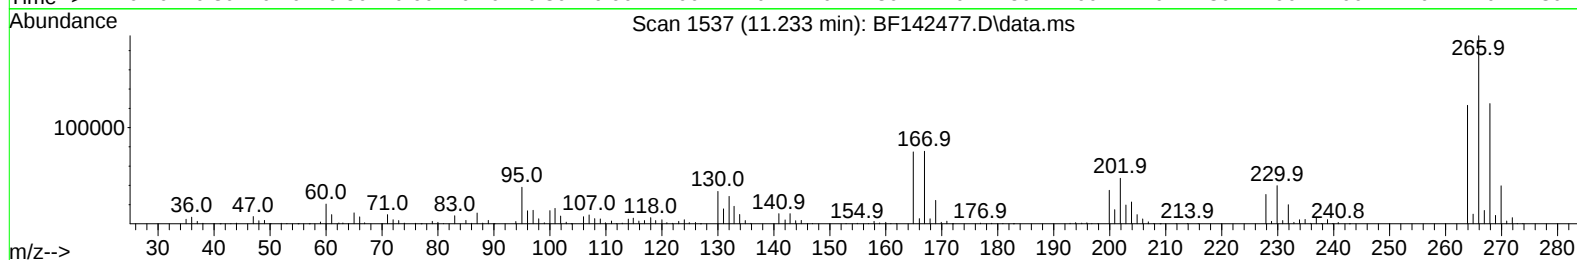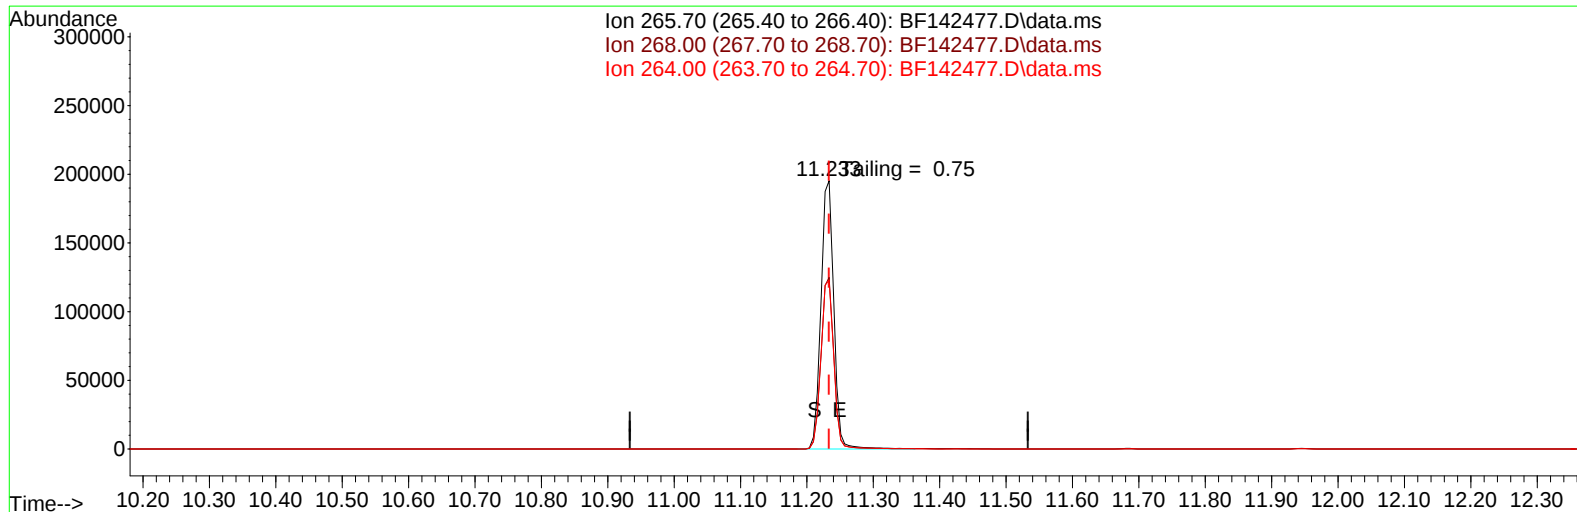

TIC: BF142477.D\data.ms

(70) Pentachlorophenol (C)

11.233min (+ 0.000) 40990.32 ng




response 263008

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.60	63.94
264.00	63.00	63.00
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052125\  
Data File : BF142477.D  
Acq On    : 21 May 2025  09:41  
Operator  : RC/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 21 11:31:19 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 20 16:26:47 2025
Response via : Initial Calibration

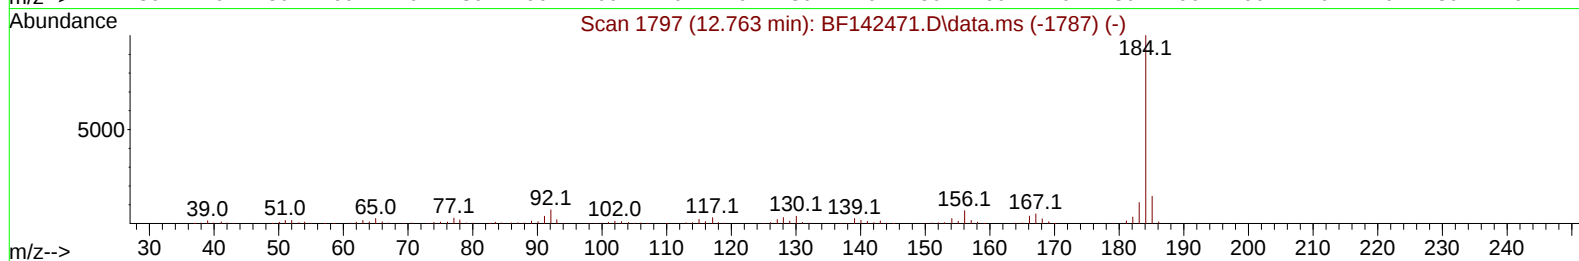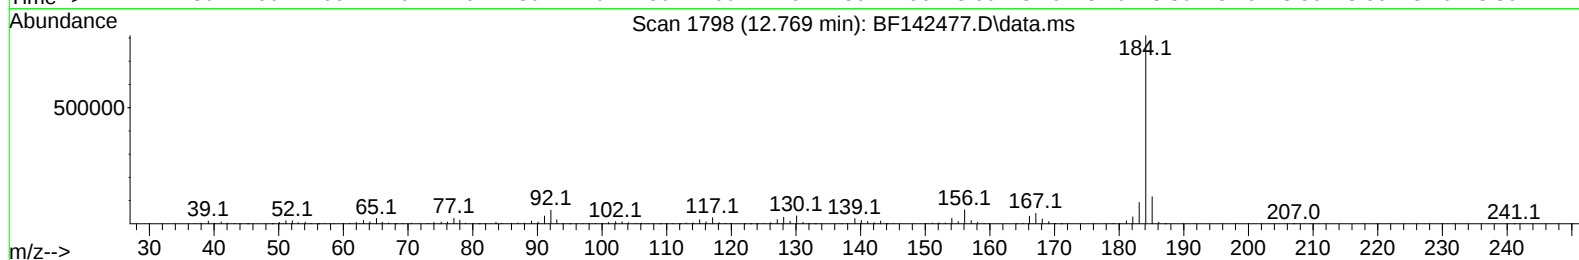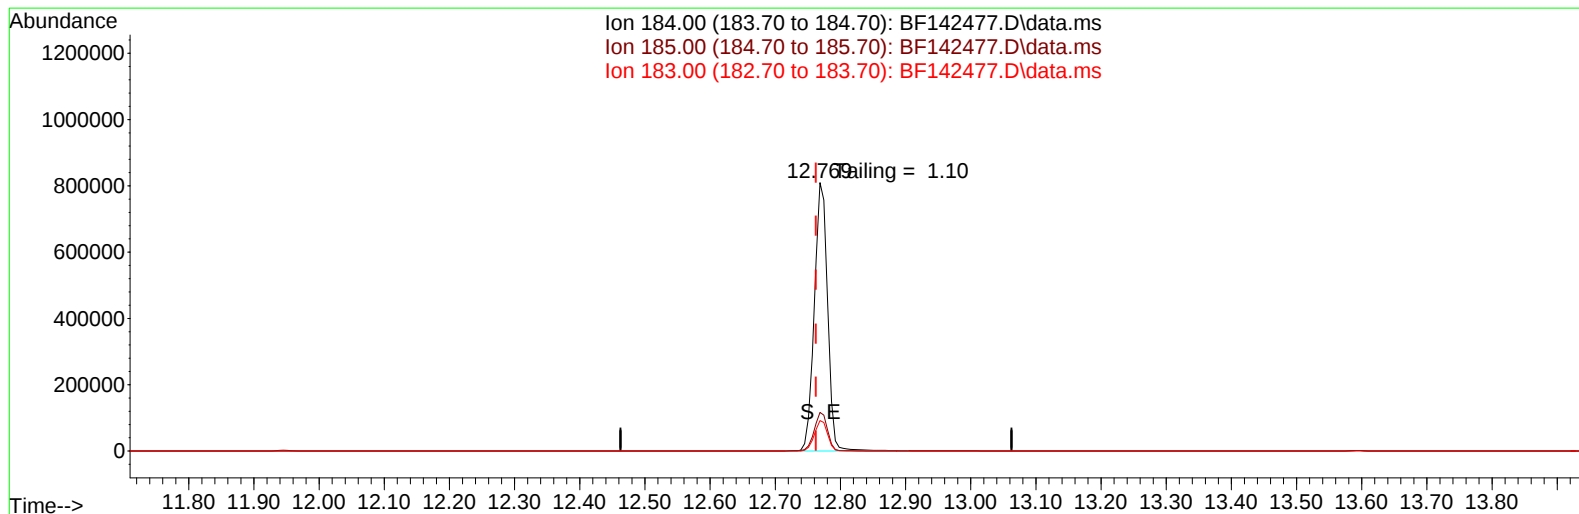

TIC: BF142477.D\data.ms

(77) Benzidine

12.769min (+ 0.006) 6765.19 ng

response **1148498**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.39
183.00	11.20	11.34
0.00	0.00	0.00