


Data Path : Z:\HPCHEM1\BNA_F\Data\BF052215\
Data File : BF079430.D
Acq On : 22 May 2015 12:28
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed May 20 05:08:22 2015

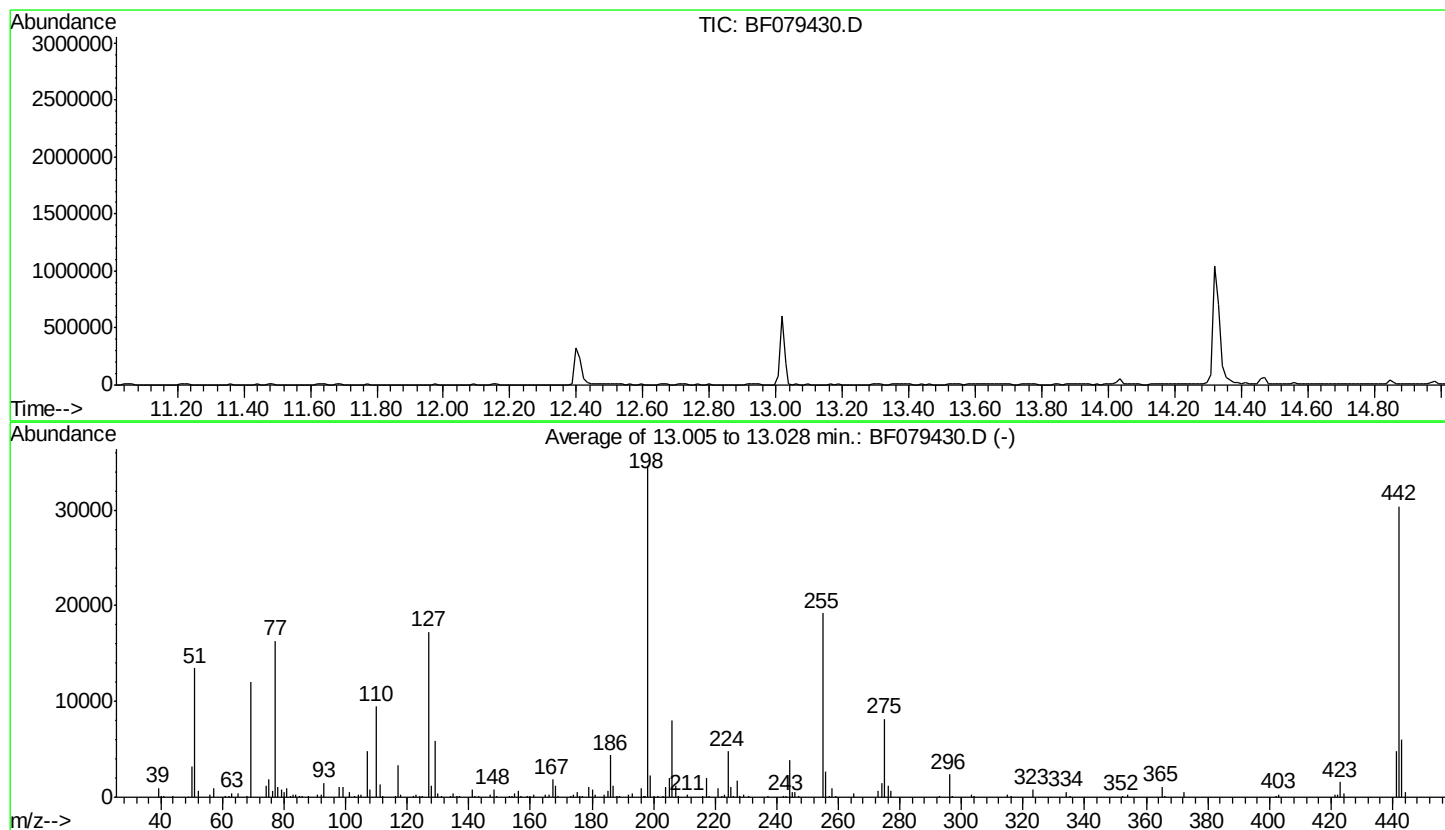

AutoFind: Scans 1034, 1035, 1036; Background Corrected with Scan 1031

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.9	13480	PASS
68	69	0.00	2	1.3	160	PASS
69	198	0.00	100	34.9	12095	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.8	17255	PASS
197	198	0.00	2	0.4	134	PASS
198	198	100	100	100.0	34632	PASS
199	198	5	9	6.6	2302	PASS
275	198	10	60	23.6	8159	PASS
365	198	1	100	3.1	1084	PASS
441	442	0.01	24	15.8	4794	PASS
442	198	50	100	87.8	30401	PASS
443	442	15	24	19.6	5966	PASS