


Data Path : Z:\HPCHEM1\BNA_F\Data\BF052215\
 Data File : BF079453.D
 Acq On : 23 May 2015 2:45
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat May 23 06:12:59 2015

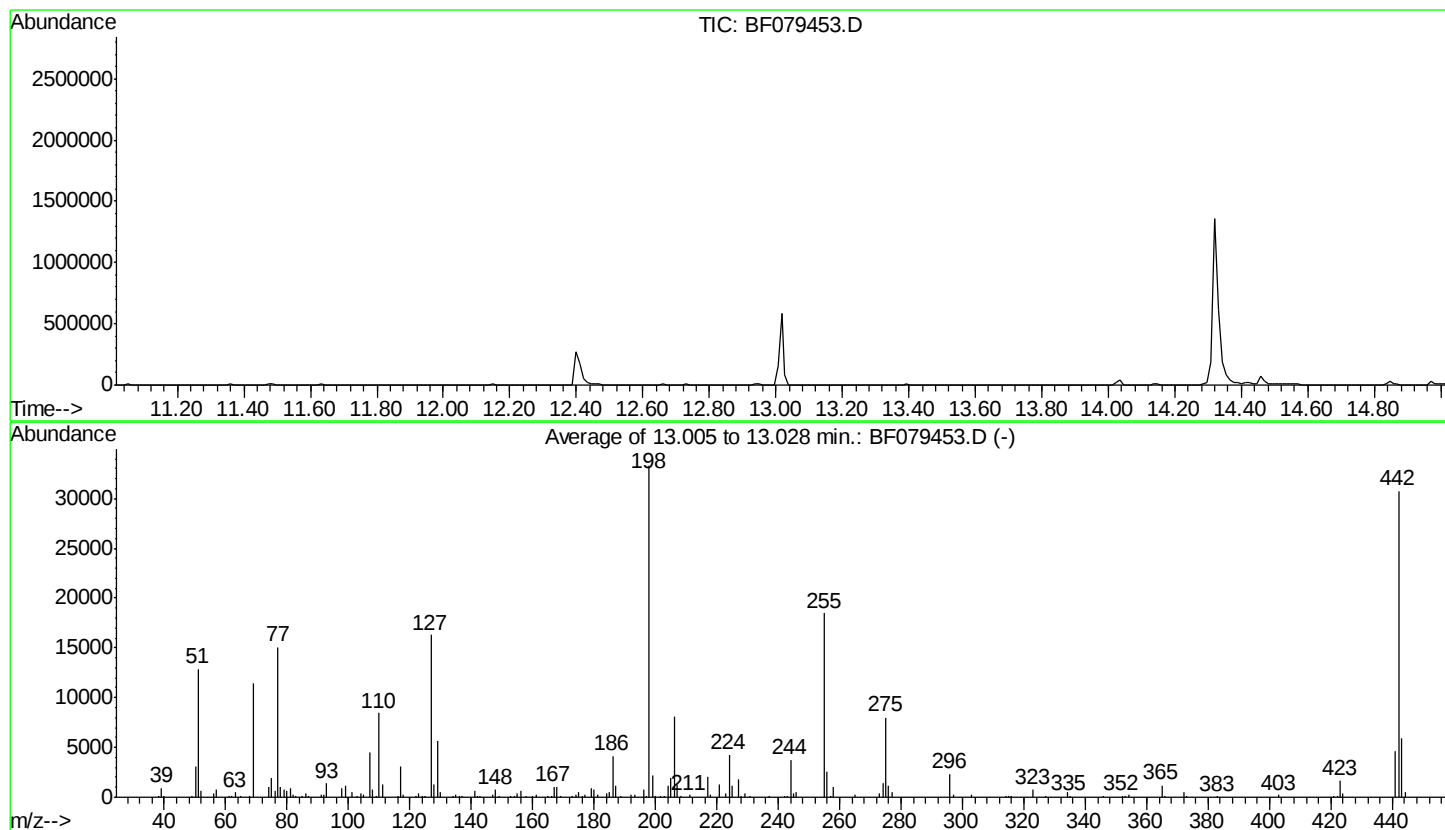

AutoFind: Scans 1034, 1035, 1036; Background Corrected with Scan 1031

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.6	12859	PASS
68	69	0.00	2	1.2	136	PASS
69	198	0.00	100	34.5	11497	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.9	16300	PASS
197	198	0.00	2	0.5	155	PASS
198	198	100	100	100.0	33308	PASS
199	198	5	9	6.6	2199	PASS
275	198	10	60	24.0	8000	PASS
365	198	1	100	3.6	1208	PASS
441	442	0.01	24	14.9	4593	PASS
442	198	50	100	92.3	30730	PASS
443	442	15	24	19.1	5862	PASS