
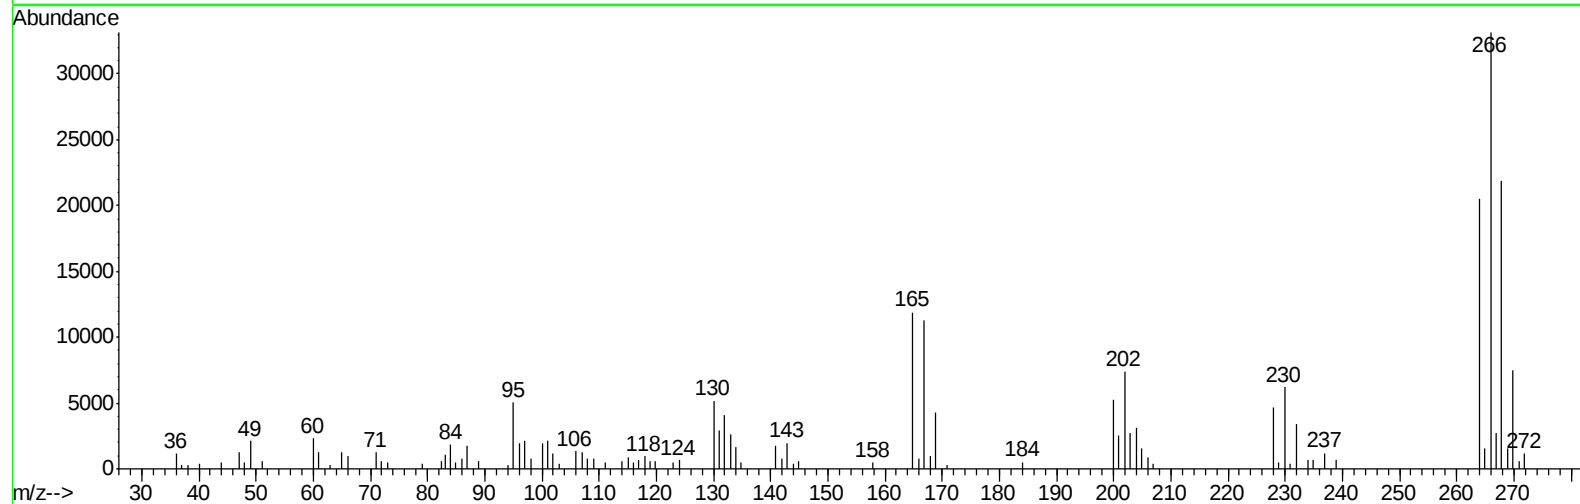


Data Path : Z:\HPCHEM1\BNA_F\Data\BF052215\
Data File : BF079430.D
Acq On : 22 May 2015 12:28
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 26 01:24:11 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 20 05:08:22 2015
Response via : Initial Calibration

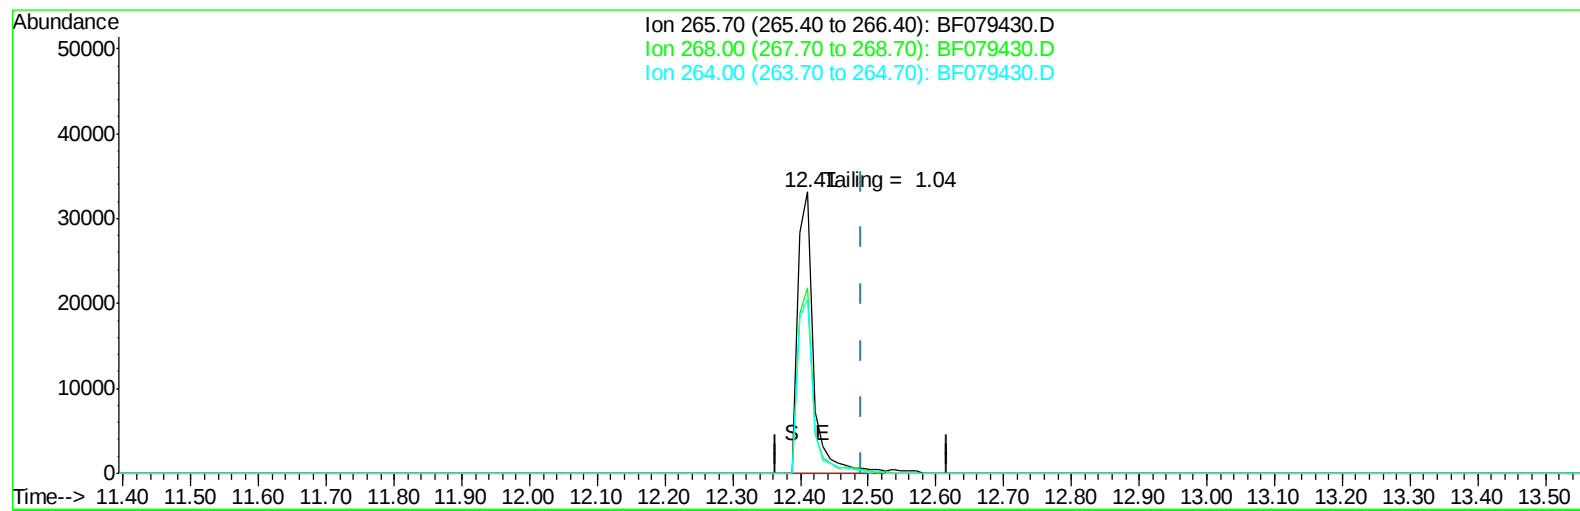

TIC: BF079430.D

(69) Pentachlorophenol (C)



12.411min (-0.080) 9925.53ng

response 54357

Ion	Exp%	Act%
265.70	100	100
268.00	68.80	66.07
264.00	63.60	61.99
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF052215\
Data File : BF079430.D
Acq On : 22 May 2015 12:28
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 26 01:24:11 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 20 05:08:22 2015
Response via : Initial Calibration

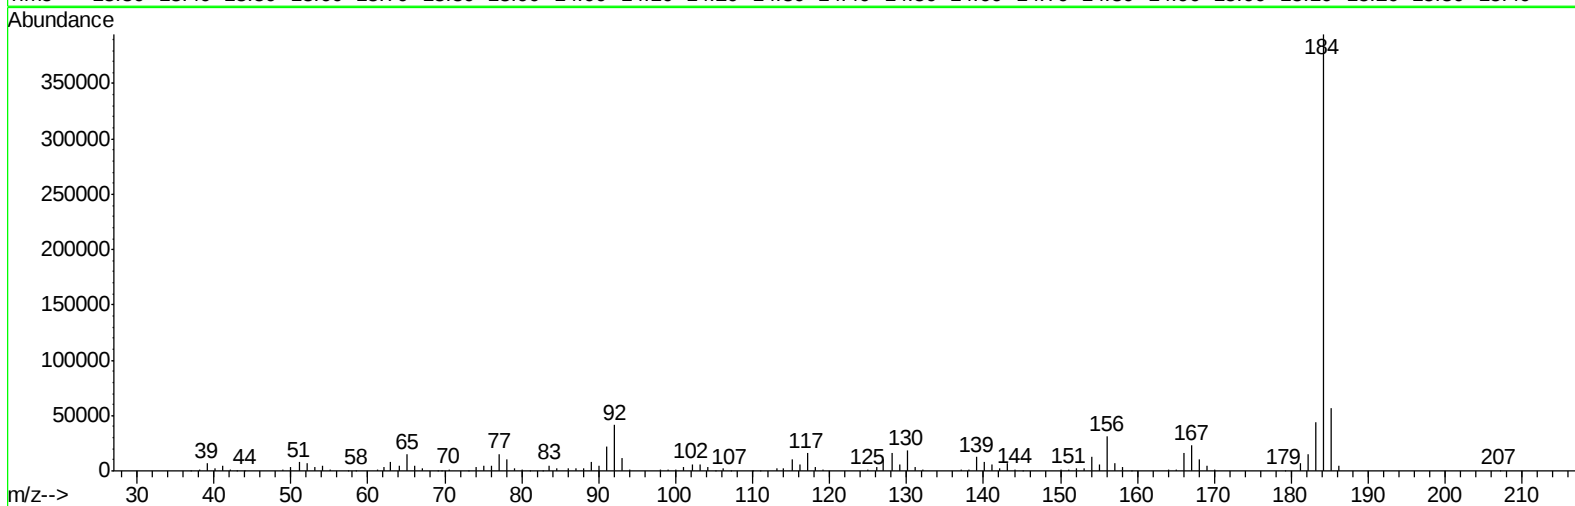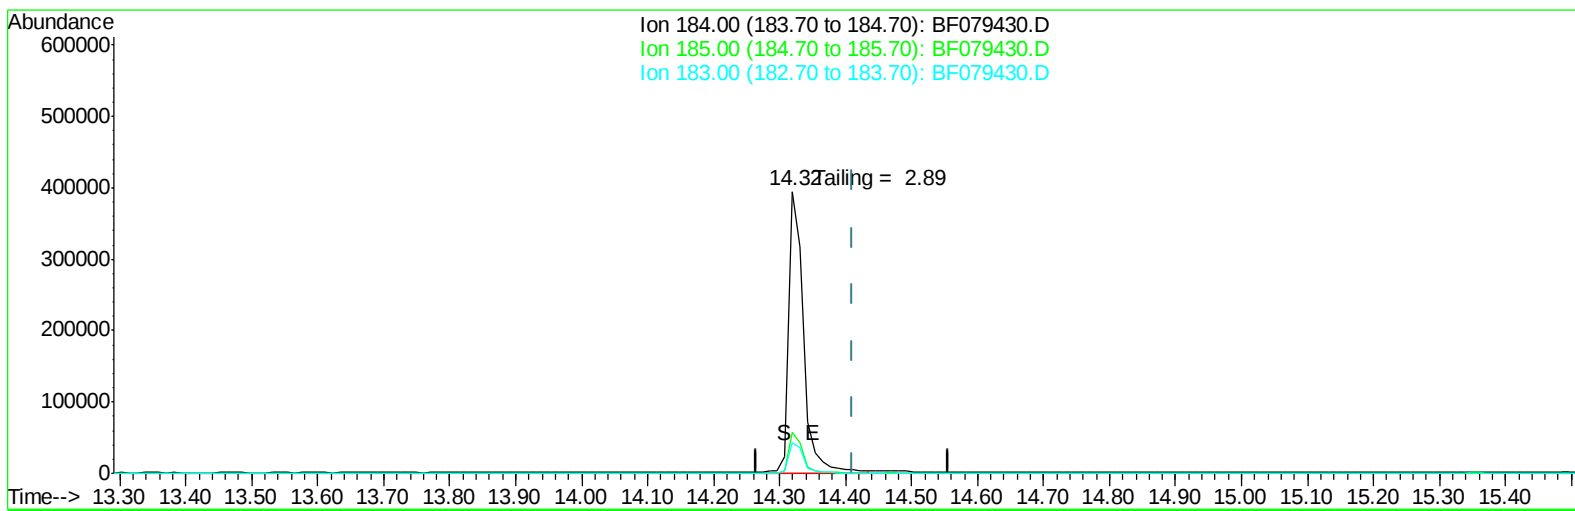

TIC: BF079430.D

(76) Benzidine

14.320min (-0.091) 0.00ng

response 591838

Ion	Exp%	Act%
184.00	100	100
185.00	16.00	14.39
183.00	11.20	11.05
0.00	0.00	0.00