
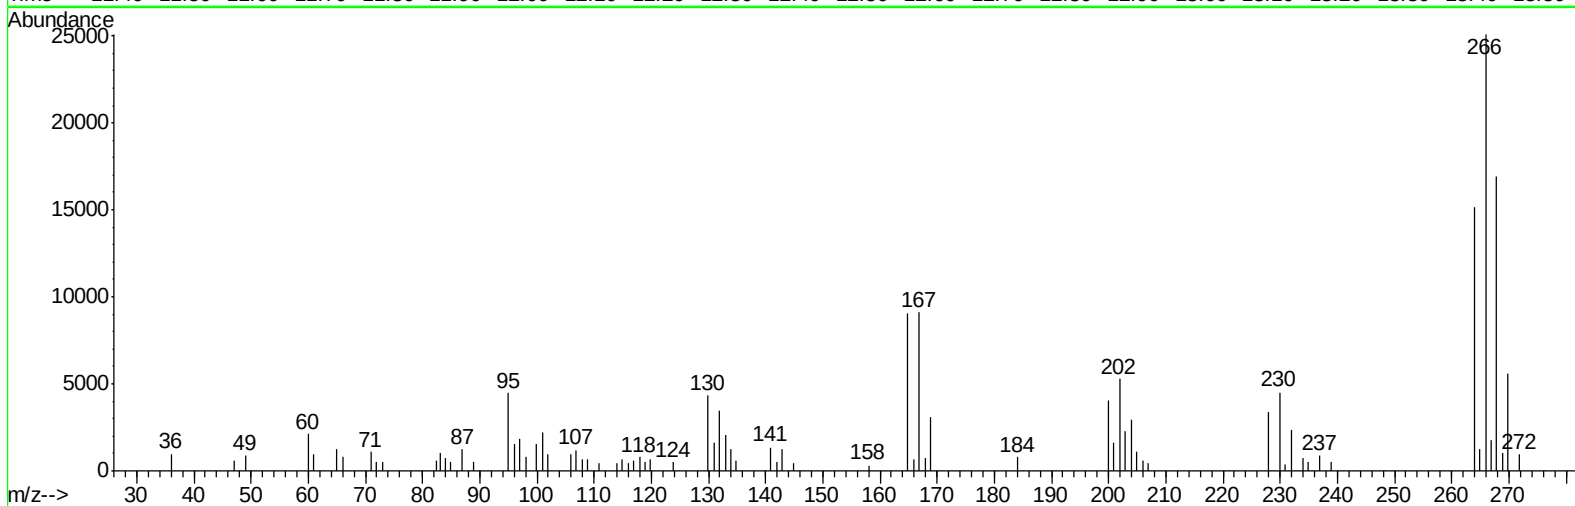


Data Path : Z:\HPCHEM1\BNA_F\Data\BF052215\
Data File : BF079453.D
Acq On : 23 May 2015 2:45
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 26 01:28:48 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 20 05:08:22 2015
Response via : Initial Calibration

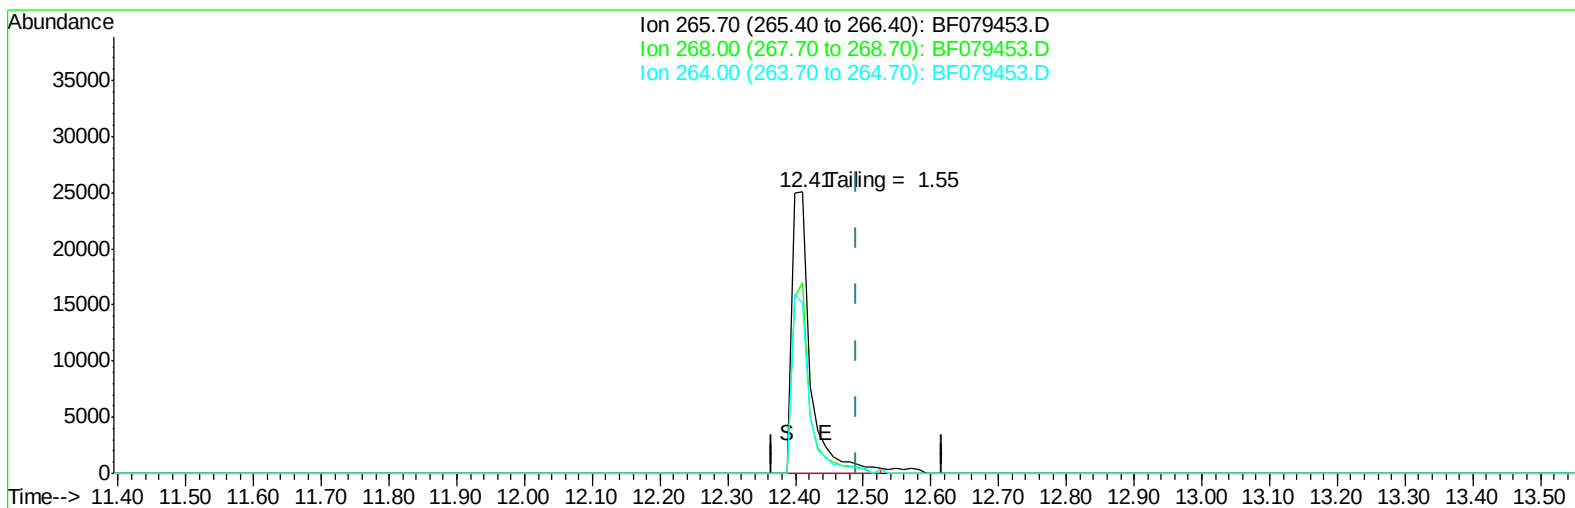

TIC: BF079453.D

(69) Pentachlorophenol (C)



12.411min (-0.080) 16983.96ng

response 48784

Ion	Exp%	Act%
265.70	100	100
268.00	68.80	67.56
264.00	63.60	60.46
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF052215\
Data File : BF079453.D
Acq On : 23 May 2015 2:45
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 26 01:28:48 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 20 05:08:22 2015
Response via : Initial Calibration

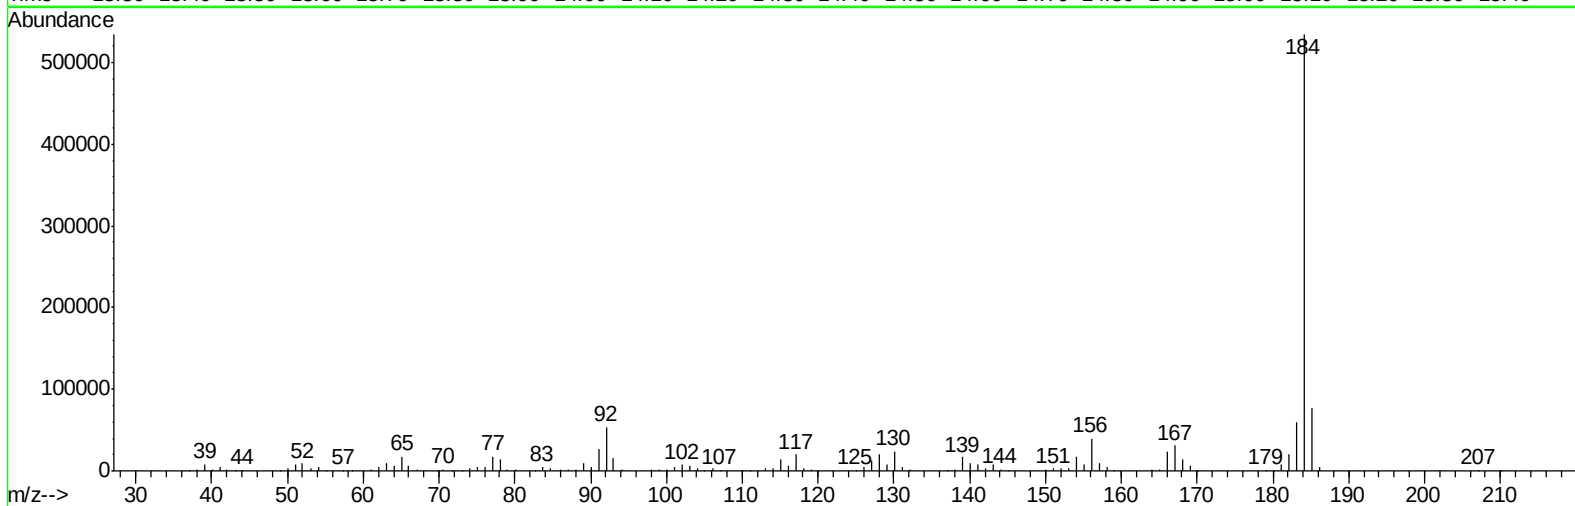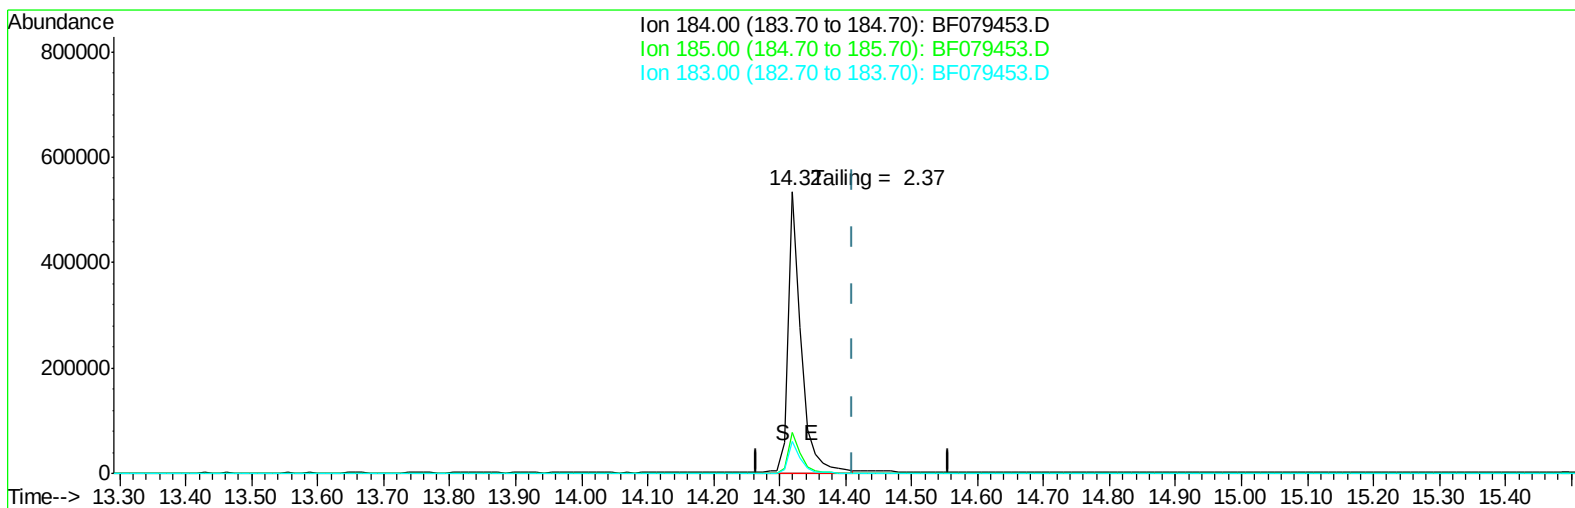

TIC: BF079453.D

(76) Benzidine

14.319min (-0.091) 0.00ng

response 695956

Ion	Exp%	Act%
184.00	100	100
185.00	16.00	14.37
183.00	11.20	11.30
0.00	0.00	0.00