

Data Path : Z:\HPCHEM1\BNA F\DATA\BF052216\
 Data File : BF087292.D
 Acq On : 22 May 2016 15:50
 Operator : UM/SJ
 Sample : H3172-08
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MW-14

Quant Time: May 23 04:23:14 2016
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF051716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon May 23 03:47:59 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.56	152	117784	20.00	ng	0.00
21) Naphthalene-d8	7.85	136	490958	20.00	ng	0.00
38) Acenaphthene-d10	9.59	164	232844	20.00	ng	-0.01
63) Phenanthrene-d10	11.06	188	379197	20.00	ng	-0.01
75) Chrysene-d12	13.69	240	260610	20.00	ng	-0.01
86) Perylene-d12	15.05	264	217695	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.14	112	563991	80.48	ng	0.00
7) Phenol-d6	6.23	99	503484	53.57	ng	-0.01
23) Nitrobenzene-d5	7.14	82	1050985	106.69	ng	0.00
41) 2,4,6-Tribromophenol	10.39	330	360579	140.14	ng	0.00
44) 2-Fluorobiphenyl	8.92	172	1501098	106.77	ng	0.00
78) Terphenyl-d14	12.65	244	1159456	100.64	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF052216\
Data File : BF087292.D
Acq On : 22 May 2016 15:50
Operator : UM/SJ
Sample : H3172-08
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-14

Quant Time: May 23 04:23:14 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF051716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 23 03:47:59 2016
Response via : Initial Calibration

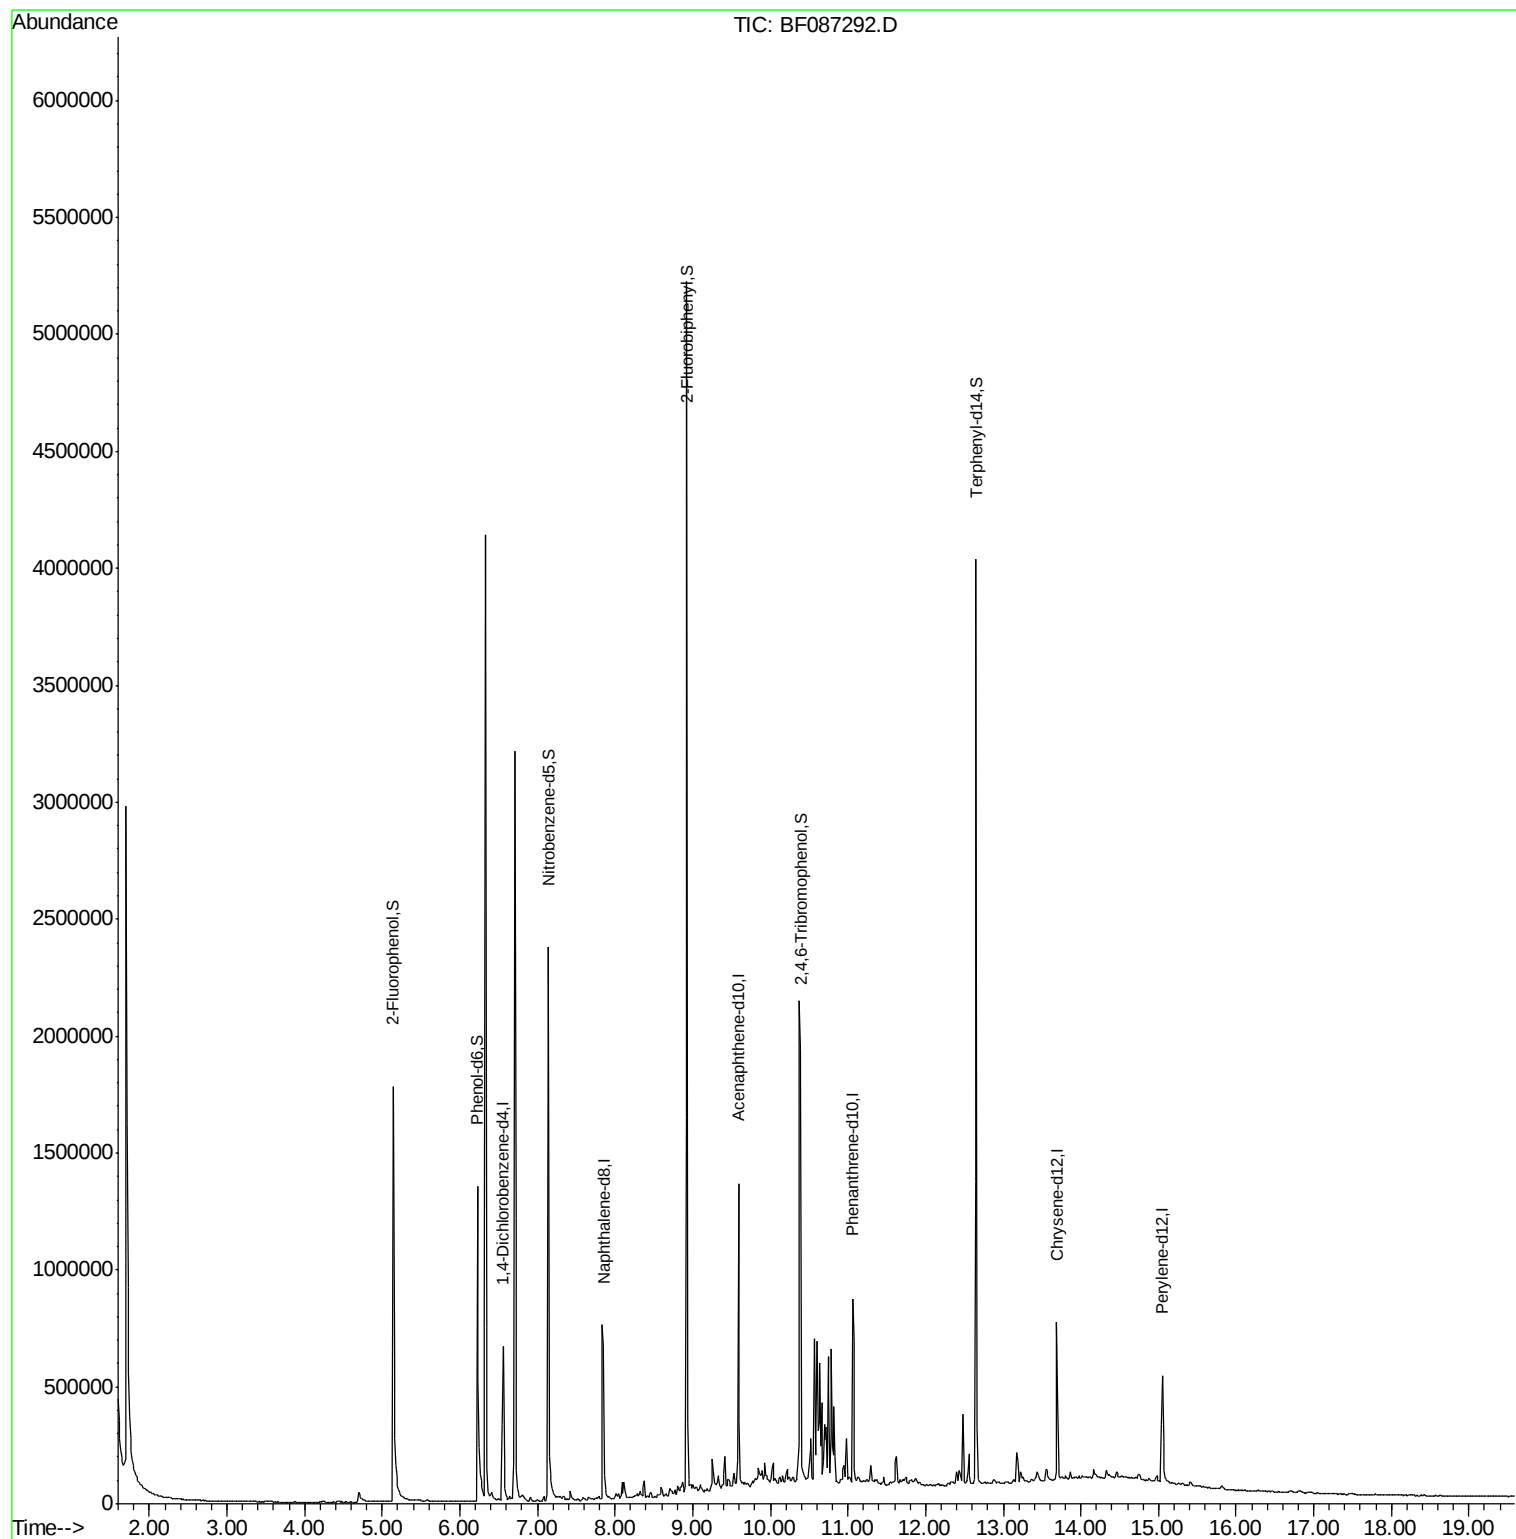

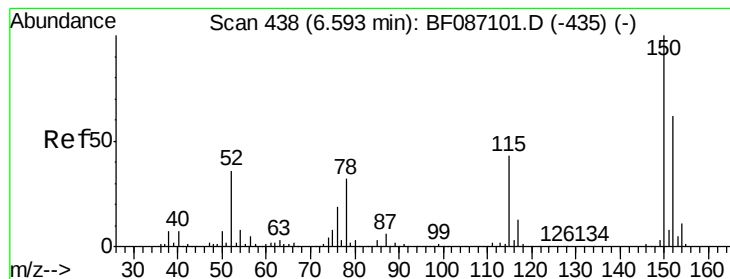

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.56 min Scan# 435

Delta R.T. 0.00 min

Lab File: BF087292.D

Acq: 22 May 2016 15:50

Instrument :

BNA_F

ClientSampleId :

MW-14


Tot Ion:152 Resp: 117784

Ion Ratio Lower Upper

152 100

150 153.0 125.8 188.6




115 60.5 51.5 77.3

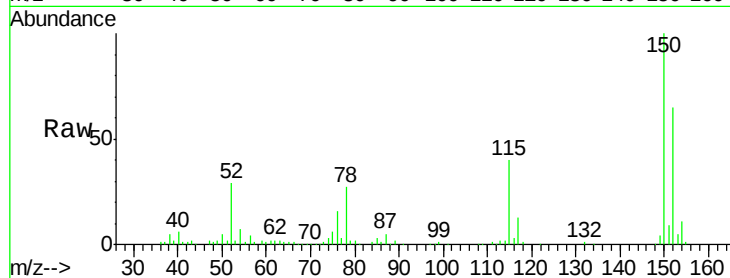

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

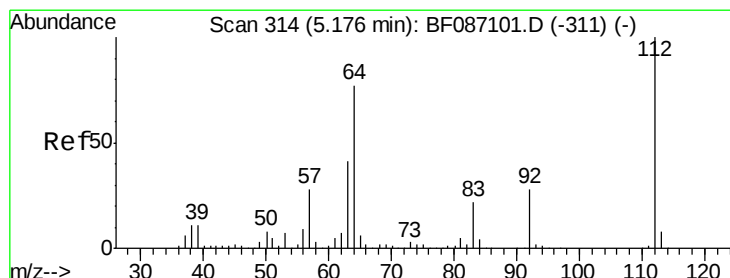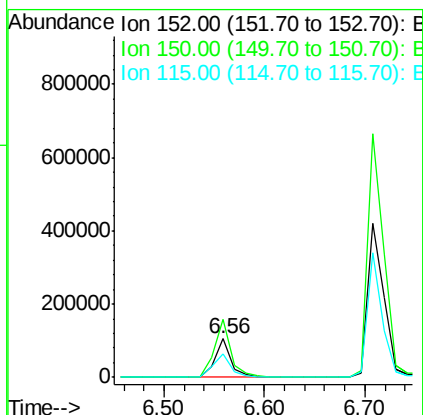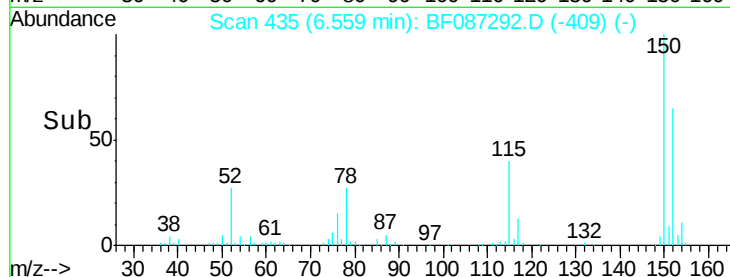

#5

2-Fluorophenol

Concen: 80.48 ng

RT: 5.14 min Scan# 311

Delta R.T. 0.00 min

Lab File: BF087292.D

Acq: 22 May 2016 15:50


Tgt Ion:112 Resp: 563991

Ion Ratio Lower Upper

112 100

64 71.1 52.1 78.1



63 39.5 25.7 38.5#

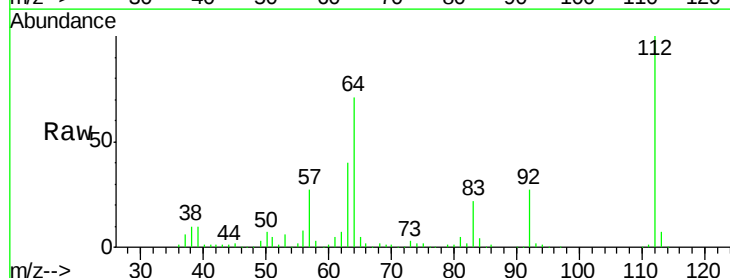

Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

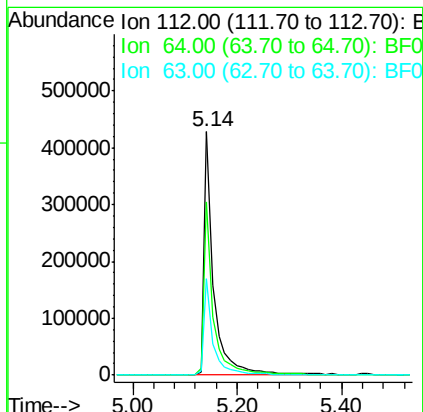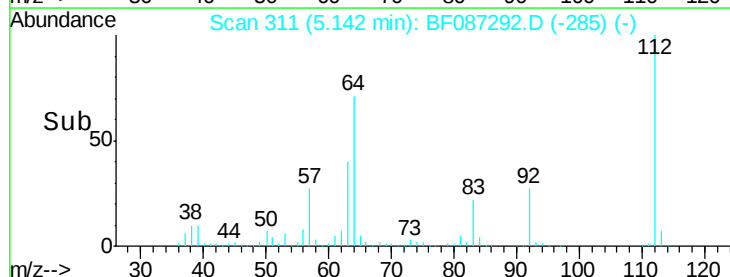



#7

Phenol-d6

Concen: 53.57 ng

RT: 6.23 min Scan# 406

Delta R.T. -0.01 min

Lab File: BF087292.D

Acq: 22 May 2016 15:50

Instrument :

BNA_F

ClientSampled :

MW-14





Tot Ion: 99 Resp: 503484

Ion Ratio Lower Upper

99 100

42 30.0 13.6 20.4#

71 39.8 24.6 36.8#

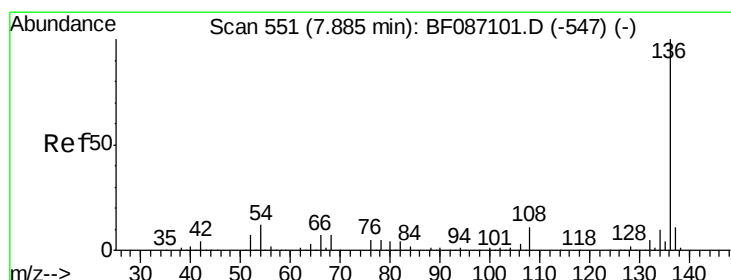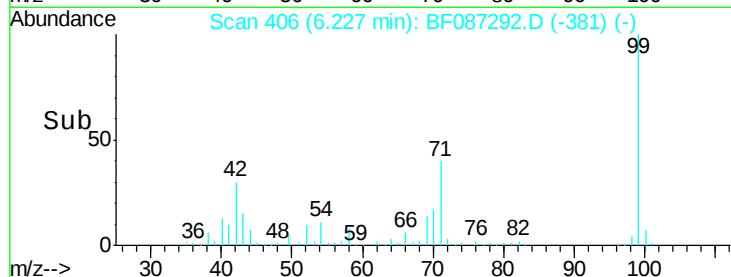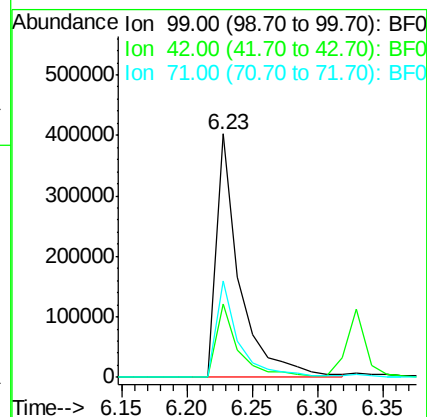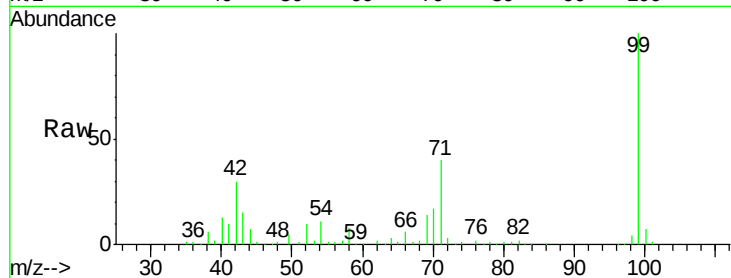

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 7.85 min Scan# 548

Delta R.T. 0.00 min

Lab File: BF087292.D

Acq: 22 May 2016 15:50

Tgt Ion: 136 Resp: 490958




Ion Ratio Lower Upper

136 100

137 10.4 8.8 13.2

54 8.6 5.0 7.4#

68 4.6 4.4 6.6

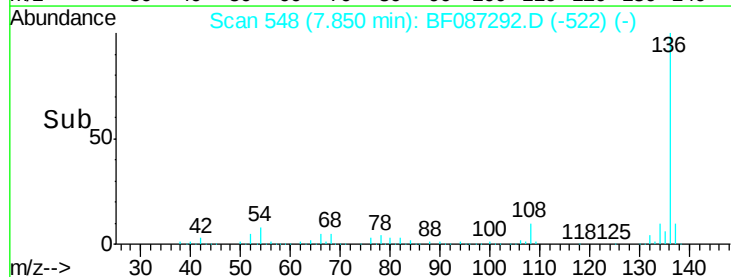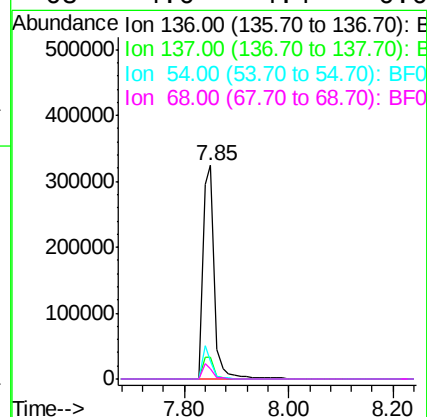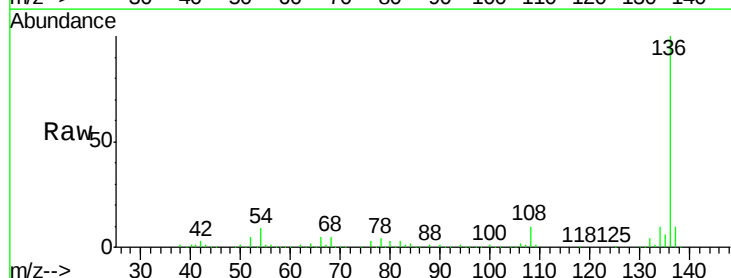







#23
 Nitrobenzene-d5
 Concen: 106.69 ng
 RT: 7.14 min Scan# 486
 Delta R.T. 0.00 min
 Lab File: BF087292.D
 Acq: 22 May 2016 15:50

Instrument :
 BNA_F
 ClientSampleId :
 MW-14

Tot Ion: 82 Resp: 1050985
 Ion Ratio Lower Upper
 82 100
 128 46.5 40.6 61.0
 54 61.6 38.1 57.1#

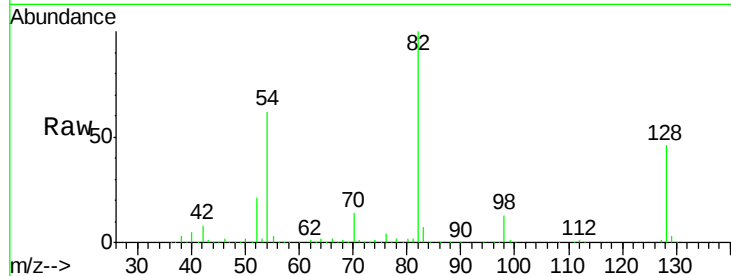


Abundance Ion 82.00 (81.70 to 82.70): BF0
 Ion 128.00 (127.70 to 128.70): E
 Ion 54.00 (53.70 to 54.70): BF0

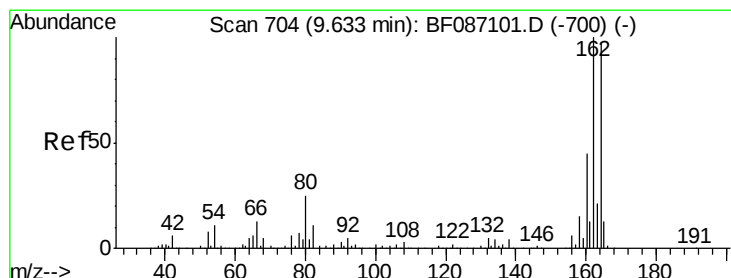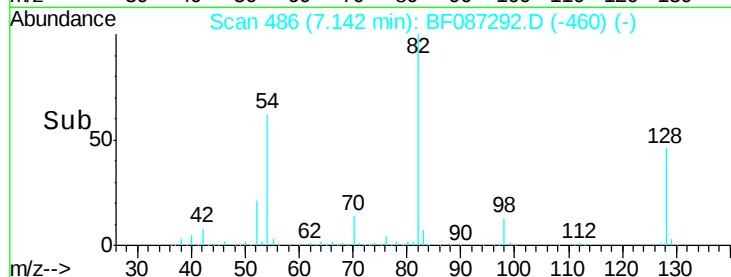
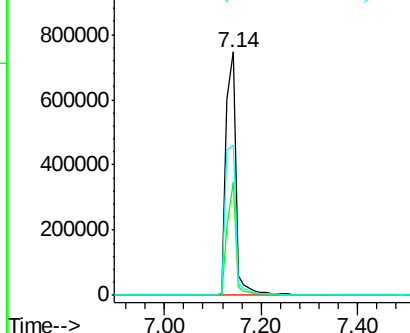


#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.59 min Scan# 700
 Delta R.T. -0.01 min
 Lab File: BF087292.D
 Acq: 22 May 2016 15:50

Tgt Ion: 164 Resp: 232844
 Ion Ratio Lower Upper
 164 100
 162 102.2 82.8 124.2
 160 46.2 36.9 55.3

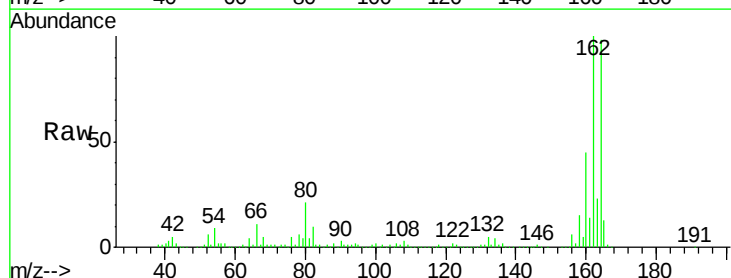

Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E



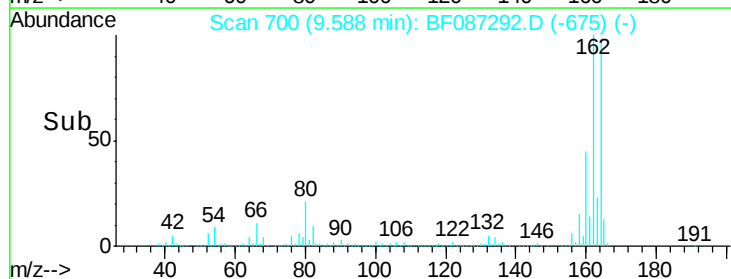
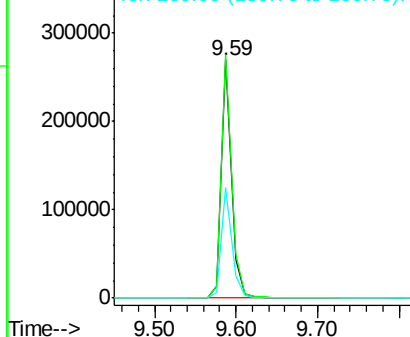




#41
 2,4,6-Tribromophenol
 Concen: 140.14 ng
 RT: 10.39 min Scan# 770
 Delta R.T. 0.00 min
 Lab File: BF087292.D
 Acq: 22 May 2016 15:50




Instrument :
 BNA_F
 ClientSampleId :
 MW-14


Tot Ion	Ratio	Lower	Upper
330	100		
332	96.6	79.0	118.4
141	34.8	31.2	46.8

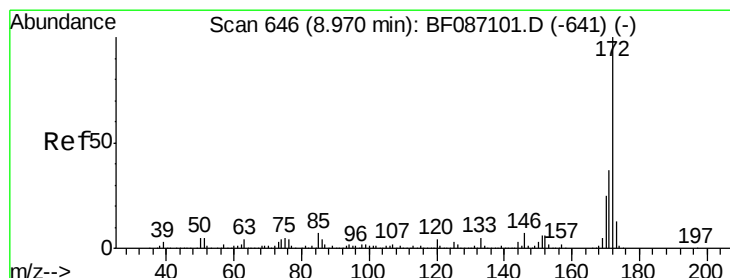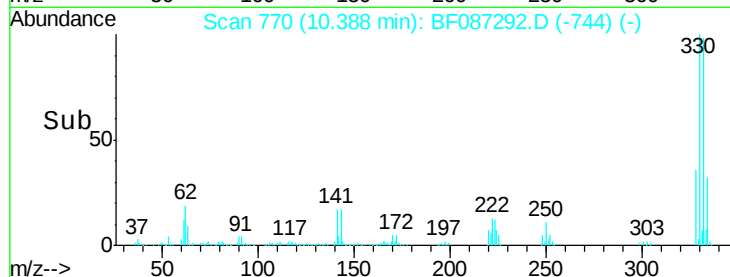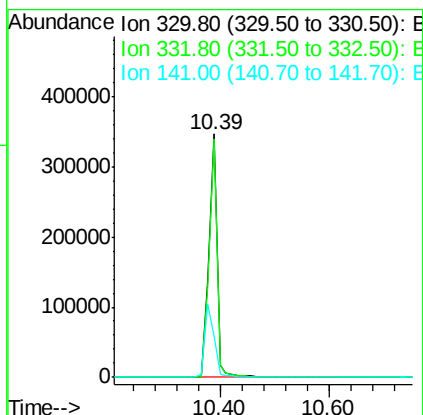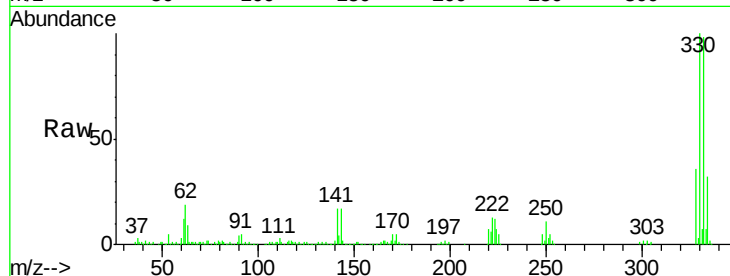

#44
 2-Fluorobiphenyl
 Concen: 106.77 ng
 RT: 8.92 min Scan# 642
 Delta R.T. 0.00 min
 Lab File: BF087292.D
 Acq: 22 May 2016 15:50

Tgt Ion	Ratio	Lower	Upper
172	100		
171	37.0	29.0	43.6
170	25.1	19.8	29.8

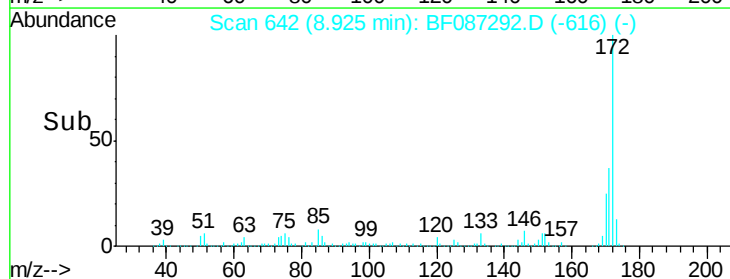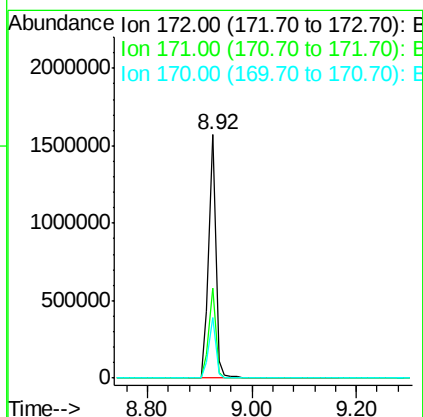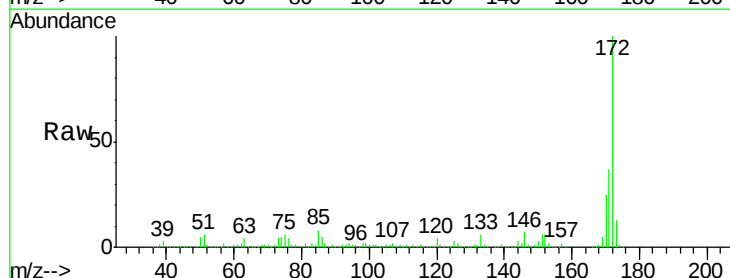


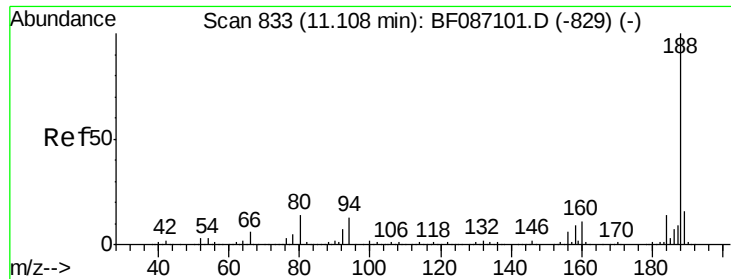




#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.06 min Scan# 829
Delta R.T. -0.01 min
Lab File: BF087292.D
Acq: 22 May 2016 15:50

Instrument :
BNA_F
ClientSampleId :
MW-14

Tot Ion:188 Resp: 379197
Ion Ratio Lower Upper
188 100
94 13.5 6.8 10.2#
80 15.1 7.1 10.7#

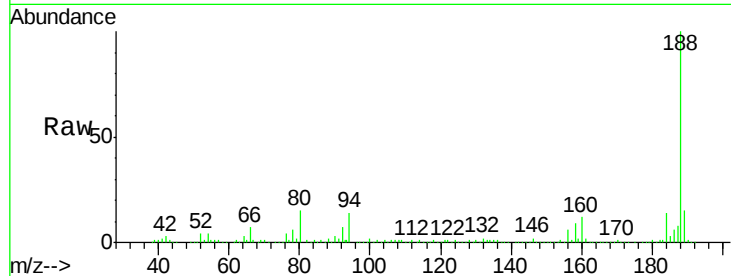


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

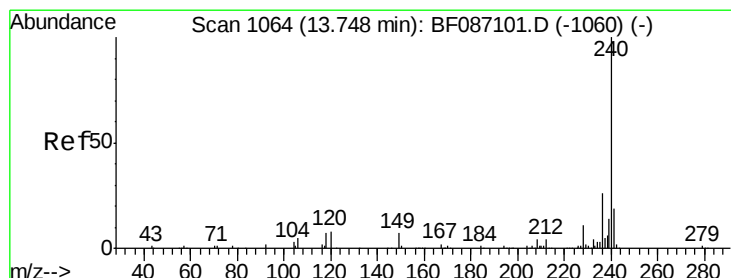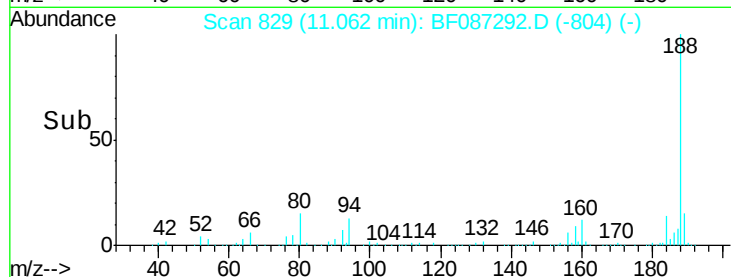
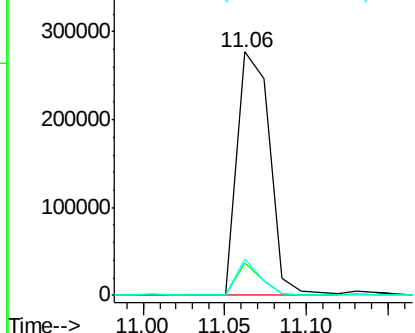



#75
Chrysene-d12
Concen: 20.00 ng
RT: 13.69 min Scan# 1059
Delta R.T. -0.01 min
Lab File: BF087292.D
Acq: 22 May 2016 15:50

Tgt Ion:240 Resp: 260610
Ion Ratio Lower Upper
240 100
120 14.2 11.2 16.8
236 26.5 21.2 31.8

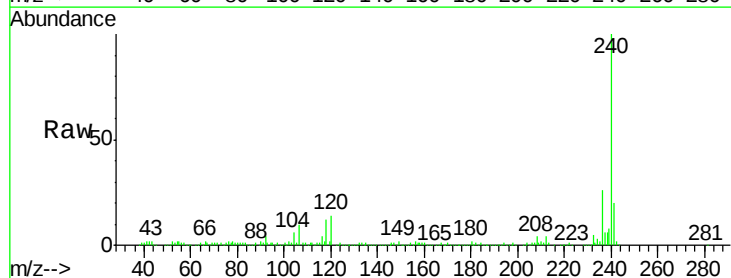

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E



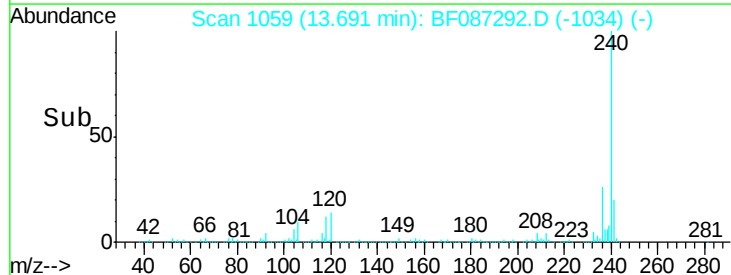
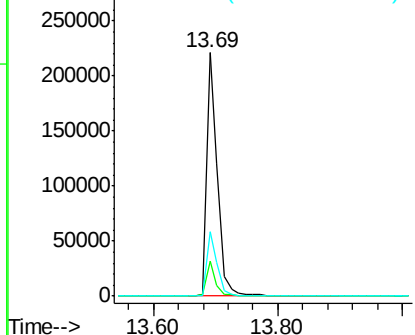


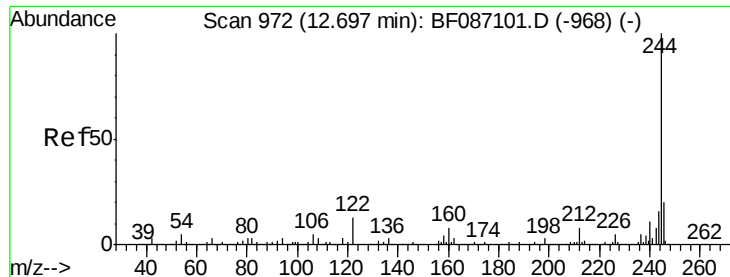

#78
 Terphenyl-d14
 Concen: 100.64 ng
 RT: 12.65 min Scan# 968
 Delta R.T. 0.00 min
 Lab File: BF087292.D
 Acq: 22 May 2016 15:50

Instrument :
 BNA_F
 ClientSampleId :
 MW-14

Tot Ion:244 Resp: 1159456
 Ion Ratio Lower Upper
 244 100
 212 7.9 6.2 9.2
 122 12.0 12.0 18.0#

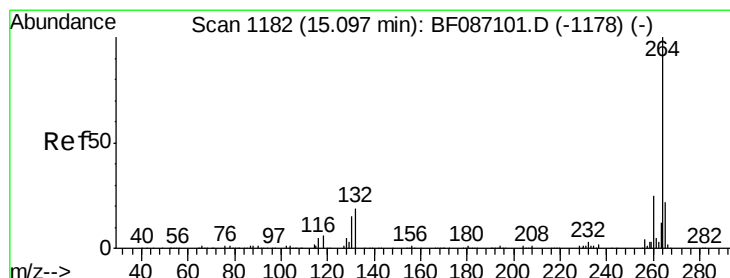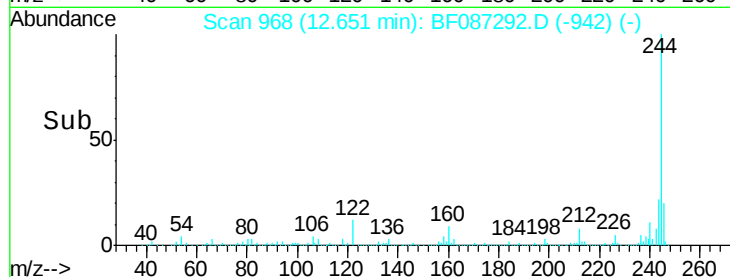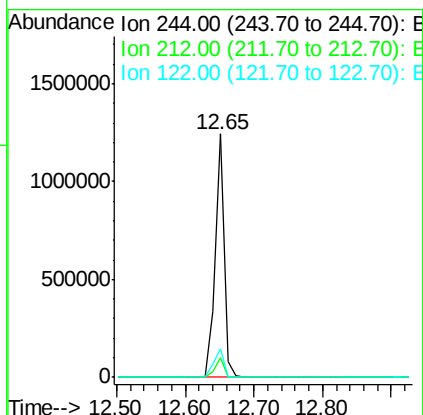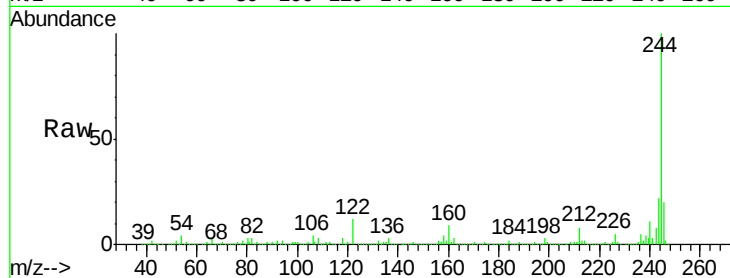

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 15.05 min Scan# 1178
 Delta R.T. 0.00 min
 Lab File: BF087292.D
 Acq: 22 May 2016 15:50

Tgt Ion:264 Resp: 217695
 Ion Ratio Lower Upper
 264 100
 260 23.9 19.5 29.3
 265 21.1 17.3 25.9

