


Data Path : Z:\HPCHEM1\BNA F\DATA\BF052216\
 Data File : BF087278.D
 Acq On : 22 May 2016 9:05
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF051716.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon May 23 13:51:43 2016

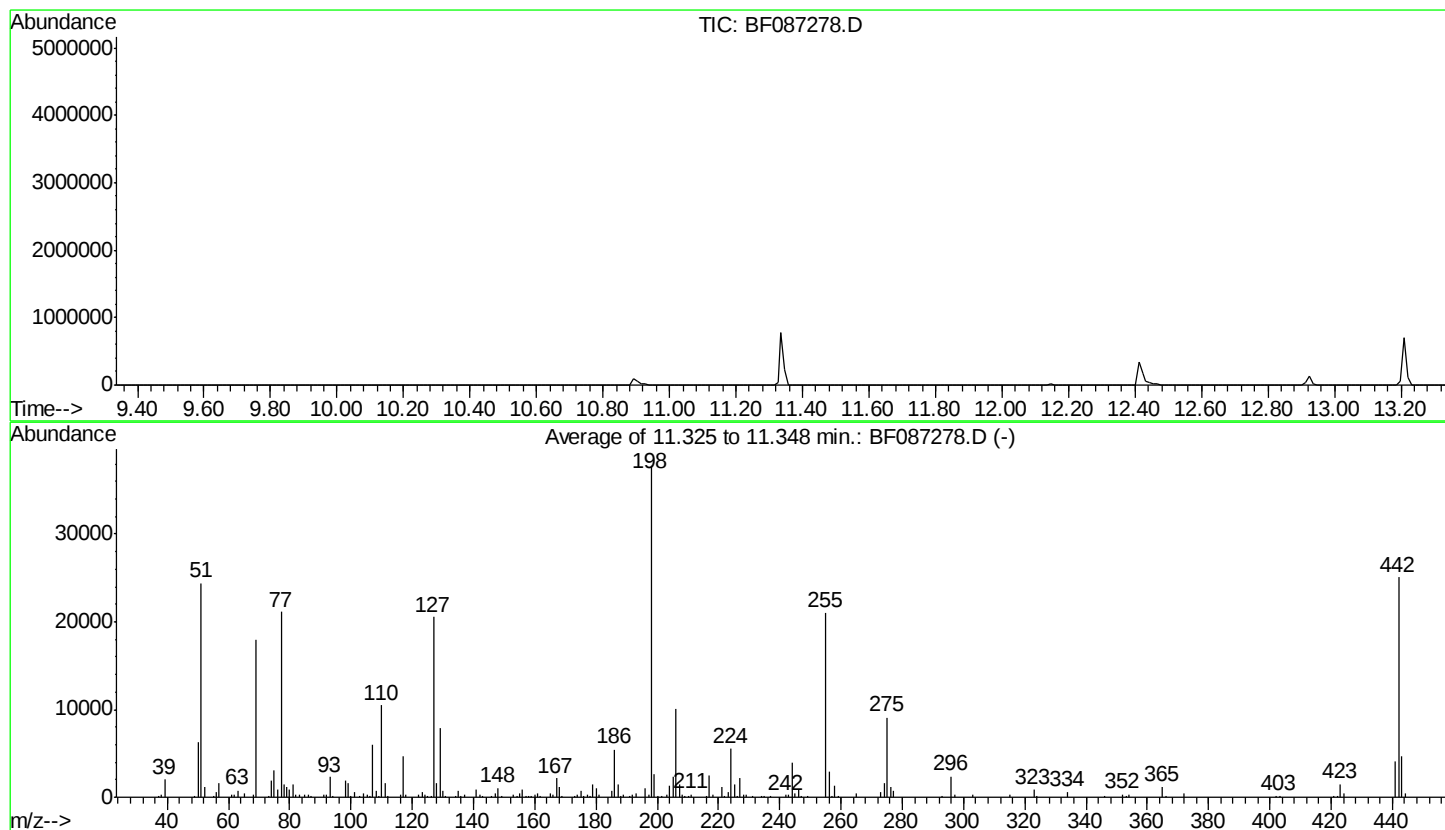

AutoFind: Scans 852, 853, 854; Background Corrected with Scan 849

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	64.6	24424	PASS
68	69	0.00	2	1.8	325	PASS
69	198	0.00	100	47.4	17901	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	54.4	20550	PASS
197	198	0.00	2	0.7	268	PASS
198	198	100	100	100.0	37801	PASS
199	198	5	9	7.1	2675	PASS
275	198	10	60	23.9	9049	PASS
365	198	1	100	3.2	1222	PASS
441	442	0.01	24	16.1	4045	PASS
442	198	50	100	66.3	25048	PASS
443	442	15	24	18.4	4609	PASS