


Data Path : Z:\HPCHEM1\BNA F\DATA\BF052217\
Data File : BF095307.D
Acq On : 22 May 2017 10:58
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 23 18:02:00 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 18 17:07:53 2017
Response via : Initial Calibration

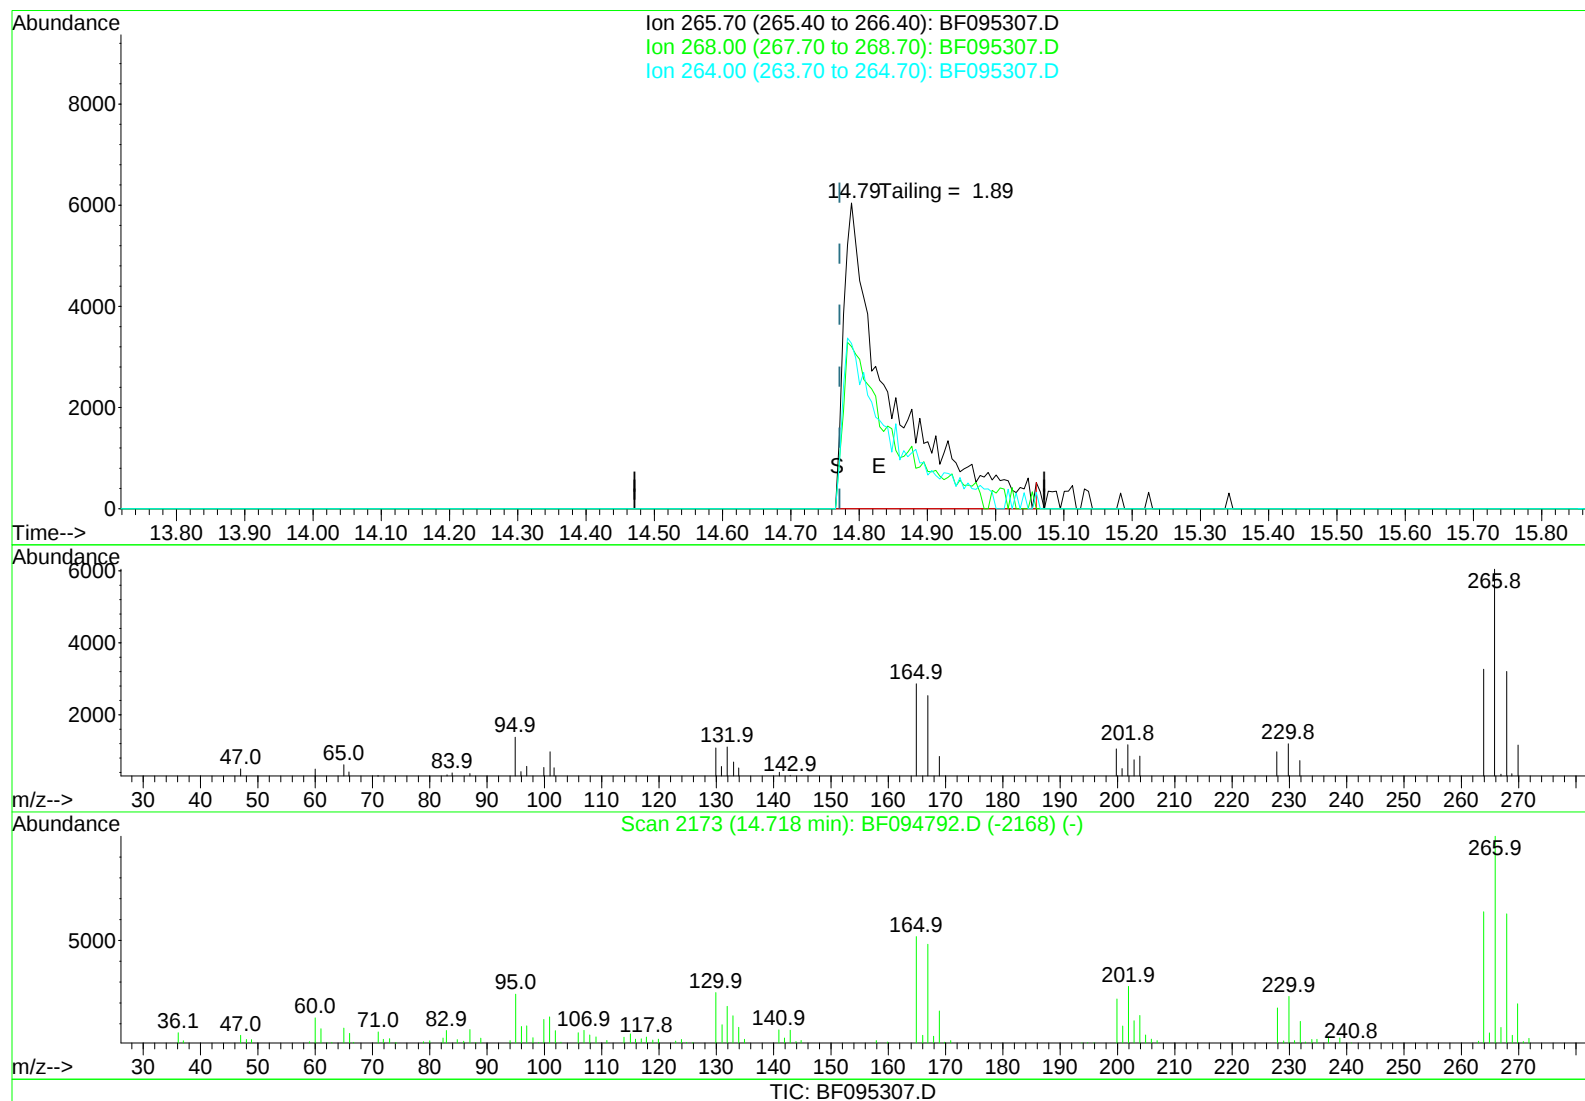

(69) Pentachlorophenol (C)




14.789min (+0.018) 0.00ng m

response 29239

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	53.02
264.00	64.60	54.01
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF052217\
Data File : BF095307.D
Acq On : 22 May 2017 10:58
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 23 18:02:00 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 18 17:07:53 2017
Response via : Initial Calibration

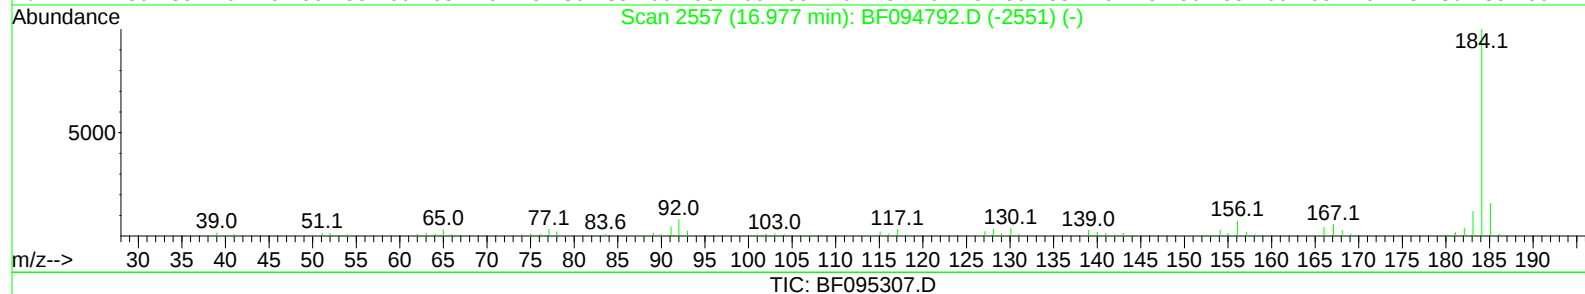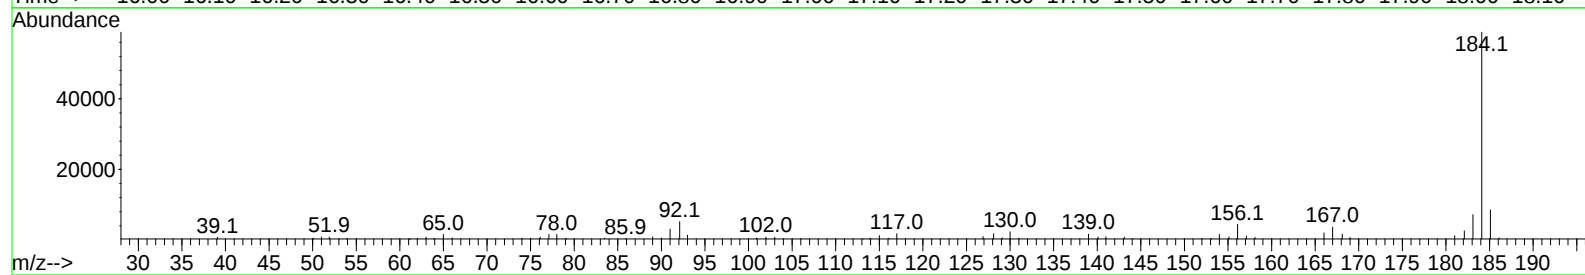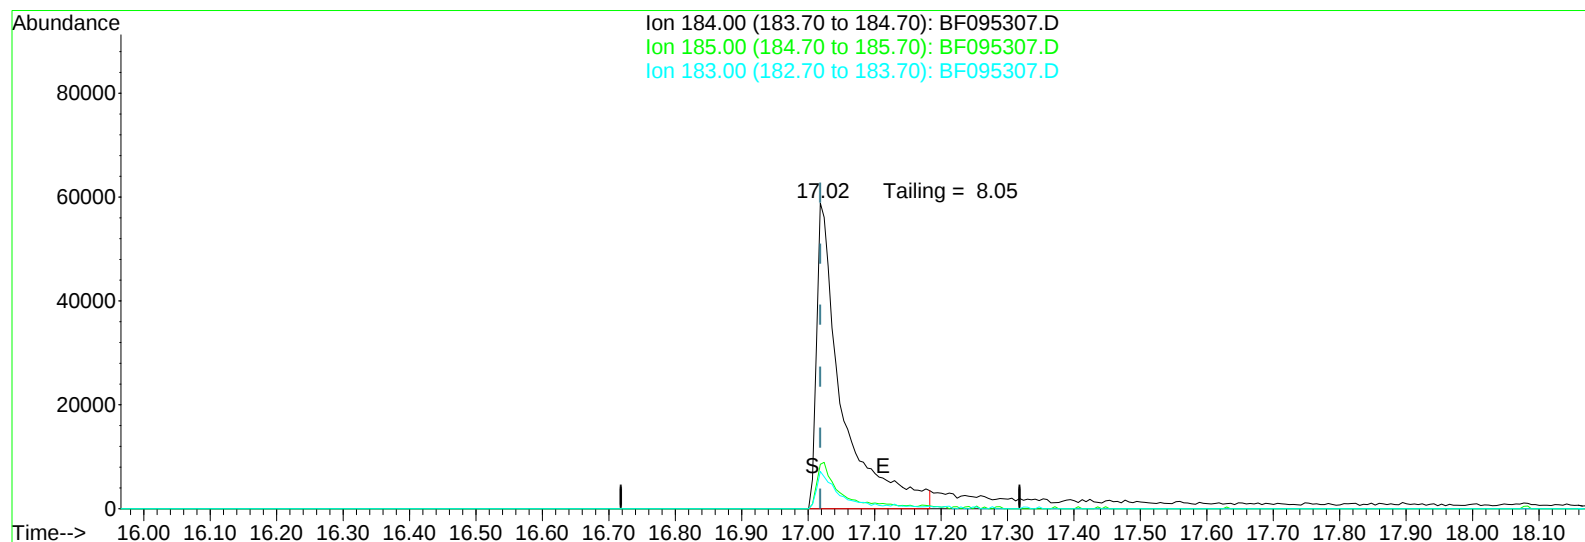

(76) Benzidine

17.018min (+0.000) 0.00ng

response 152834

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	14.50#
183.00	12.20	12.16
0.00	0.00	0.00