

Data Path : Z:\HPCHEM1\BNA F\DATA\BF052217\
 Data File : BF095343.D
 Acq On : 23 May 2017 8:49
 Operator : SJ/MA
 Sample : I3243-10
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TP-5-TP-6

Quant Time: May 23 11:38:29 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF050217.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu May 18 17:07:53 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.76	152	82488	20.00	ng	0.00
21) Naphthalene-d8	9.78	136	332335	20.00	ng	0.00
38) Acenaphthene-d10	12.61	164	147397	20.00	ng	0.00
63) Phenanthrene-d10	15.02	188	185635	20.00	ng	0.00
75) Chrysene-d12	18.69	240	163017	20.00	ng	0.00
86) Perylene-d12	20.37	264	134250	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.74	112	658318	133.06	ng	0.00
7) Phenol-d6	7.31	99	759766	127.98	ng	0.00
23) Nitrobenzene-d5	8.66	82	489746	92.93	ng	-0.01
41) 2,4,6-Tribromophenol	13.91	330	147757	122.40	ng	0.00
44) 2-Fluorobiphenyl	11.55	172	1016310	99.24	ng	-0.01
78) Terphenyl-d14	17.33	244	636004	85.93	ng	-0.02


Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF052217\
Data File : BF095343.D
Acq On : 23 May 2017 8:49
Operator : SJ/MA
Sample : I3243-10
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP-5-TP-6

Quant Time: May 23 11:38:29 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 18 17:07:53 2017
Response via : Initial Calibration

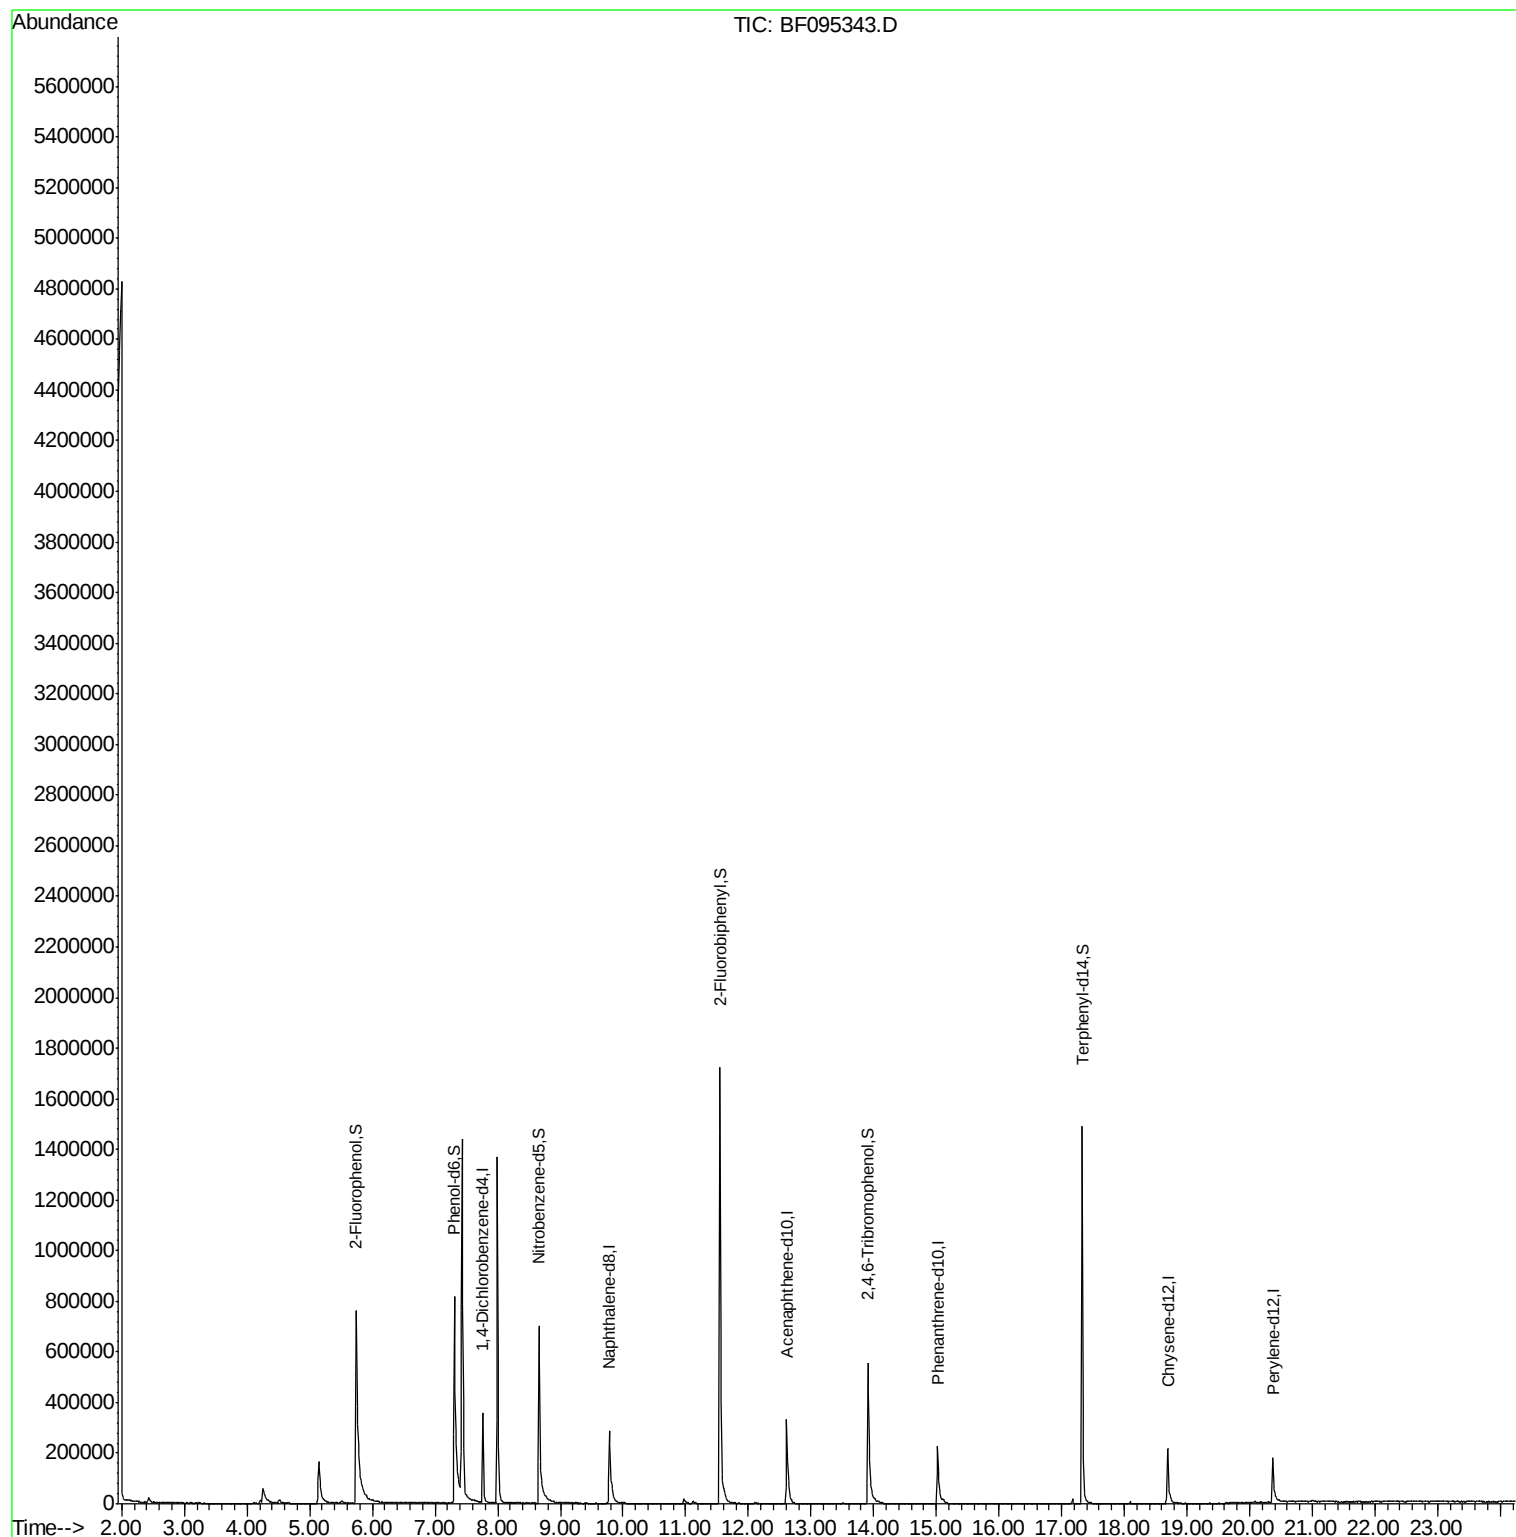




#1



1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 7.76 min Scan# 990
Delta R.T. -0.01 min
Lab File: BF095343.D
Acq: 23 May 2017 8:49

Instrument :
BNA_F
ClientSampleId :
TP-5-TP-6

Tot Ion:152 Resp: 82488
Ion Ratio Lower Upper
152 100
150 161.5 126.2 189.2
115 60.0 52.2 78.2

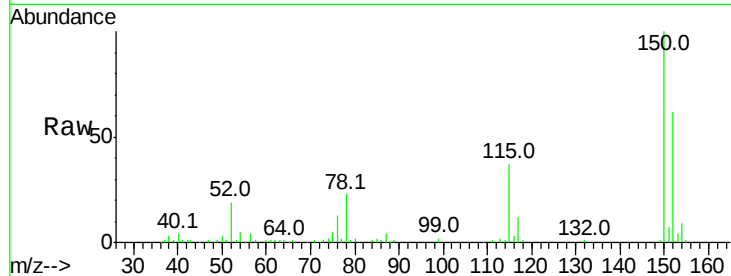


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

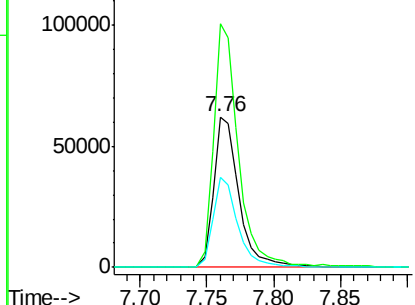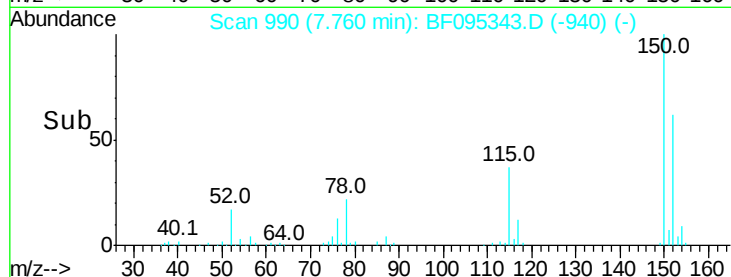



#5

2-Fluorophenol
Concen: 133.06 ng
RT: 5.74 min Scan# 647
Delta R.T. 0.01 min
Lab File: BF095343.D
Acq: 23 May 2017 8:49

Tgt Ion:112 Resp: 658318
Ion Ratio Lower Upper
112 100
64 54.3 46.0 69.0
63 26.3 23.4 35.0

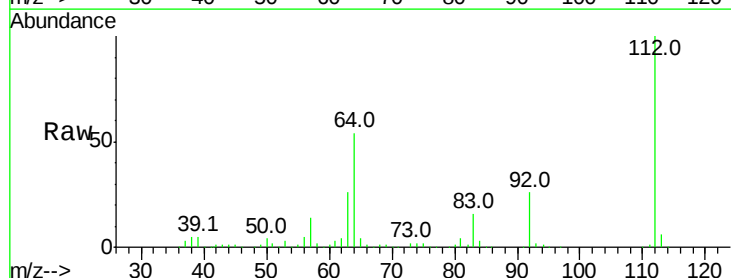

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

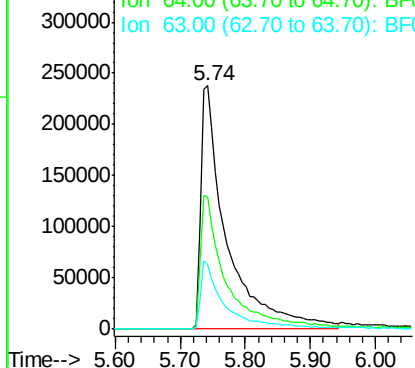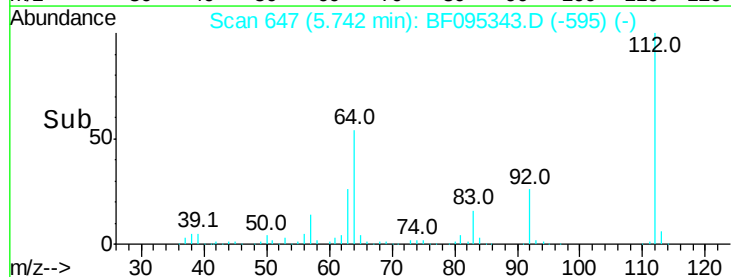



#7

Phenol-d6

Concen: 127.98 ng

RT: 7.31 min Scan# 913

Delta R.T. -0.01 min

Lab File: BF095343.D

Acq: 23 May 2017 8:49

Instrument :

BNA_F

ClientSampleId :

TP-5-TP-6


Tot Ion: 99 Resp: 759766

Ion Ratio Lower Upper

99 100

42 14.9 13.5 20.3




71 30.6 24.5 36.7

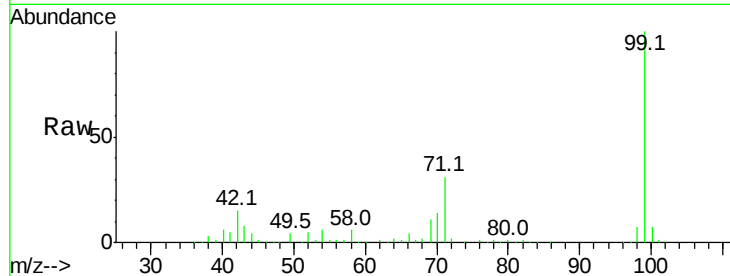

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

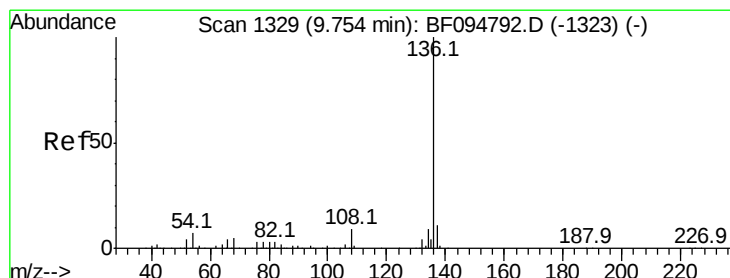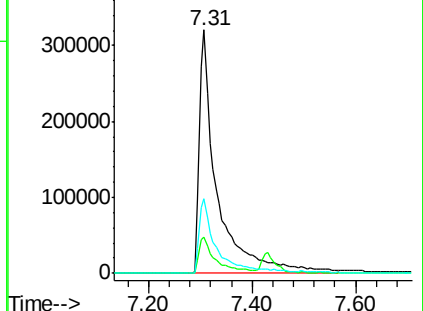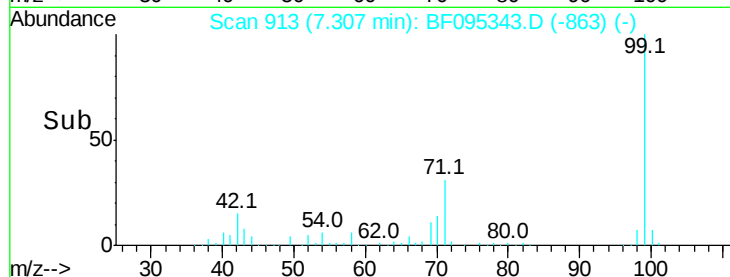

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 9.78 min Scan# 1334

Delta R.T. -0.00 min

Lab File: BF095343.D

Acq: 23 May 2017 8:49

Tgt Ion: 136 Resp: 332335


Ion Ratio Lower Upper

136 100

137 10.6 8.5 12.7

54 6.9 4.9 7.3

68 5.4 4.1 6.1


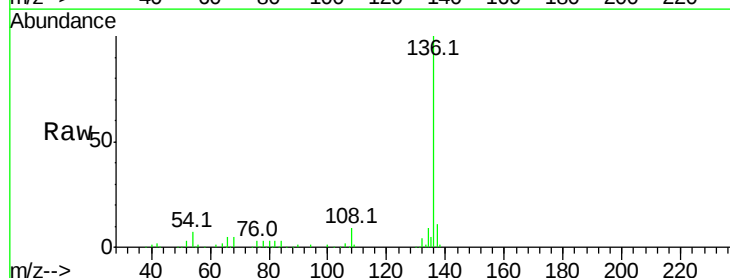



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

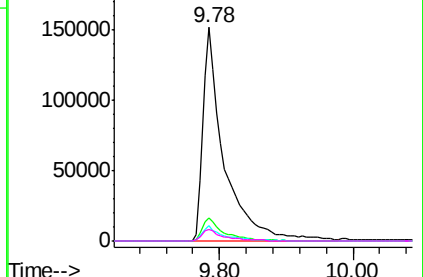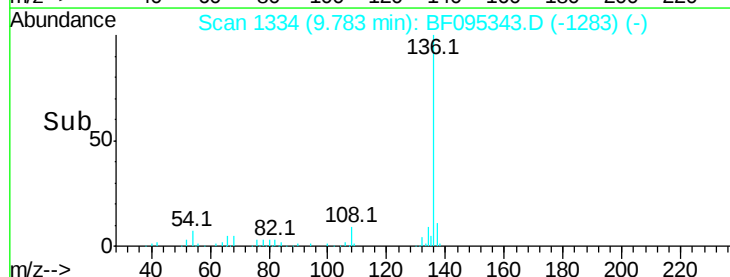

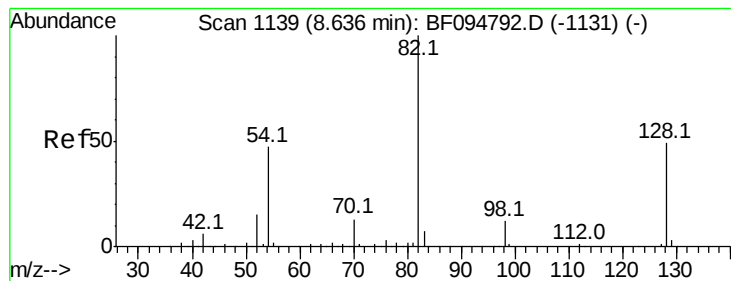

#23

Nitrobenzene-d5

Concen: 92.93 ng

RT: 8.66 min Scan# 1143

Delta R.T. -0.01 min

Lab File: BF095343.D

Acq: 23 May 2017 8:49

Instrument :

BNA_F

ClientSampleId :

TP-5-TP-6


Tot Ion: 82 Resp: 489746

Ion Ratio Lower Upper

82 100

128 47.0 34.0 51.0




54 46.8 42.2 63.2

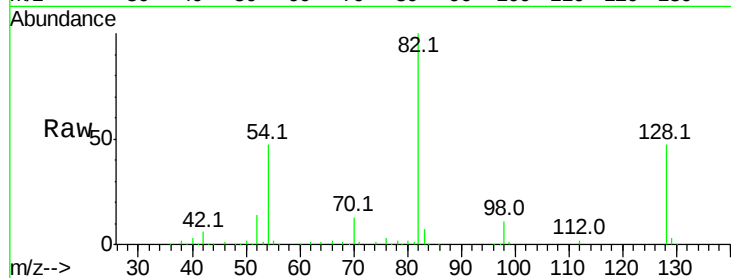

Abundance Ion 82.00 (81.70 to 82.70): BF0

Ion 128.00 (127.70 to 128.70): BF0

Ion 54.00 (53.70 to 54.70): BF0

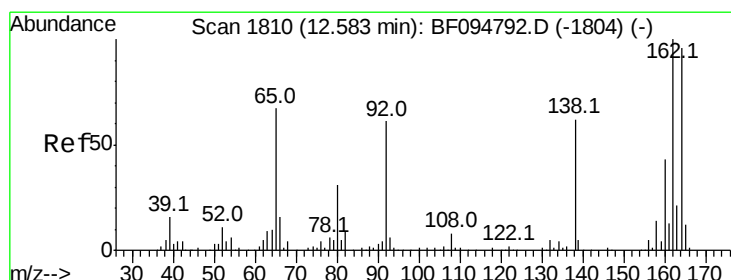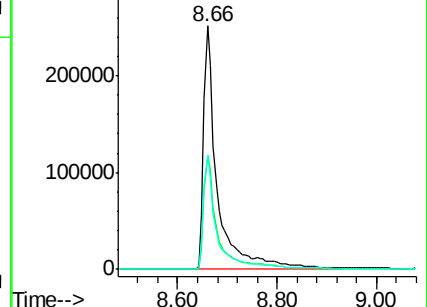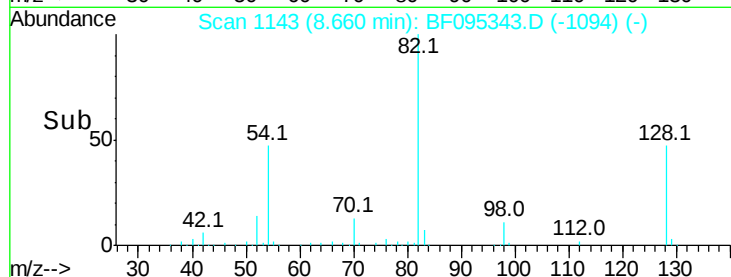

#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 12.61 min Scan# 1815

Delta R.T. -0.01 min

Lab File: BF095343.D

Acq: 23 May 2017 8:49


Tgt Ion: 164 Resp: 147397

Ion Ratio Lower Upper

164 100

162 104.2 82.6 123.8



160 46.6 36.2 54.2

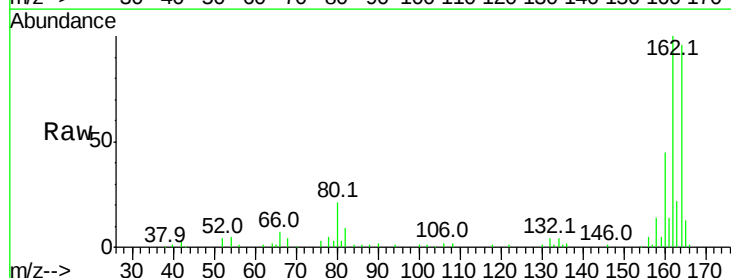

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

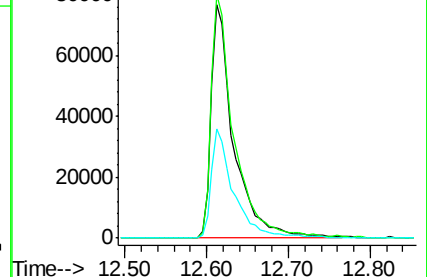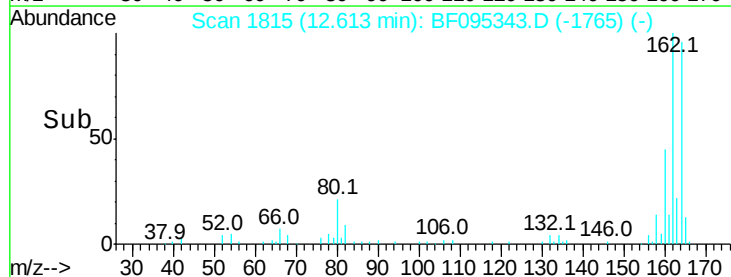







#41
 2,4,6-Tribromophenol
 Concen: 122.40 ng
 RT: 13.91 min Scan# 2036
 Delta R.T. -0.01 min
 Lab File: BF095343.D
 Acq: 23 May 2017 8:49

Instrument :
 BNA_F
 ClientSampleId :
 TP-5-TP-6

Tot Ion:330 Resp: 147757
 Ion Ratio Lower Upper
 330 100
 332 97.0 76.6 115.0
 141 39.5 31.4 47.2

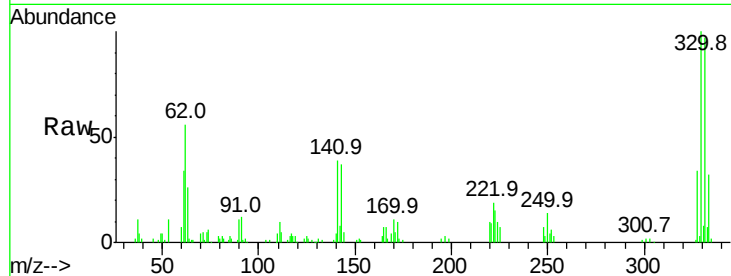


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

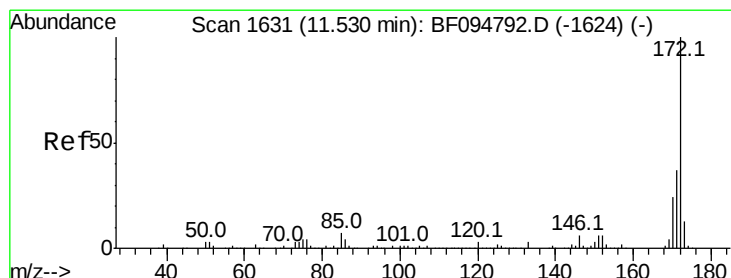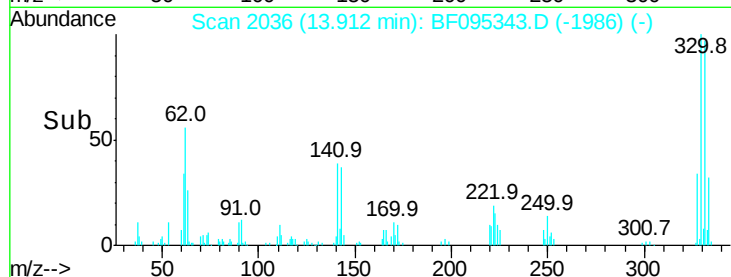
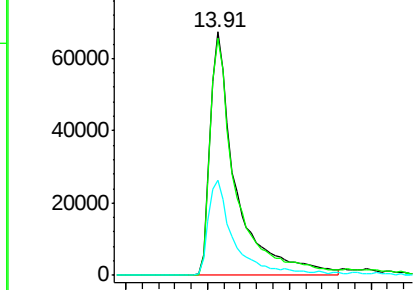



#44
 2-Fluorobiphenyl
 Concen: 99.24 ng
 RT: 11.55 min Scan# 1634
 Delta R.T. -0.01 min
 Lab File: BF095343.D
 Acq: 23 May 2017 8:49

Tgt Ion:172 Resp: 1016310
 Ion Ratio Lower Upper
 172 100
 171 36.8 29.6 44.4
 170 23.8 19.8 29.8

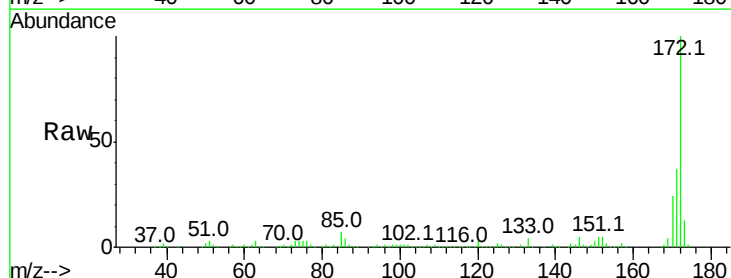

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

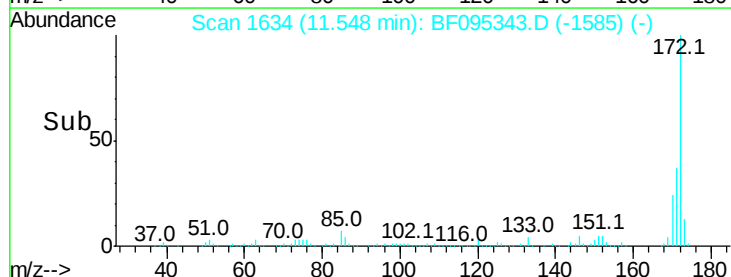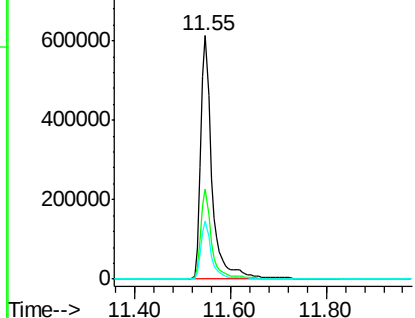


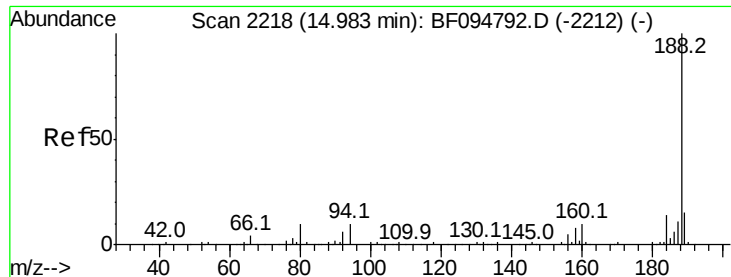




#63
 Phenanthrene-d10
 Concen: 20.00 ng
 RT: 15.02 min Scan# 2225
 Delta R.T. 0.00 min
 Lab File: BF095343.D
 Acq: 23 May 2017 8:49

Instrument :
 BNA_F
 ClientSampleId :
 TP-5-TP-6

Tot Ion:188 Resp: 185635
 Ion Ratio Lower Upper
 188 100
 94 10.6 9.4 14.2
 80 11.0 10.2 15.2

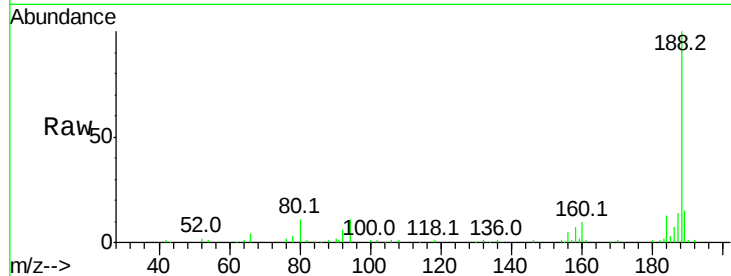


Abundance Ion 188.00 (187.70 to 188.70): E
 Ion 94.00 (93.70 to 94.70): BF0
 Ion 80.00 (79.70 to 80.70): BF0

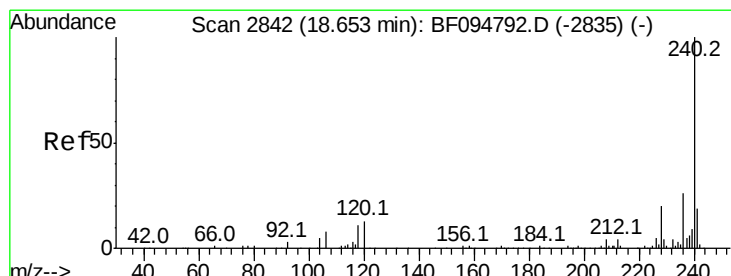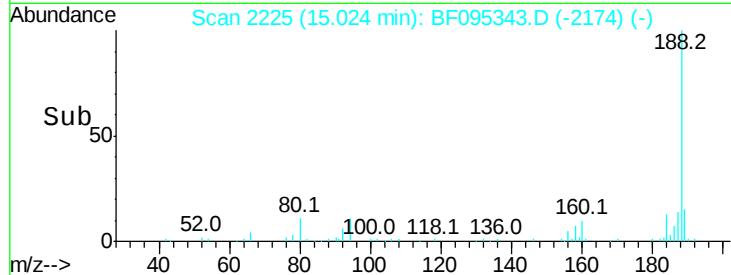
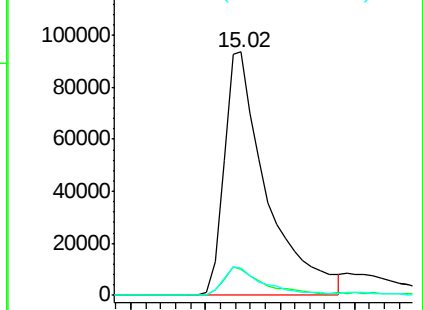



#75
 Chrysene-d12
 Concen: 20.00 ng
 RT: 18.69 min Scan# 2849
 Delta R.T. 0.00 min
 Lab File: BF095343.D
 Acq: 23 May 2017 8:49

Tgt Ion:240 Resp: 163017
 Ion Ratio Lower Upper
 240 100
 120 14.2 5.8 8.8#
 236 25.7 20.5 30.7

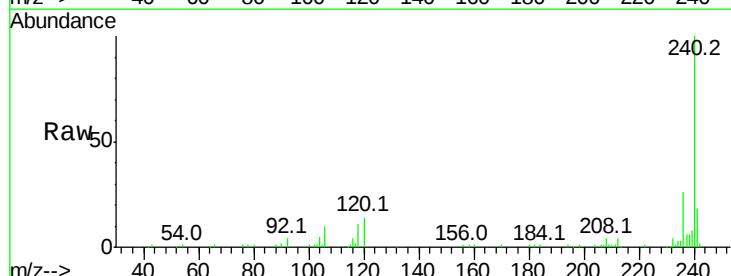

Abundance Ion 240.00 (239.70 to 240.70): E
 Ion 120.00 (119.70 to 120.70): E
 Ion 236.00 (235.70 to 236.70): E

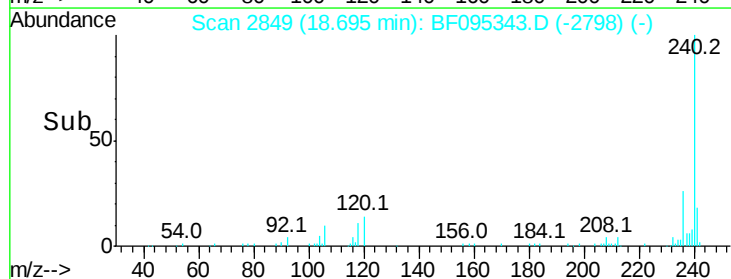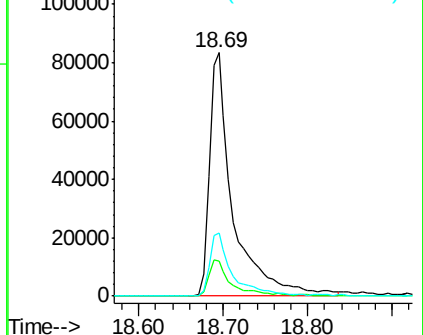

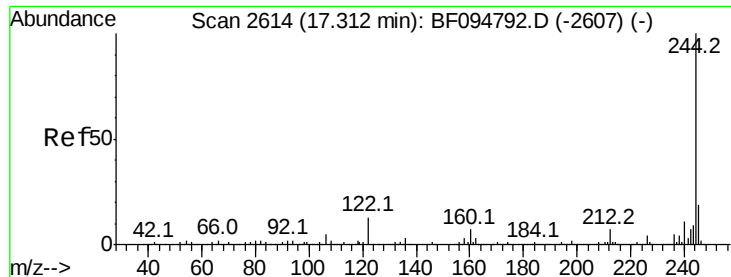

#78

Terphenyl-d14

Concen: 85.93 ng

RT: 17.33 min Scan# 2617

Delta R.T. -0.02 min

Lab File: BF095343.D

Acq: 23 May 2017 8:49

Instrument :

BNA_F

ClientSampleId :

TP-5-TP-6


Tot Ion:244 Resp: 636004

Ion Ratio Lower Upper

244 100

212 6.6 6.0 9.0




122 14.0 10.3 15.5

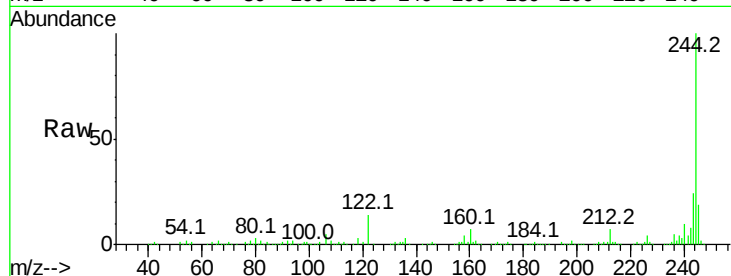

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

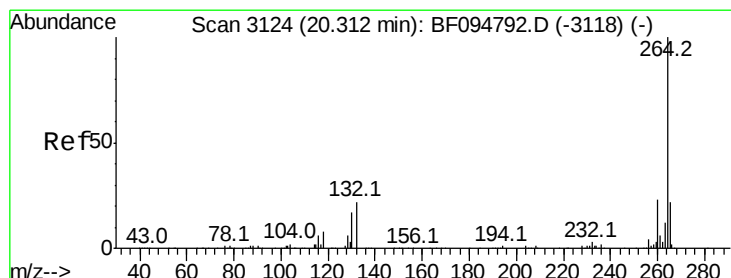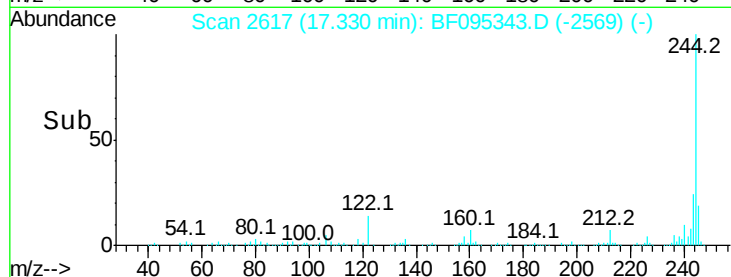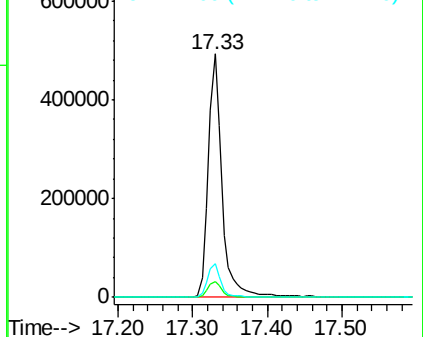

#86

Perylene-d12

Concen: 20.00 ng

RT: 20.37 min Scan# 3134

Delta R.T. 0.01 min

Lab File: BF095343.D

Acq: 23 May 2017 8:49


Tgt Ion:264 Resp: 134250

Ion Ratio Lower Upper

264 100

260 23.2 19.5 29.3

265 20.7 17.2 25.8

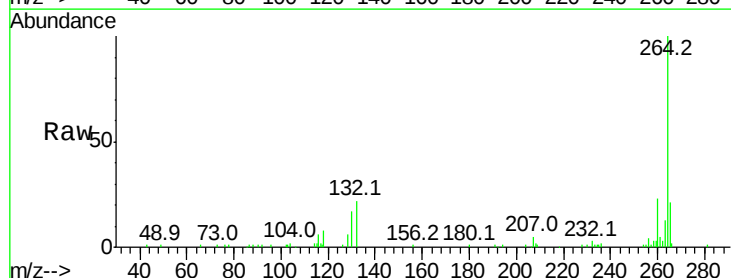

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

