


Data Path : Z:\HPCHEM1\BNA F\Data\BF052217\
 Data File : BF095307.D
 Acq On : 22 May 2017 10:58
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu May 18 17:07:53 2017

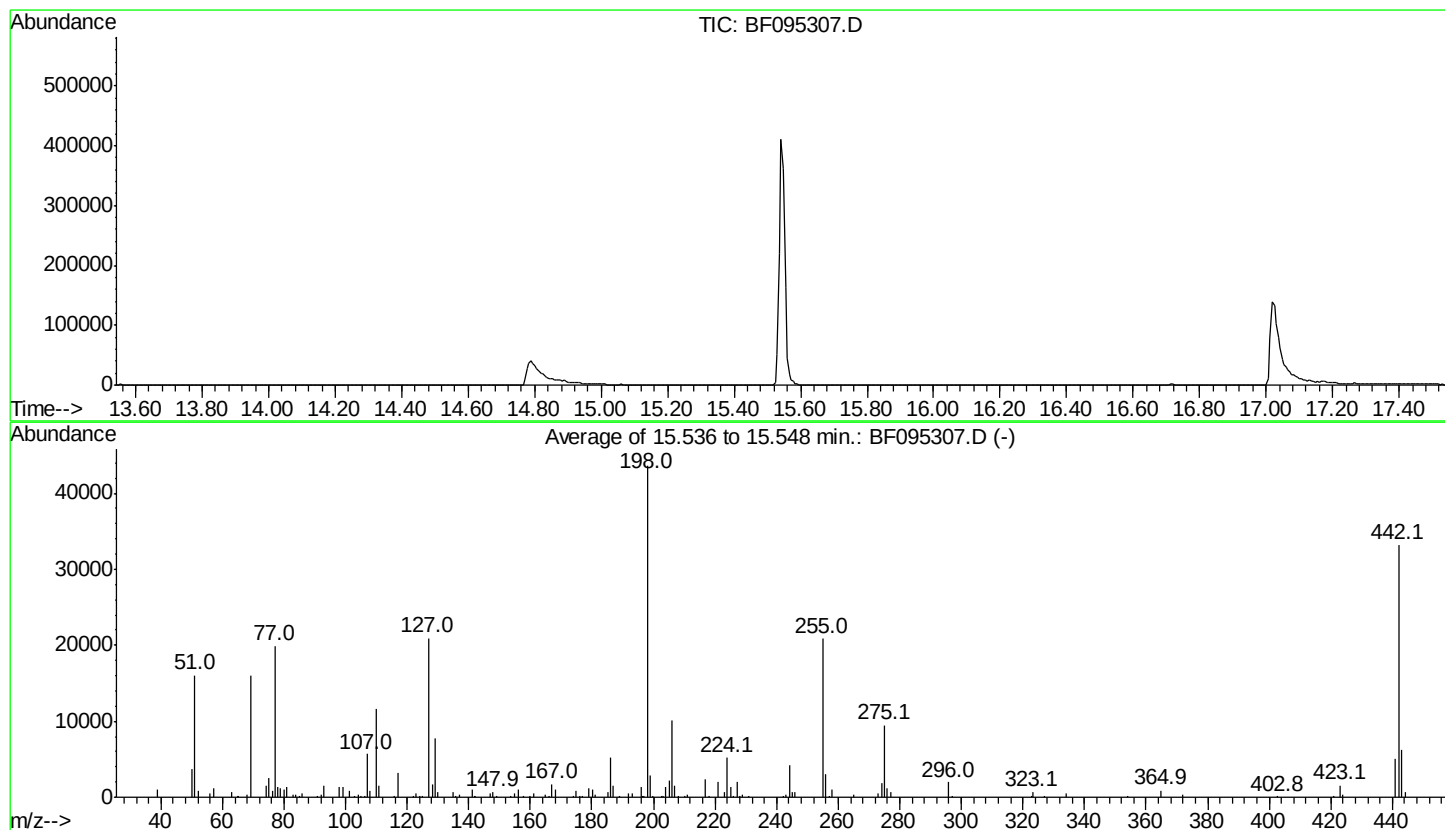

AutoFind: Scans 2312, 2313, 2314; Background Corrected with Scan 2307

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.9	16088	PASS
68	69	0.00	2	1.6	260	PASS
69	198	0.00	100	36.6	15988	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.1	20970	PASS
197	198	0.00	2	0.5	199	PASS
198	198	100	100	100.0	43629	PASS
199	198	5	9	6.7	2919	PASS
275	198	10	60	21.7	9454	PASS
365	198	1	100	2.0	891	PASS
441	442	0.01	24	15.5	5131	PASS
442	198	50	100	76.1	33185	PASS
443	442	15	24	18.9	6266	PASS