
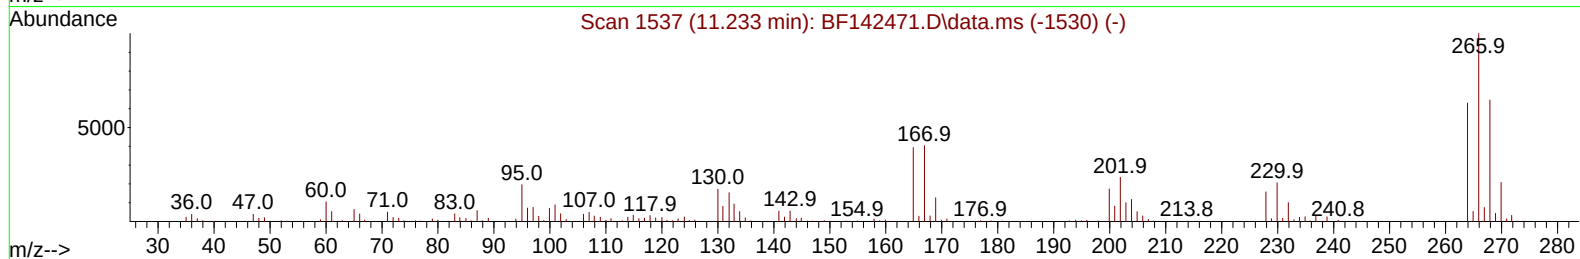
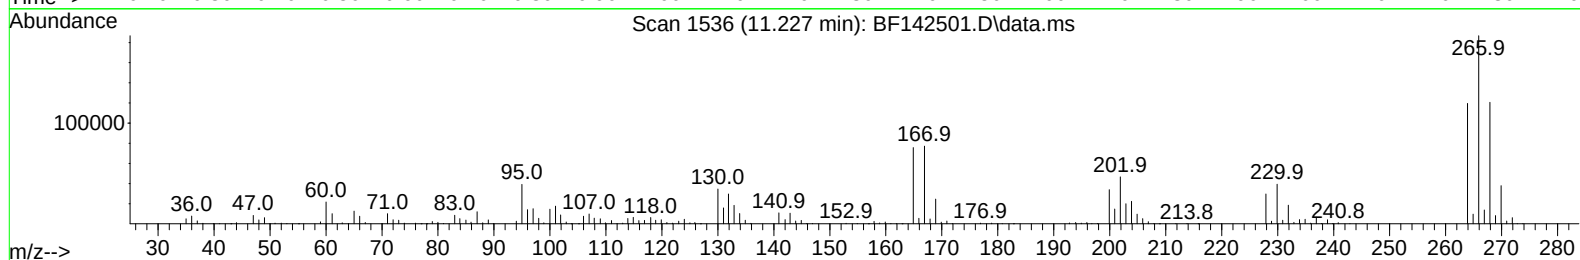


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052225\
Data File : BF142501.D
Acq On : 22 May 2025 10:43
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 22 12:24:21 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 20 16:26:47 2025
Response via : Initial Calibration

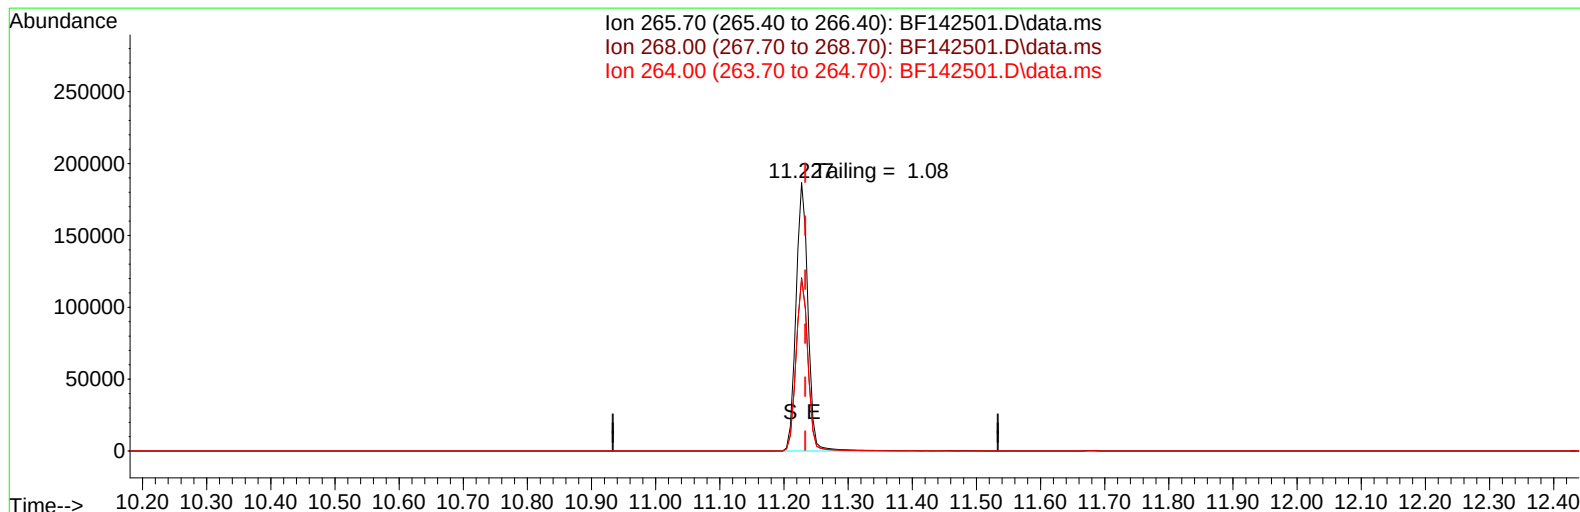

TIC: BF142501.D\data.ms

(70) Pentachlorophenol (C)




11.227min (-0.006) 79510.36 ng

response 243635

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.60	64.59
264.00	63.00	64.05
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052225\
Data File : BF142501.D
Acq On : 22 May 2025 10:43
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 22 12:24:21 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 20 16:26:47 2025
Response via : Initial Calibration

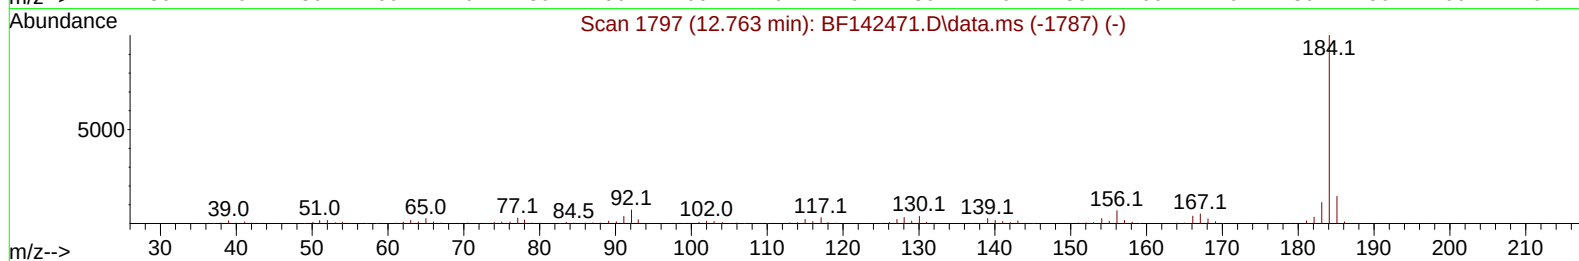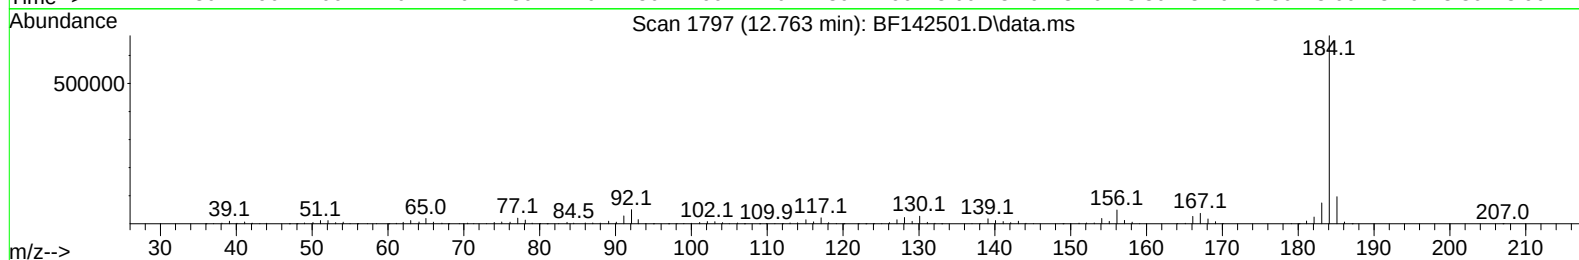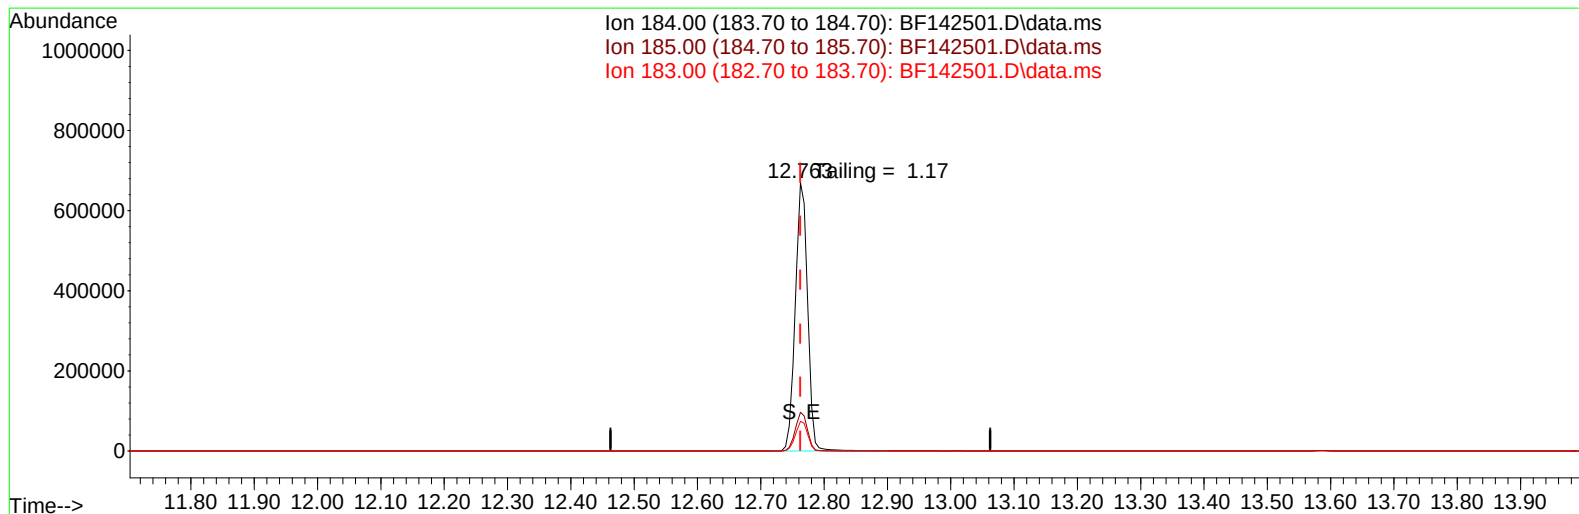

TIC: BF142501.D\data.ms

(77) Benzidine**12.763min (+ 0.000) 104325.96 ng****response 908454**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.43
183.00	11.20	11.07
0.00	0.00	0.00