

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052225\
 Data File : BF142522.D
 Acq On : 22 May 2025 20:53
 Operator : RC/JU
 Sample : Q2097-17
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 RT-3888

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052025.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF142522.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.116	488	497	505	rBV	137972	208097	11.08%	1.494%
2	5.510	558	564	570	rBV	1334059	1818398	96.79%	13.055%
3	6.516	729	735	748	rVB	1332154	1814509	96.59%	13.027%
4	6.898	795	800	805	rBV	506550	614003	32.68%	4.408%
5	7.457	889	895	900	rBV	868180	1103709	58.75%	7.924%
6	8.181	1013	1018	1023	rBV	579126	709768	37.78%	5.096%
7	9.251	1195	1200	1206	rBV	1452228	1878630	100.00%	13.487%
8	9.933	1311	1316	1321	rBV	545537	675529	35.96%	4.850%
9	10.345	1382	1386	1391	rVB4	16531	23104	1.23%	0.166%
10	10.645	1433	1437	1445	rBV	292547	371803	19.79%	2.669%
11	10.722	1445	1450	1456	rBV	834643	1048510	55.81%	7.527%
12	10.957	1486	1490	1494	rBV	42669	56593	3.01%	0.406%
13	11.422	1565	1569	1576	rBV	509607	647516	34.47%	4.649%
14	11.945	1654	1658	1667	rBV	94766	150632	8.02%	1.081%
15	13.010	1834	1839	1844	rVB	1357628	1697253	90.35%	12.185%
16	13.904	1987	1991	2007	rBV	64218	127080	6.76%	0.912%
17	14.063	2013	2018	2027	rVB	409465	550896	29.32%	3.955%
18	15.557	2266	2272	2288	rVB	263027	433139	23.06%	3.110%




Sum of corrected areas: 13929169

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052225\
Data File : BF142522.D
Acq On : 22 May 2025 20:53
Operator : RC/JU
Sample : Q2097-17
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
RT-3888

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

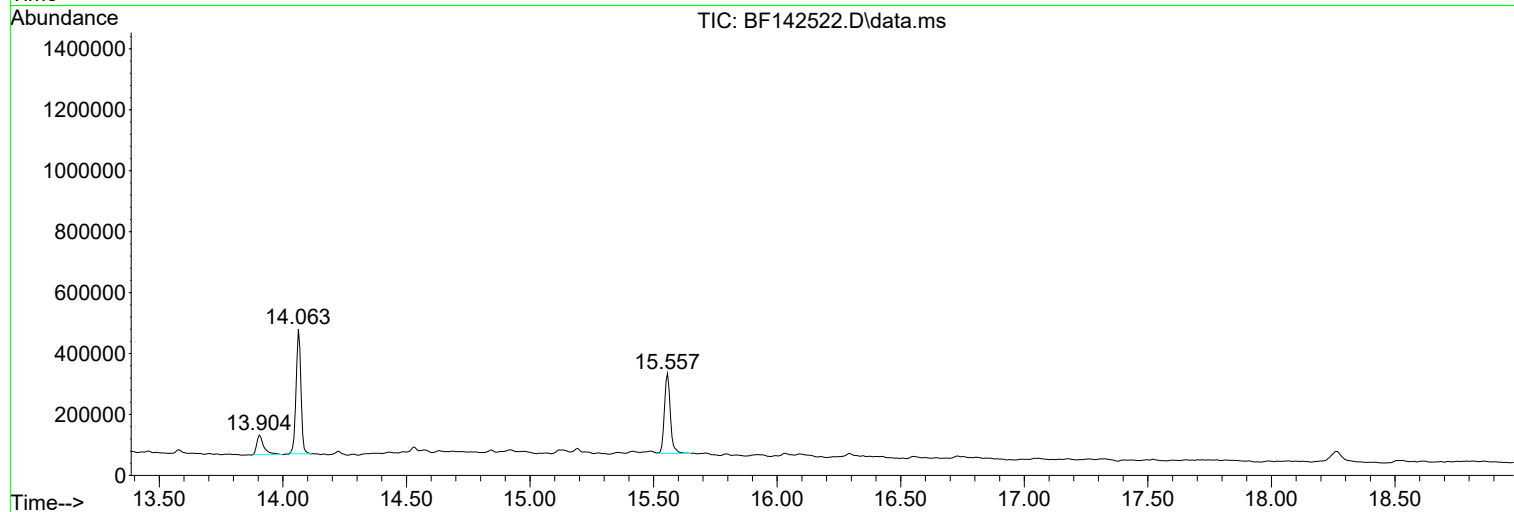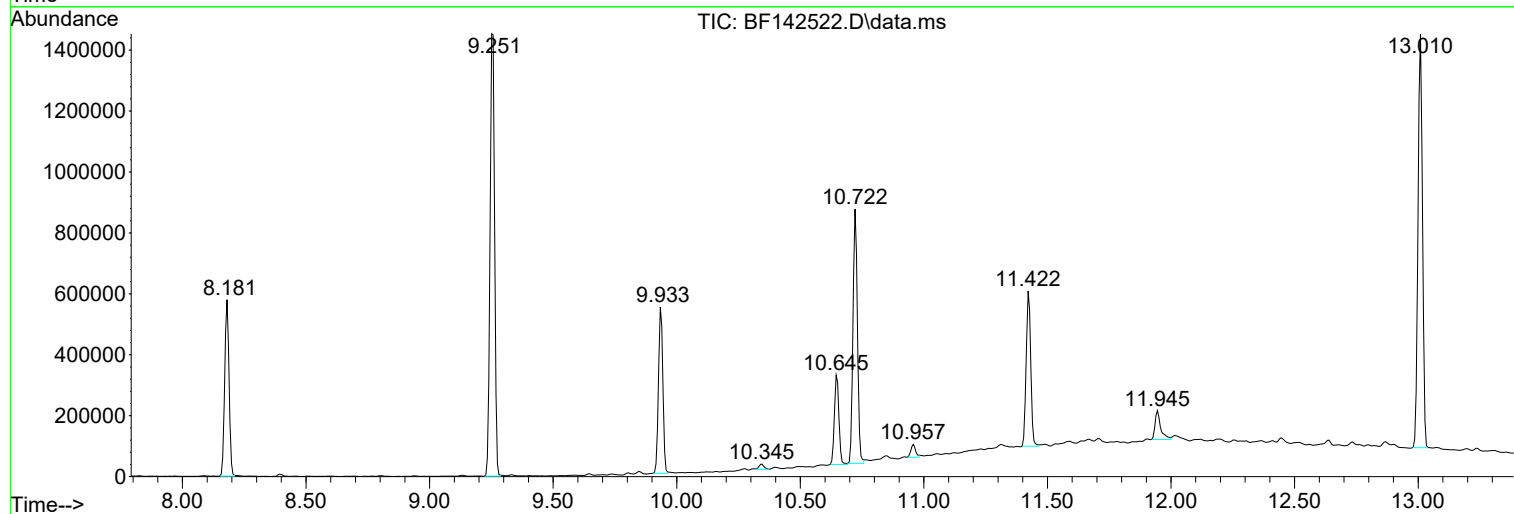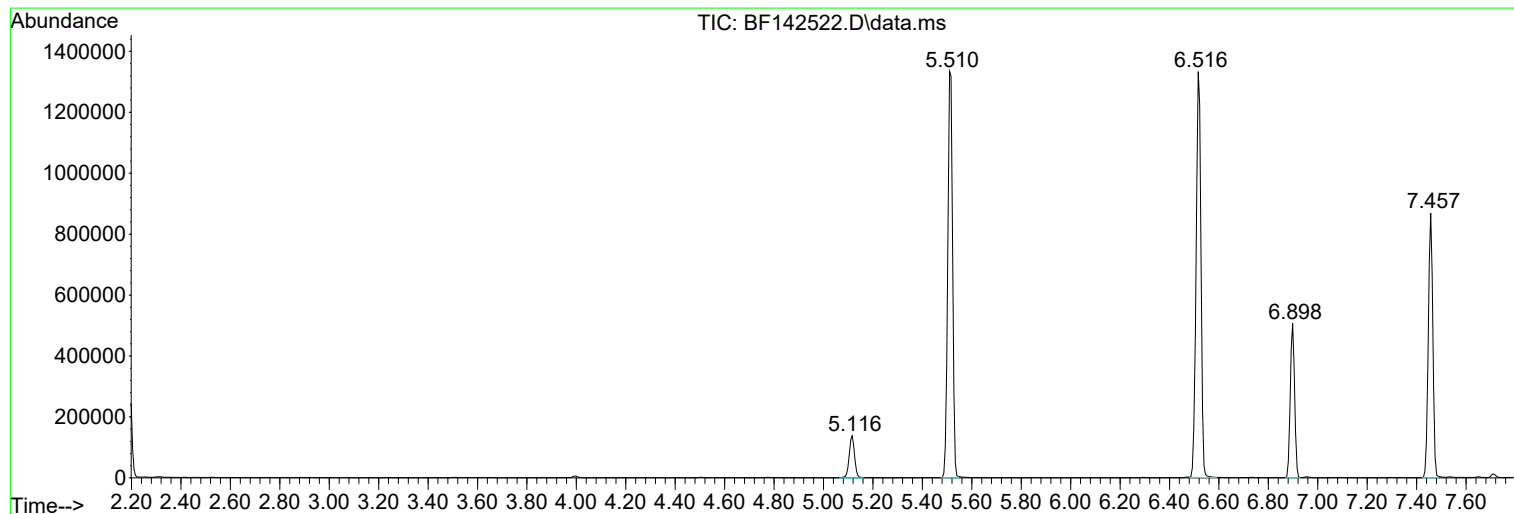

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052225\
Data File : BF142522.D
Acq On : 22 May 2025 20:53
Operator : RC/JU
Sample : Q2097-17
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
RT-3888

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052225\
Data File : BF142522.D
Acq On : 22 May 2025 20:53
Operator : RC/JU
Sample : Q2097-17
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
RT-3888

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------