



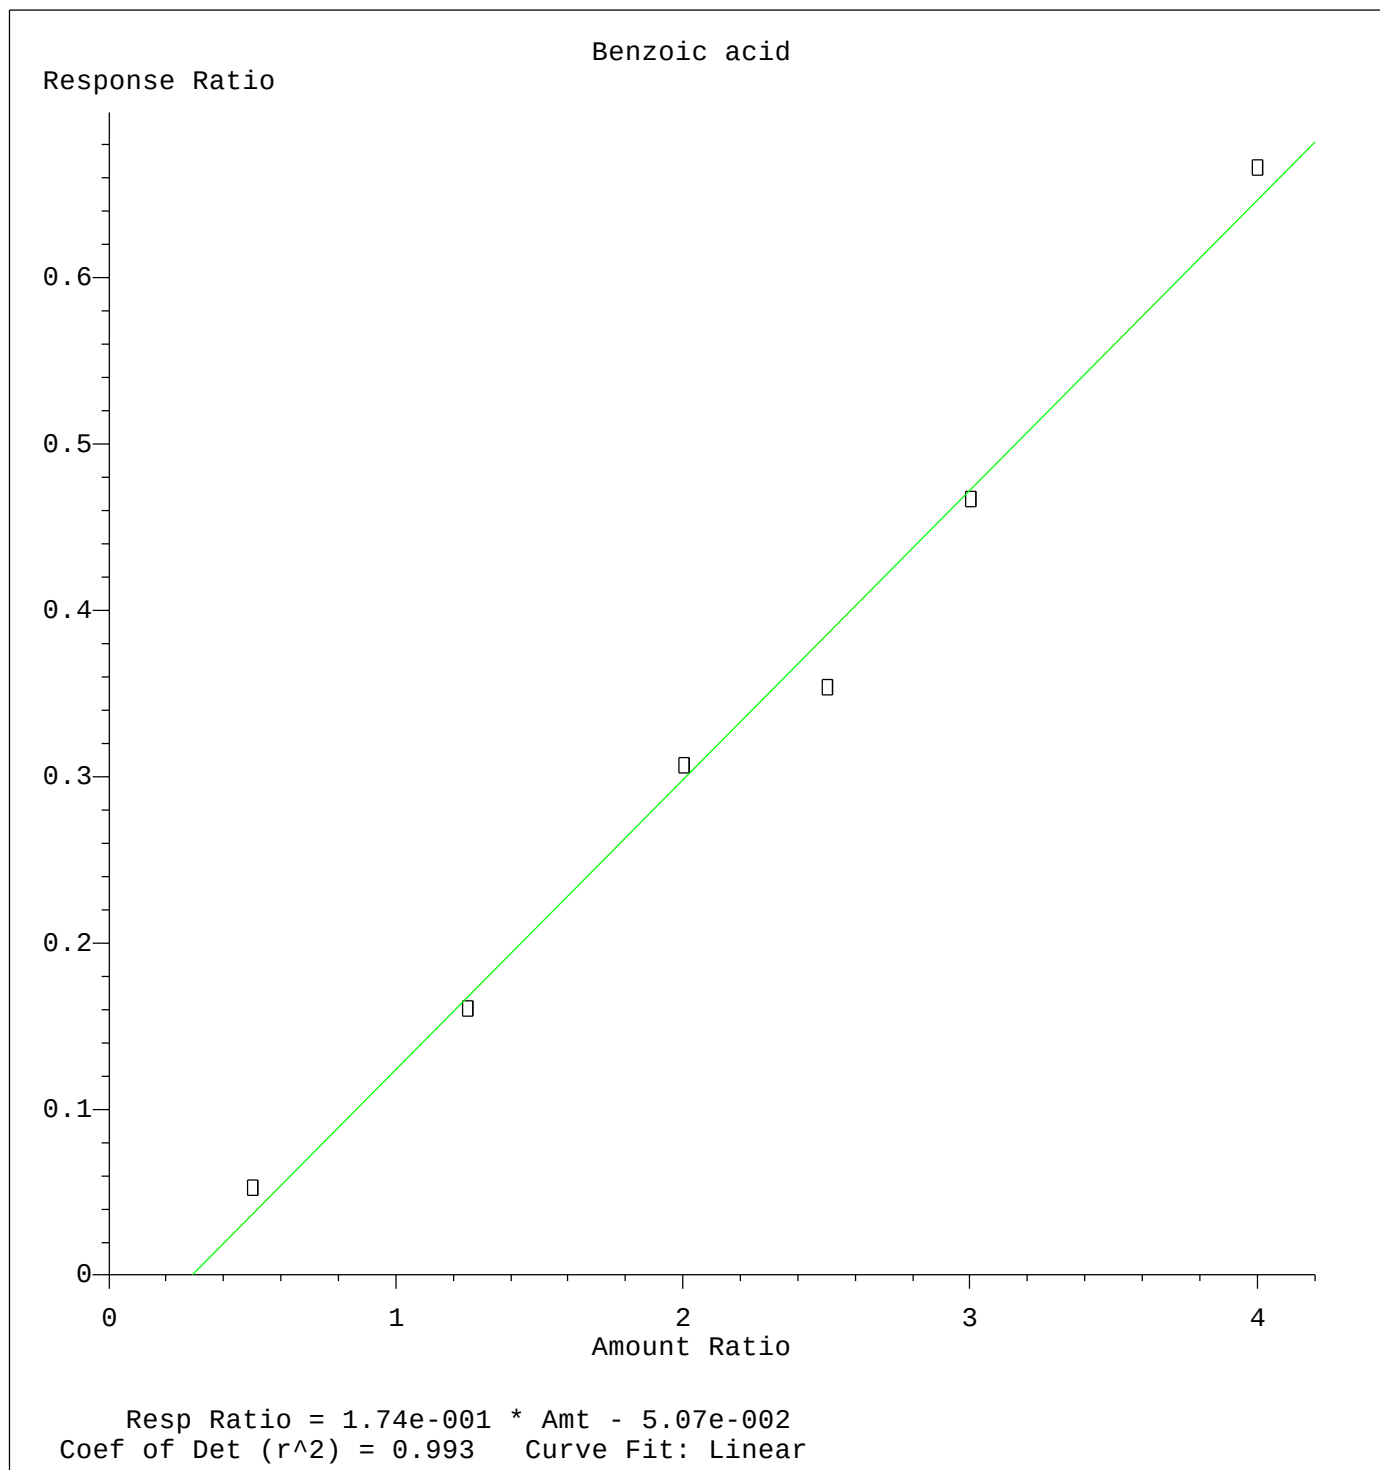

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF052316.M
Calibration Table Last Updated: Tue May 24 01:40:43 2016


Hexachlorocyclopentadiene

Response Ratio

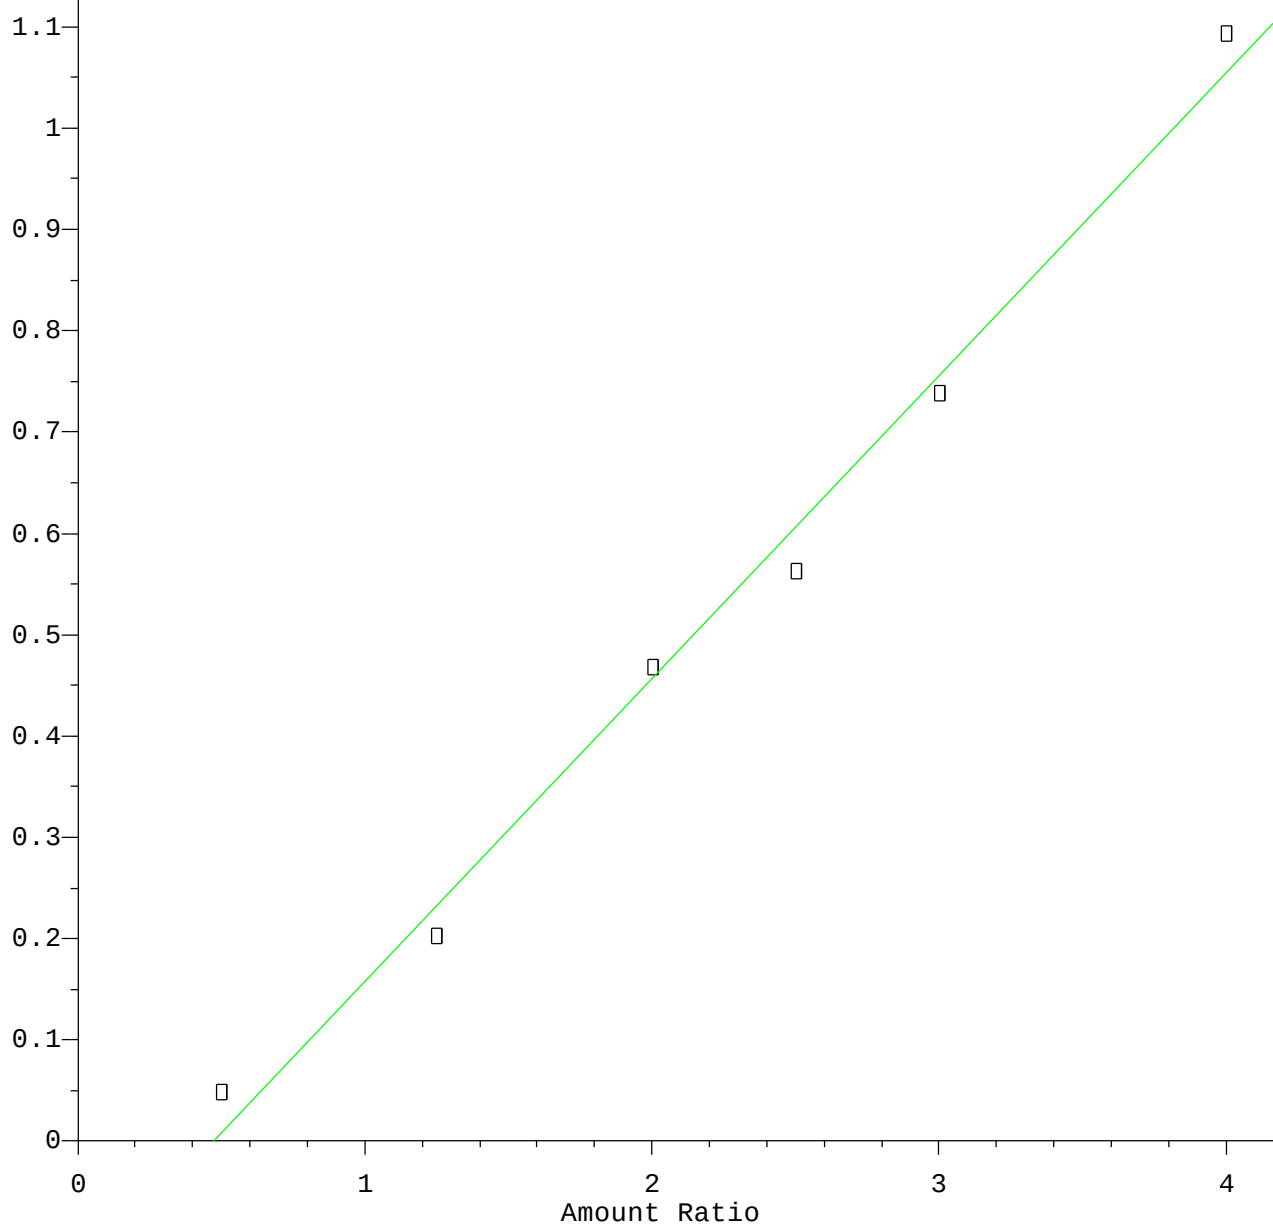


Resp Ratio = $2.99 \times 10^{-1} \times \text{Amt} - 1.41 \times 10^{-1}$
Coef of Det (r^2) = 0.991 Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF052316.M
Calibration Table Last Updated: Tue May 24 01:40:43 2016

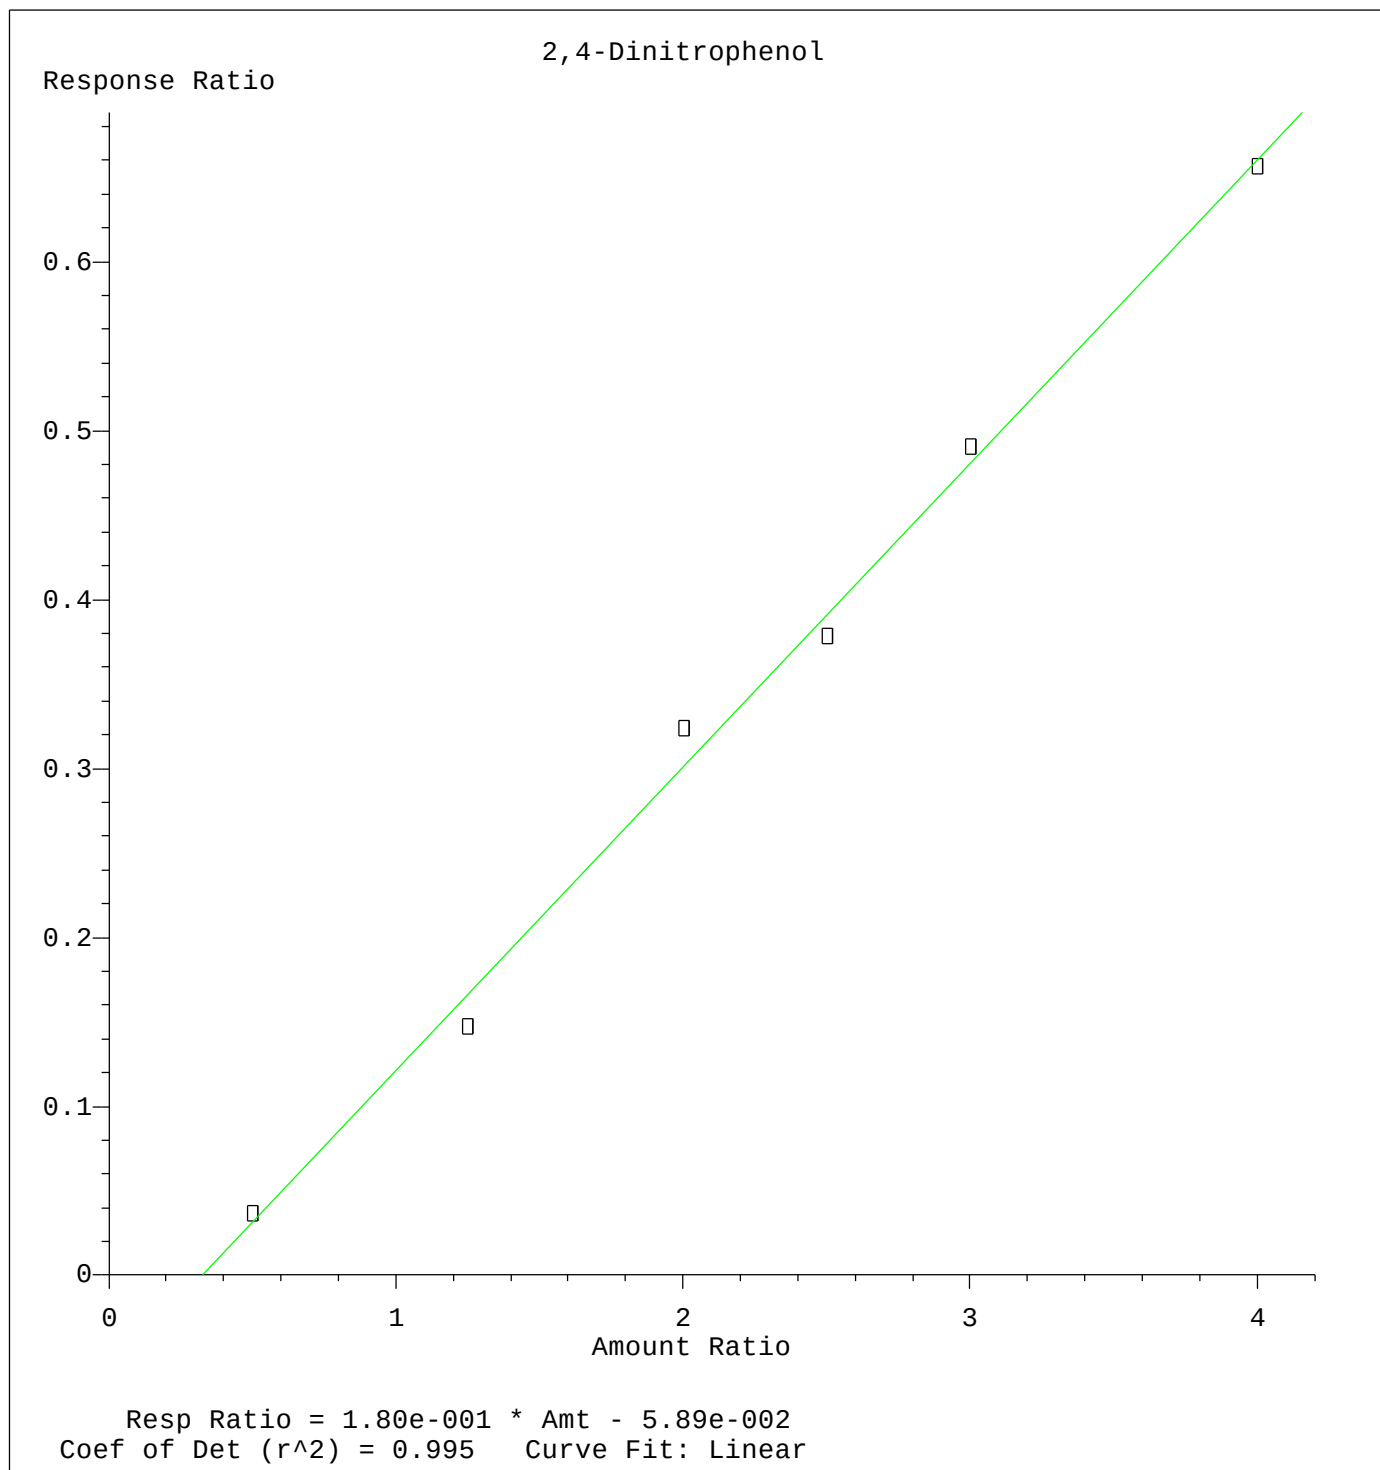

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF052316.M
Calibration Table Last Updated: Tue May 24 01:40:43 2016

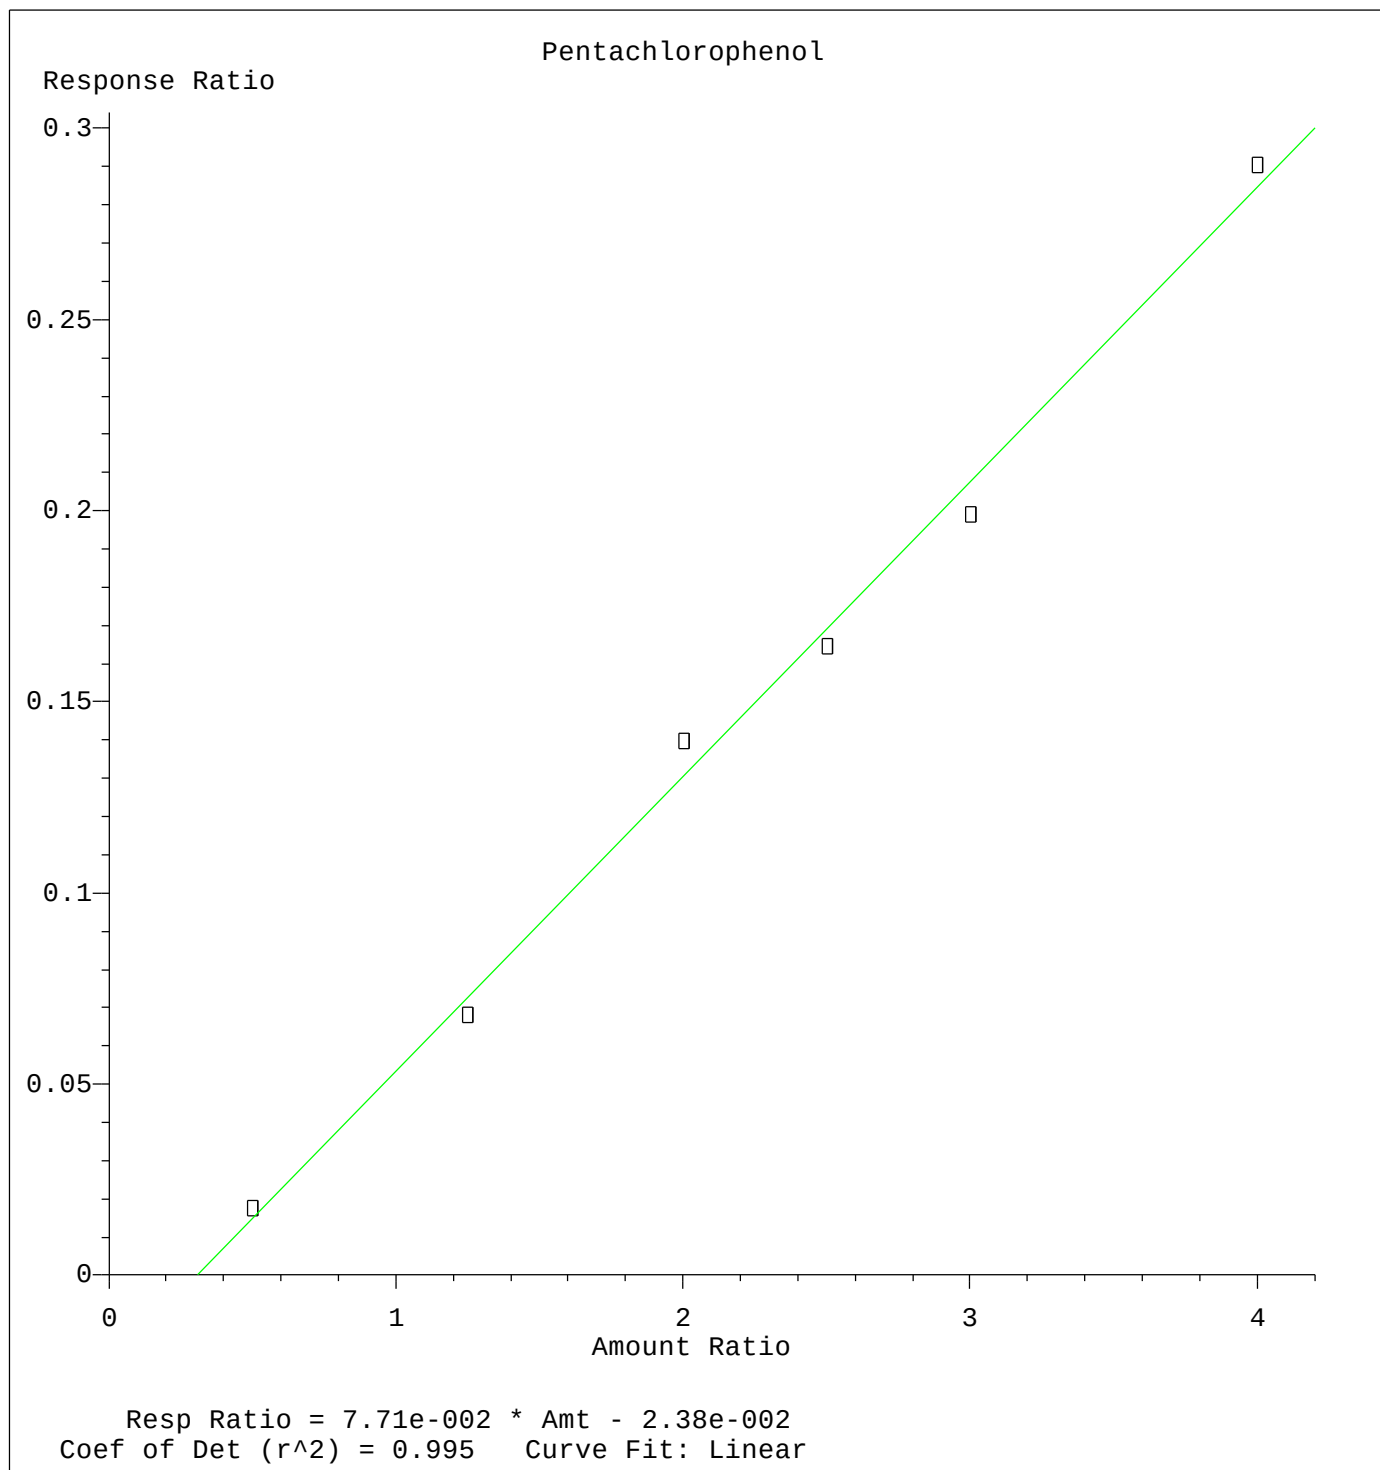

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF052316.M
Calibration Table Last Updated: Tue May 24 01:40:43 2016