

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF052316\
 Data File : BF087340.D
 Acq On : 24 May 2016 14:02
 Operator : UM/SJ
 Sample : H3169-08
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-06-COMP

Quant Time: May 24 19:03:11 2016
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052316.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 24 01:40:43 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.61	152	134505	20.00	ng	0.00
21) Naphthalene-d8	9.64	136	570161	20.00	ng	0.00
38) Acenaphthene-d10	12.47	164	259079	20.00	ng	-0.01
63) Phenanthrene-d10	14.88	188	462226	20.00	ng	0.00
75) Chrysene-d12	18.56	240	315827	20.00	ng	0.00
86) Perylene-d12	20.22	264	254283	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.53	112	908341	118.66	ng	0.01
7) Phenol-d6	7.15	99	1192627	115.30	ng	-0.01
23) Nitrobenzene-d5	8.52	82	822874	72.74	ng	-0.01
41) 2,4,6-Tribromophenol	13.77	330	264469	106.23	ng	-0.01
44) 2-Fluorobiphenyl	11.42	172	1354064	73.68	ng	-0.01
78) Terphenyl-d14	17.21	244	1056889	71.14	ng	-0.01
Target Compounds						
49) Dimethylphthalate	12.11	163	164688	7.94	ng	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF052316\
Data File : BF087340.D
Acq On : 24 May 2016 14:02
Operator : UM/SJ
Sample : H3169-08
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-06-COMP

Quant Time: May 24 19:03:11 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 24 01:40:43 2016
Response via : Initial Calibration

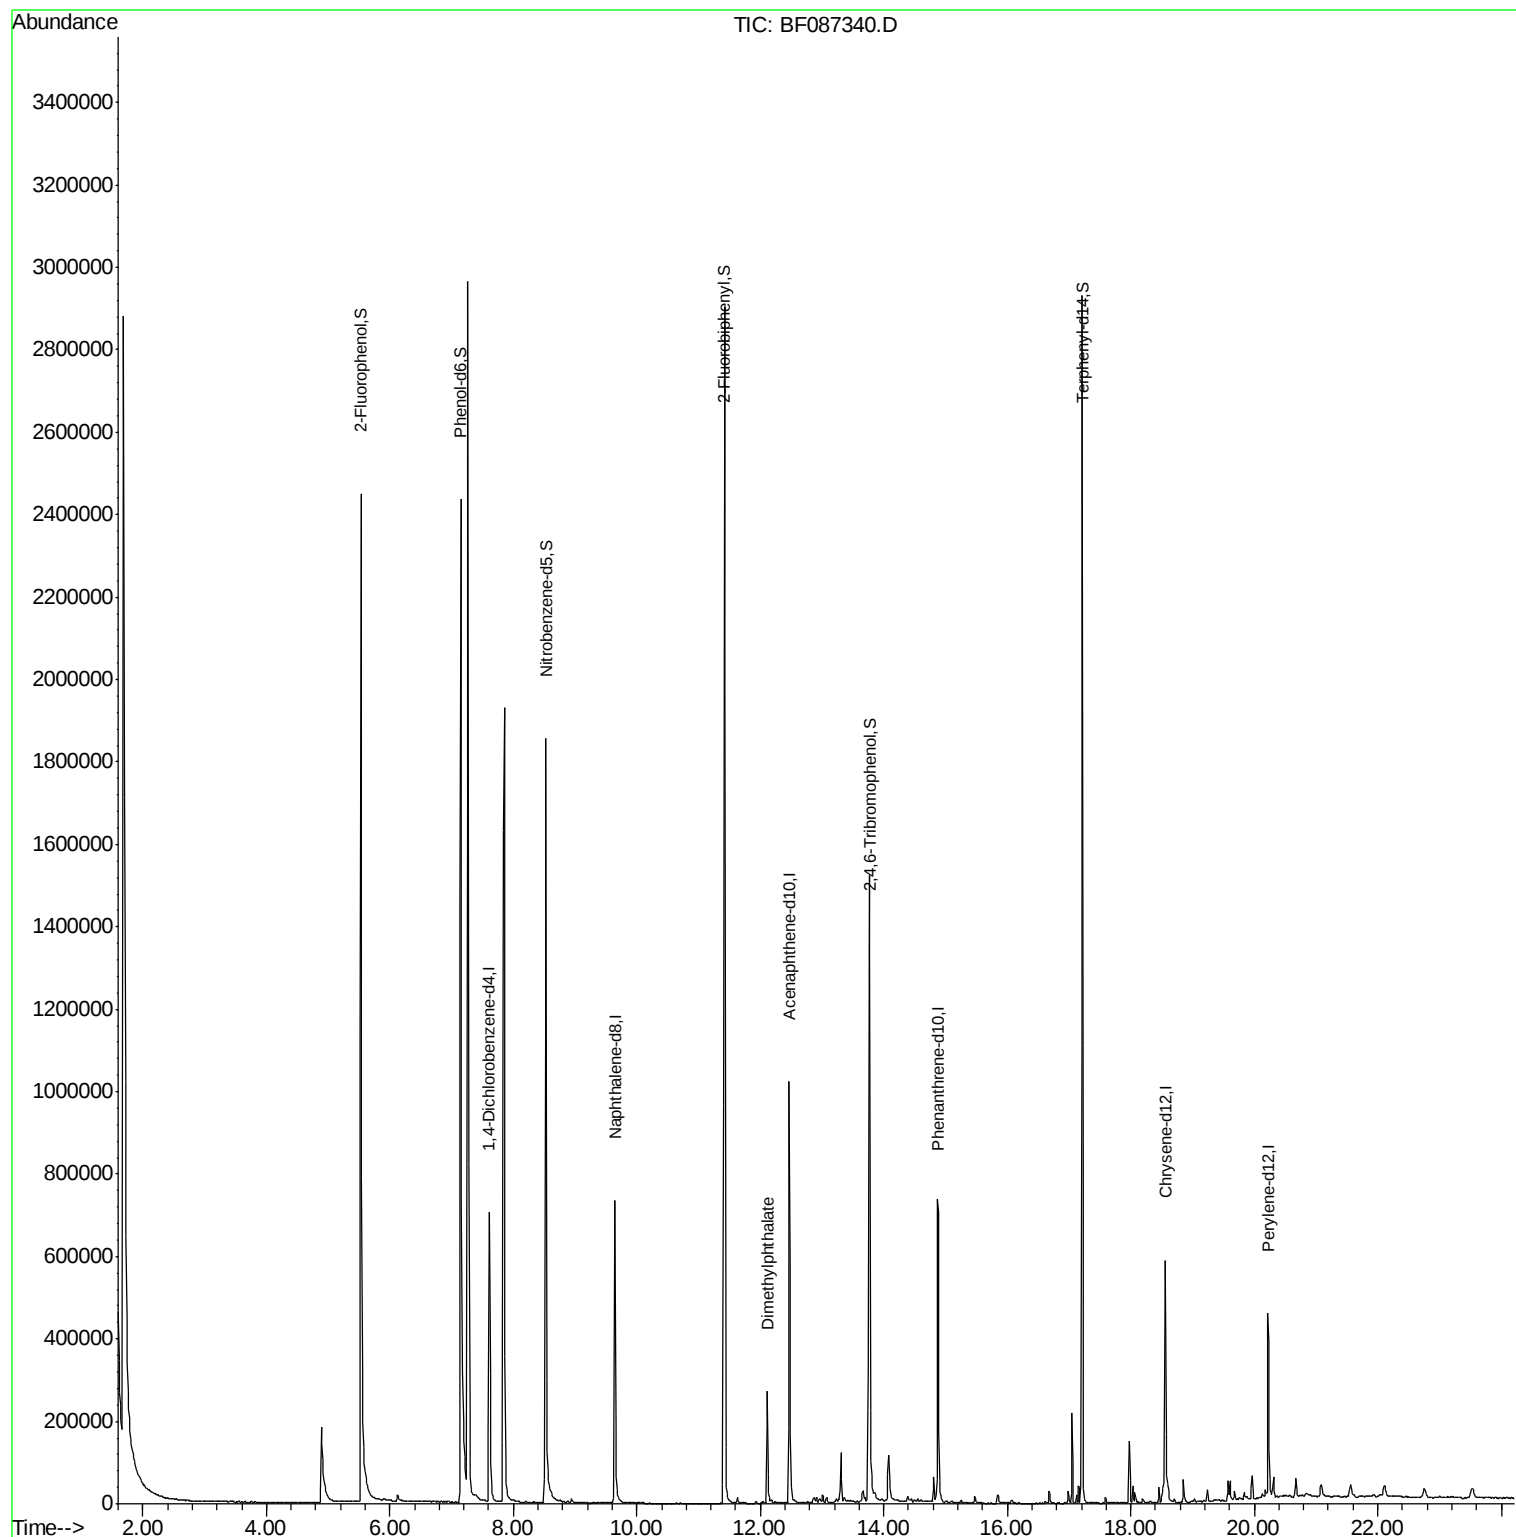

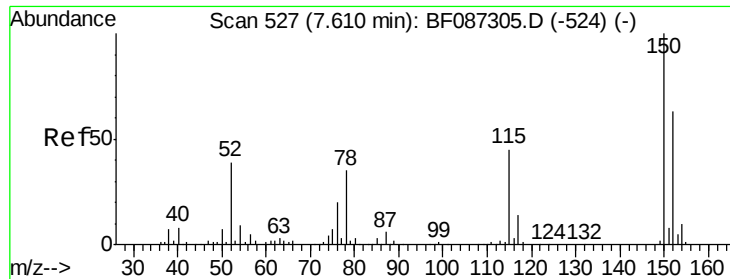


#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 7.61 min Scan# 527
Delta R.T. 0.00 min
Lab File: BF087340.D
Acq: 24 May 2016 14:02

Instrument :
BNA_F
ClientSampleId :
SB-06-COMP

Tgt Ion:152 Resp: 134505
Ion Ratio Lower Upper
152 100
150 157.0 125.8 188.6
115 66.7 51.5 77.3

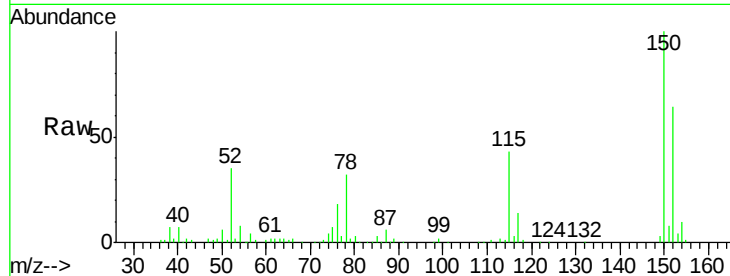


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

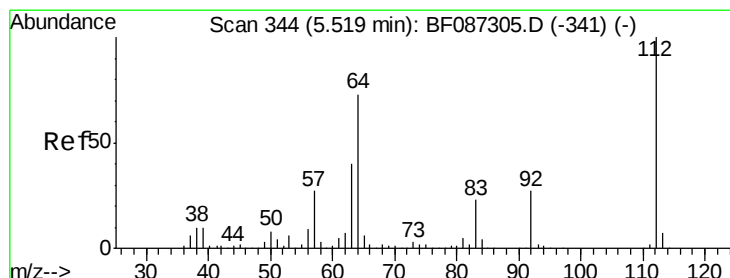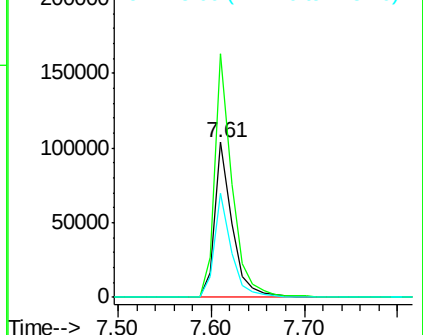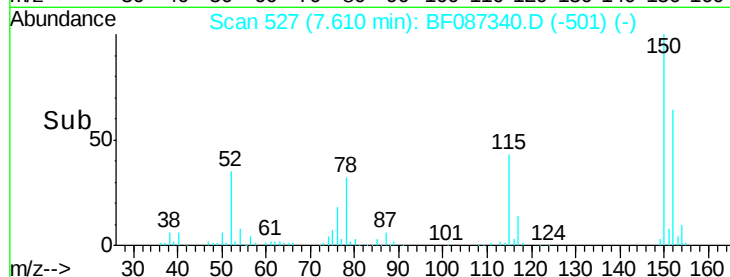



#5

2-Fluorophenol
Concen: 118.66 ng
RT: 5.53 min Scan# 345
Delta R.T. 0.01 min
Lab File: BF087340.D
Acq: 24 May 2016 14:02

Tgt Ion:112 Resp: 908341
Ion Ratio Lower Upper
112 100
64 71.5 52.1 78.1
63 39.9 25.7 38.5#

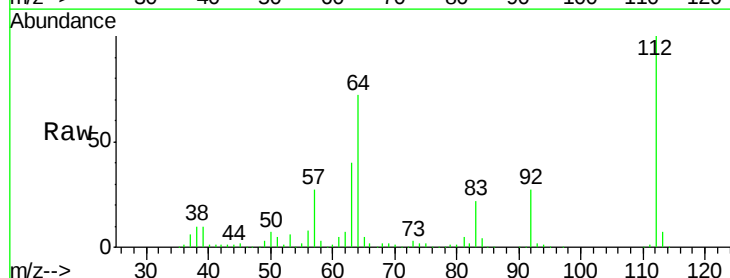

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

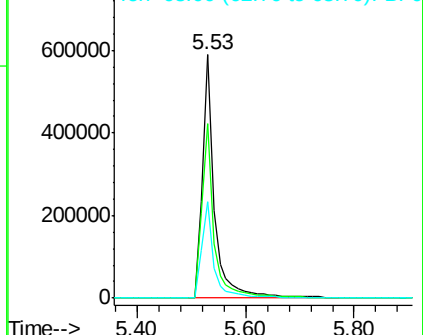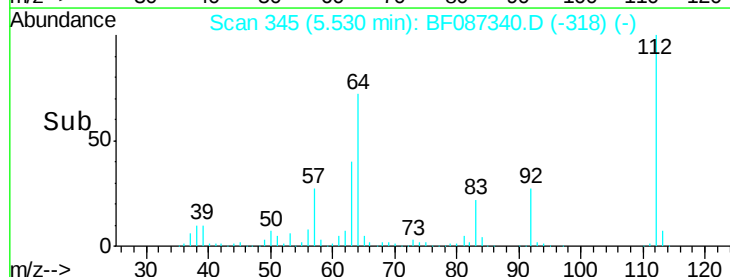



#7

Phenol-d6

Concen: 115.30 ng

RT: 7.15 min Scan# 487

Delta R.T. -0.01 min

Lab File: BF087340.D

Acq: 24 May 2016 14:02

Instrument :

BNA_F

ClientSampleId :

SB-06-COMP


Tgt Ion: 99 Resp: 1192627

Ion Ratio Lower Upper

99 100

42 29.3 13.6 20.4#




71 40.0 24.6 36.8#

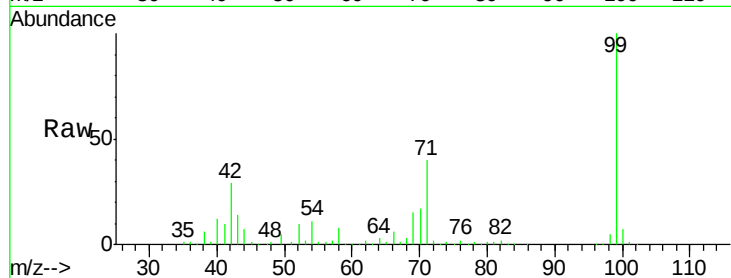

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

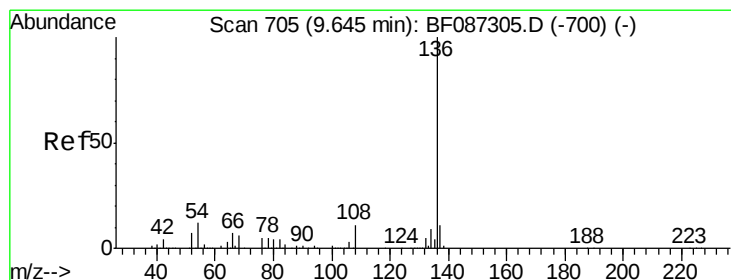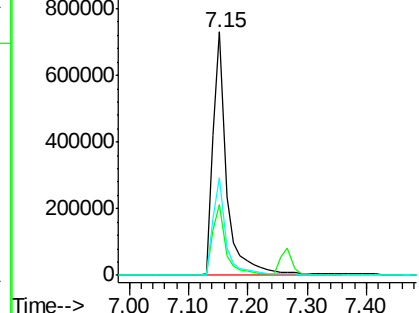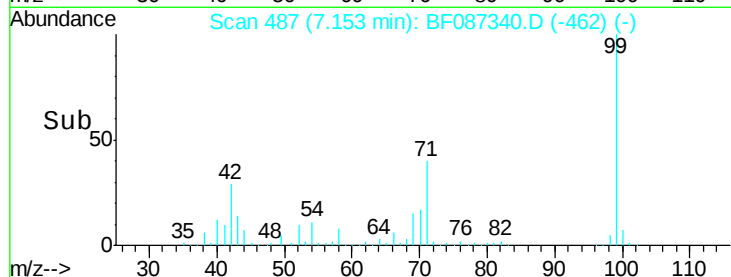

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 9.64 min Scan# 705

Delta R.T. 0.00 min

Lab File: BF087340.D

Acq: 24 May 2016 14:02

Tgt Ion: 136 Resp: 570161


Ion Ratio Lower Upper

136 100

137 10.6 8.8 13.2

54 10.4 5.0 7.4#

68 5.3 4.4 6.6


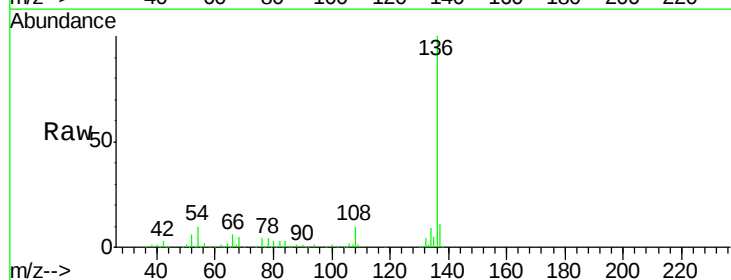


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0


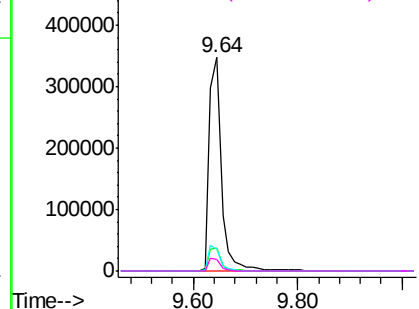
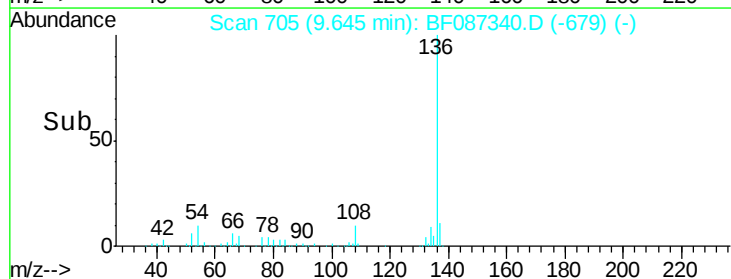




#23
Nitrobenzene-d5
Concen: 72.74 ng
RT: 8.52 min Scan# 607
Delta R.T. -0.01 min
Lab File: BF087340.D
Acq: 24 May 2016 14:02




Instrument :
BNA_F
ClientSampleId :
SB-06-COMP


Tgt Ion: 82 Resp: 822874
Ion Ratio Lower Upper
82 100
128 40.5 40.6 61.0#
54 68.7 38.1 57.1#

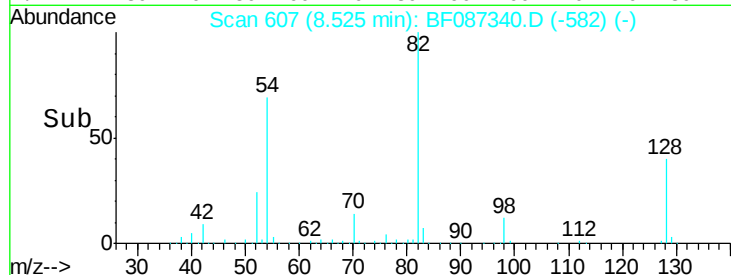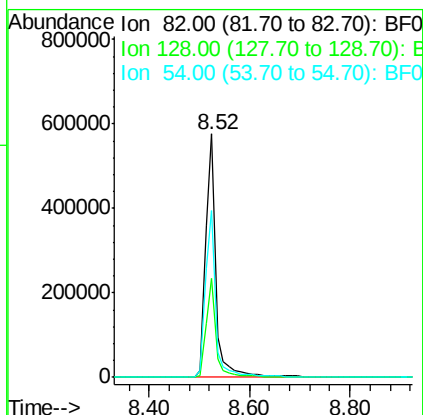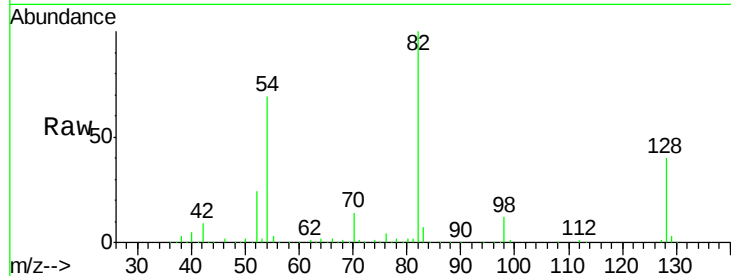

#38
Acenaphthene-d10
Concen: 20.00 ng
RT: 12.47 min Scan# 952
Delta R.T. -0.01 min
Lab File: BF087340.D
Acq: 24 May 2016 14:02

Tgt Ion: 164 Resp: 259079
Ion Ratio Lower Upper
164 100
162 103.8 82.8 124.2
160 47.0 36.9 55.3

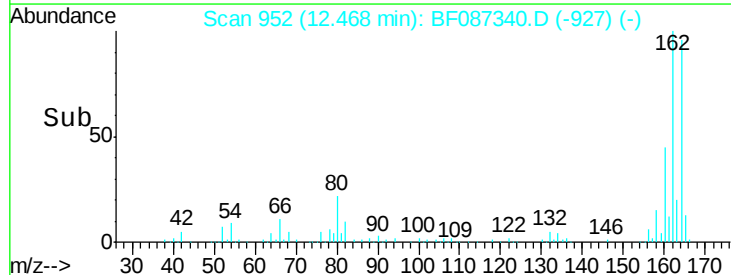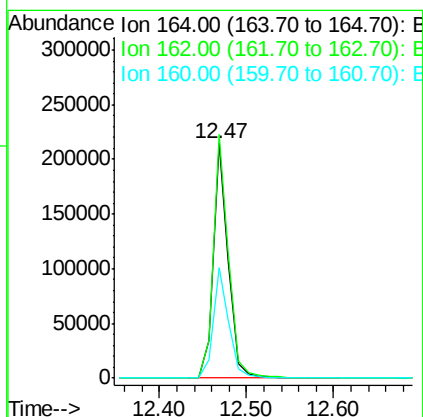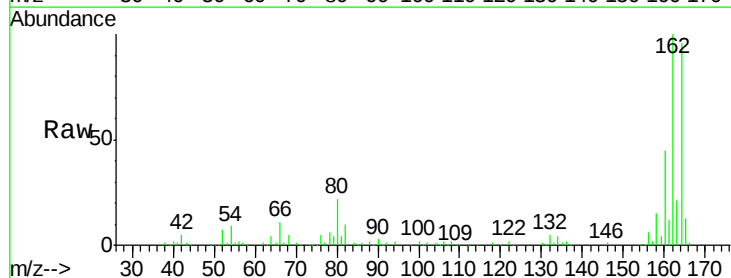


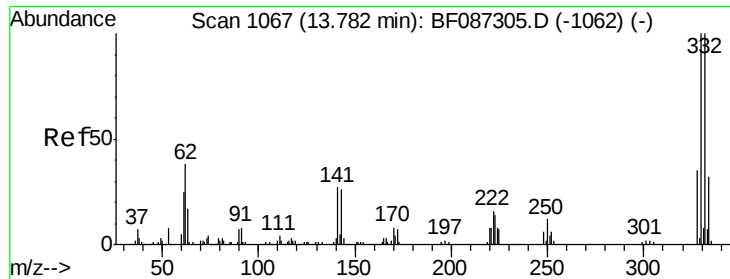

#41
 2,4,6-Tribromophenol
 Concen: 106.23 ng
 RT: 13.77 min Scan# 1066
 Delta R.T. -0.01 min
 Lab File: BF087340.D
 Acq: 24 May 2016 14:02

Instrument :
 BNA_F
 ClientSampleId :
 SB-06-COMP

Tgt Ion	Ratio	Lower	Upper
330	100		
332	96.3	79.0	118.4
141	42.2	31.2	46.8



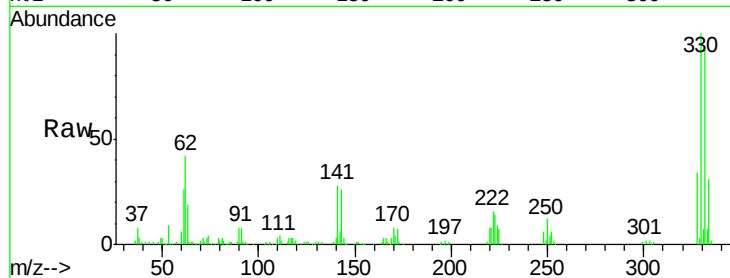


Abundance

Ion 329.80 (329.50 to 330.50): E


Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

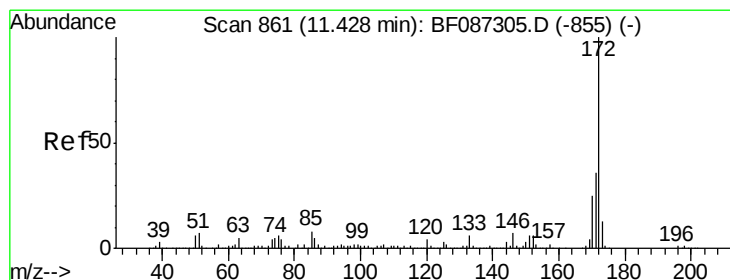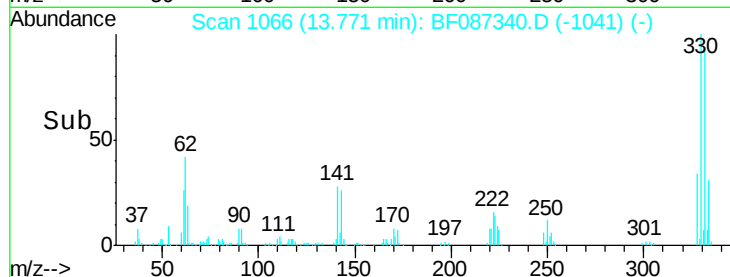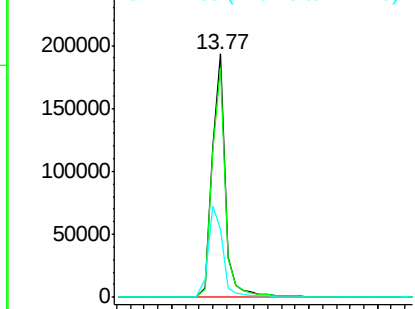

#44
 2-Fluorobiphenyl
 Concen: 73.68 ng
 RT: 11.42 min Scan# 860
 Delta R.T. -0.01 min
 Lab File: BF087340.D
 Acq: 24 May 2016 14:02

Tgt Ion	Ratio	Lower	Upper
172	100		
171	35.9	29.0	43.6
170	24.5	19.8	29.8


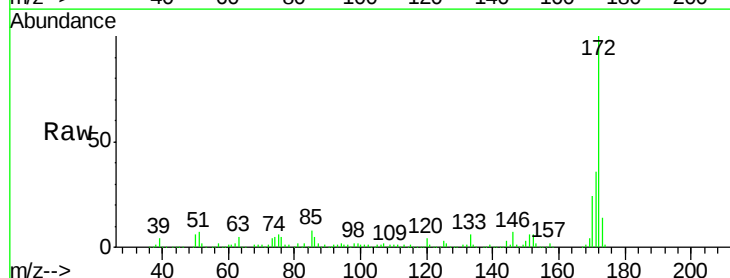



Abundance

Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E



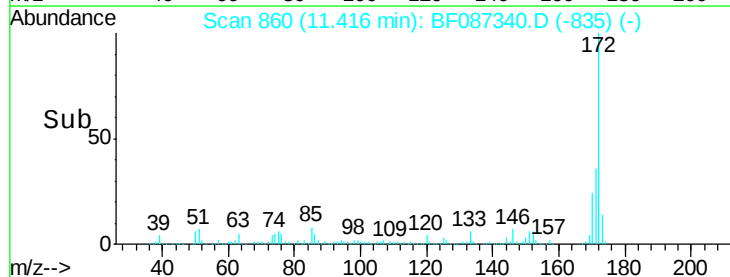
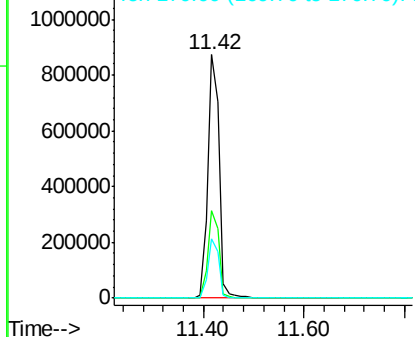


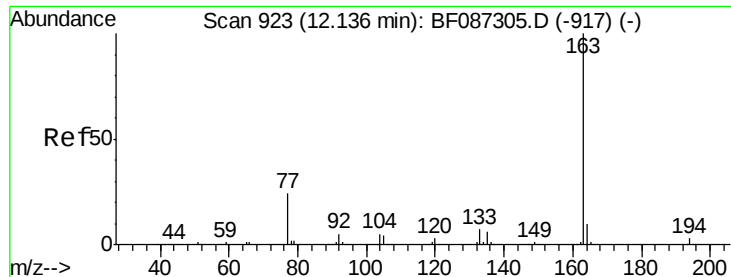

#49
Dimethylphthalate
Concen: 7.94 ng
RT: 12.11 min Scan# 921
Delta R.T. -0.02 min
Lab File: BF087340.D
Acq: 24 May 2016 14:02




Instrument :
BNA_F
ClientSampleId :
SB-06-COMP

Tgt Ion:163 Resp: 164688
Ion Ratio Lower Upper
163 100
194 3.4 2.6 4.0
164 9.7 8.2 12.4

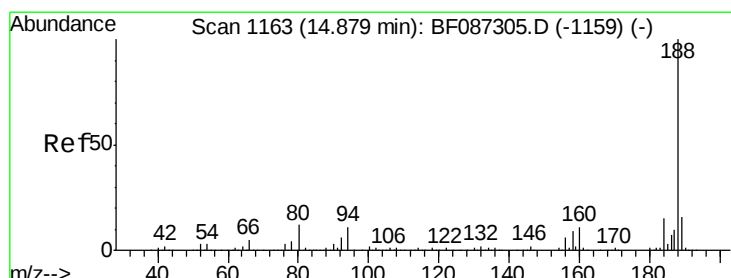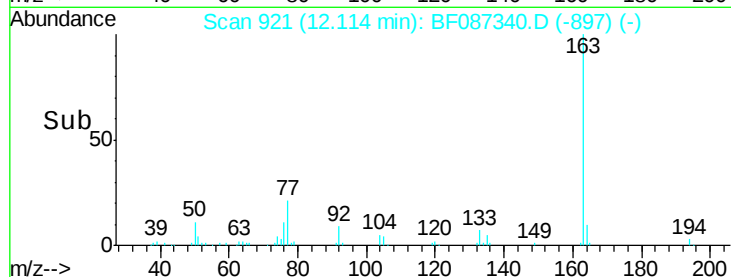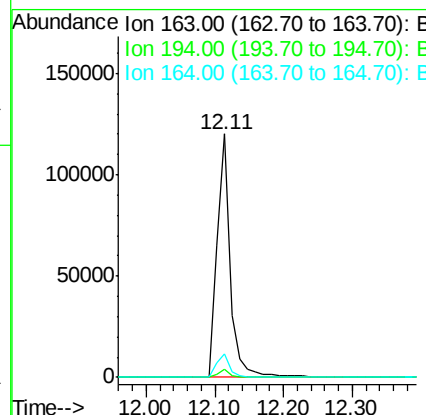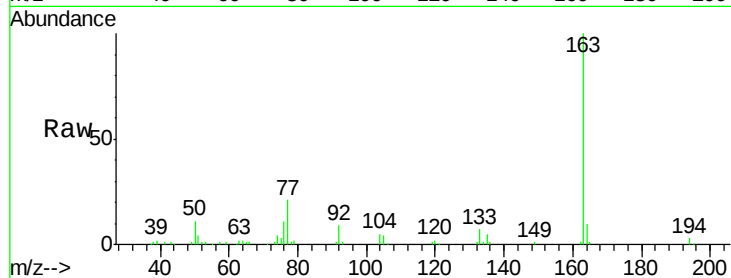

#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 14.88 min Scan# 1163
Delta R.T. 0.00 min
Lab File: BF087340.D
Acq: 24 May 2016 14:02

Tgt Ion:188 Resp: 462226
Ion Ratio Lower Upper
188 100
94 7.7 6.8 10.2
80 8.7 7.1 10.7

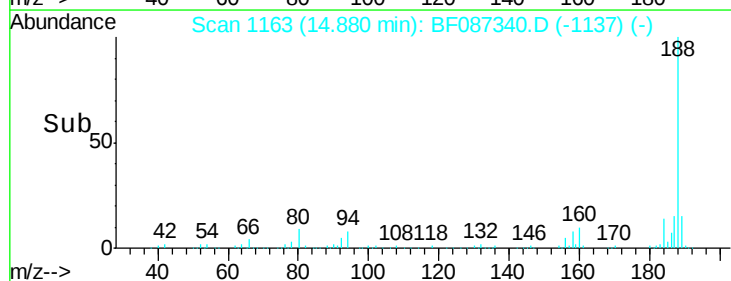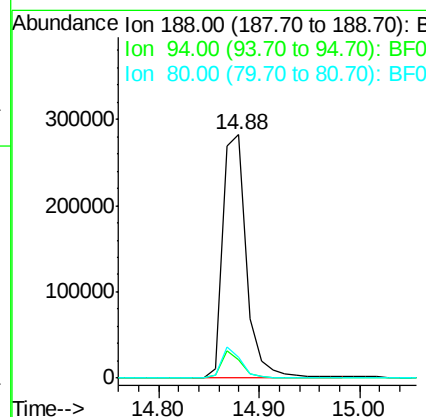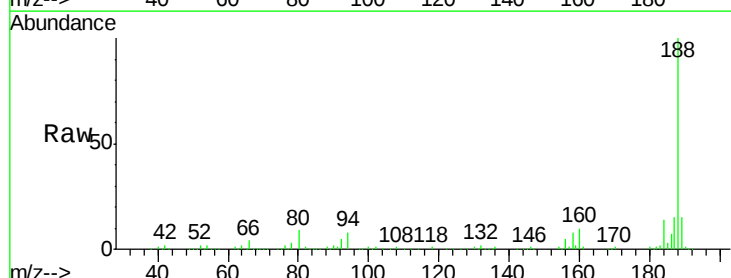



#75

Chrysene-d12

Concen: 20.00 ng

RT: 18.56 min Scan# 1485

Delta R.T. 0.00 min

Lab File: BF087340.D

Acq: 24 May 2016 14:02

Instrument :

BNA_F

ClientSampled :

SB-06-COMP


Tgt Ion:240 Resp: 315827

Ion Ratio Lower Upper

240 100

120 9.4 11.2 16.8#




236 26.4 21.2 31.8

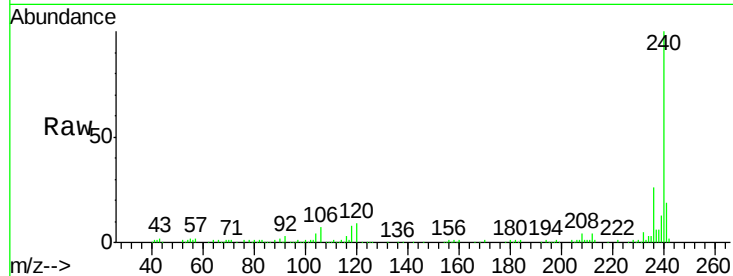

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

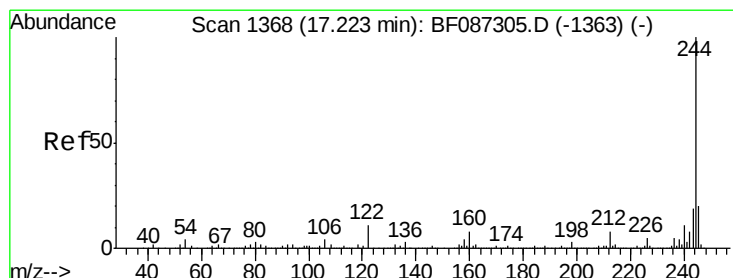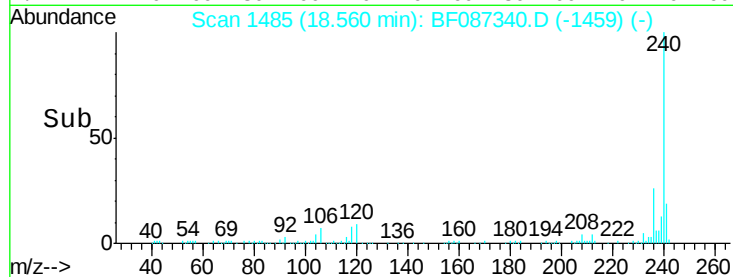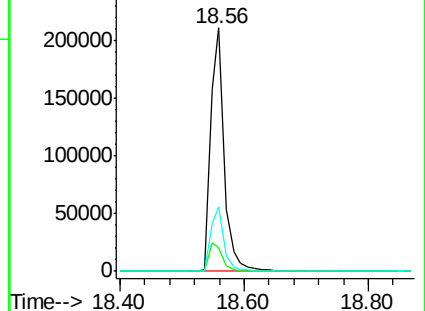

#78

Terphenyl-d14

Concen: 71.14 ng

RT: 17.21 min Scan# 1367

Delta R.T. -0.01 min

Lab File: BF087340.D

Acq: 24 May 2016 14:02


Tgt Ion:244 Resp: 1056889

Ion Ratio Lower Upper

244 100

212 8.0 6.2 9.2



122 12.8 12.0 18.0

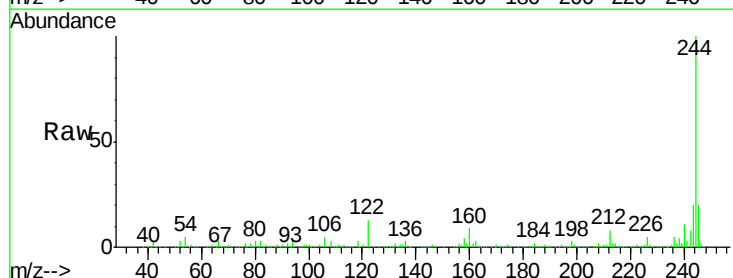


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

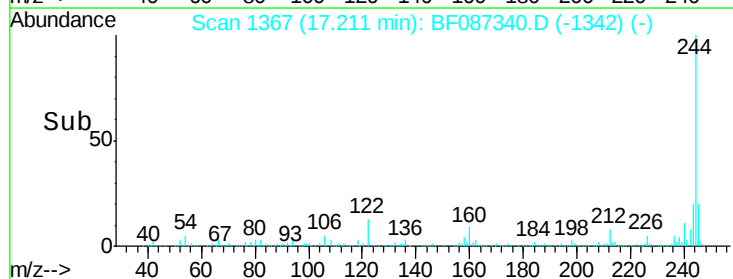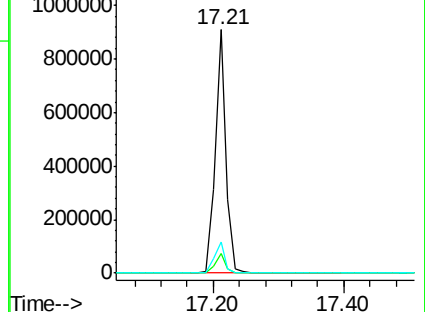

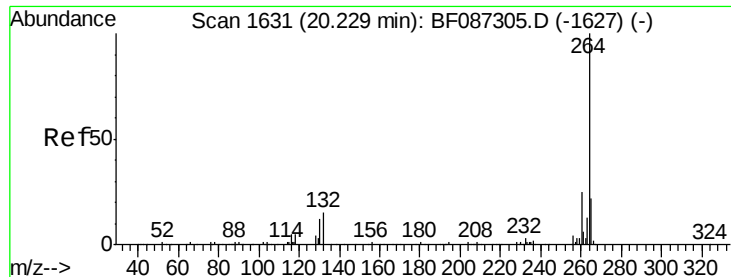

#86
Perylene-d12
Concen: 20.00 ng
RT: 20.22 min Scan# 1630
Delta R.T. -0.01 min
Lab File: BF087340.D
Acq: 24 May 2016 14:02

Instrument :
BNA_F
ClientSampleId :
SB-06-COMP

Tgt Ion	Ratio	Lower	Upper
264	100		
260	24.6	19.5	29.3
265	21.6	17.3	25.9

