

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF052316\
 Data File : BF087317.D
 Acq On : 24 May 2016 00:32
 Operator : UM/SJ
 Sample : PB90819BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB90819BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052316.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.678	7	8	31	rVB	1100318	2161682	47.51%	5.725%
2	4.924	290	292	308	rBV	95711	347813	7.64%	0.921%
3	5.530	342	345	364	rBV	2347602	3758264	82.60%	9.953%
4	7.142	483	486	494	rBV	2231595	3862675	84.89%	10.229%
5	7.268	494	497	503	rVB	2696648	3989553	87.68%	10.565%
6	7.610	525	527	536	rVB	625541	854739	18.78%	2.264%
7	7.839	545	547	558	rBV	1824618	3037548	66.76%	8.044%
8	8.525	604	607	609	rBV	1509563	2365400	51.98%	6.264%
9	9.645	702	705	724	rBV	661376	1113596	24.47%	2.949%
10	11.416	856	860	863	rBV	2980616	4314876	94.83%	11.427%
11	12.468	950	952	966	rBV	889231	1226220	26.95%	3.247%
12	13.760	1062	1065	1092	rBV	1568374	2796854	61.47%	7.407%
13	14.880	1160	1163	1174	rBV	755995	1297171	28.51%	3.435%
14	17.211	1364	1367	1370	rBV	3336956	4550209	100.00%	12.050%
15	18.560	1482	1485	1497	rBV	671589	1153715	25.36%	3.055%
16	20.217	1628	1630	1647	rBV	570825	930873	20.46%	2.465%




Sum of corrected areas: 37761188

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF052316\
Data File : BF087317.D
Acq On : 24 May 2016 00:32
Operator : UM/SJ
Sample : PB90819BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB90819BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

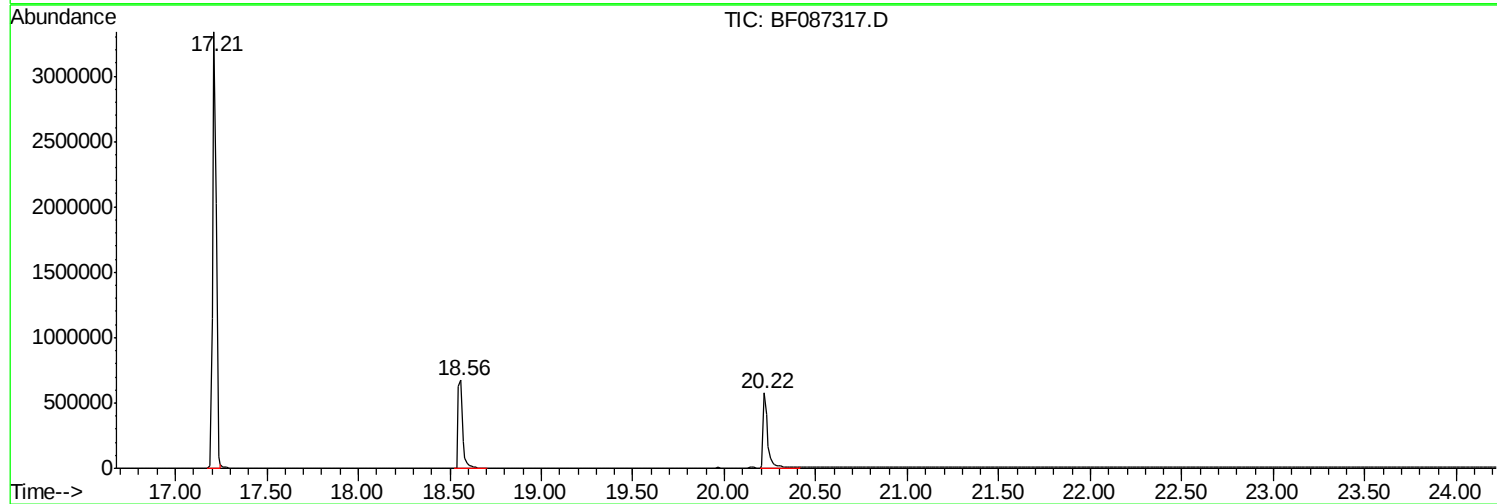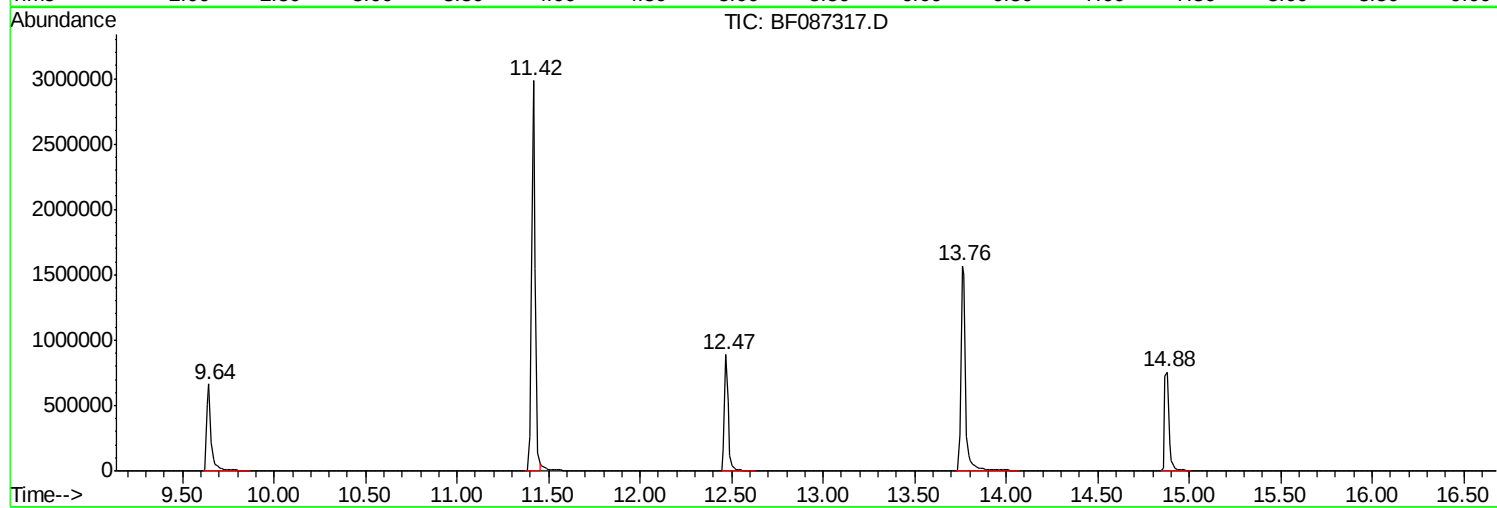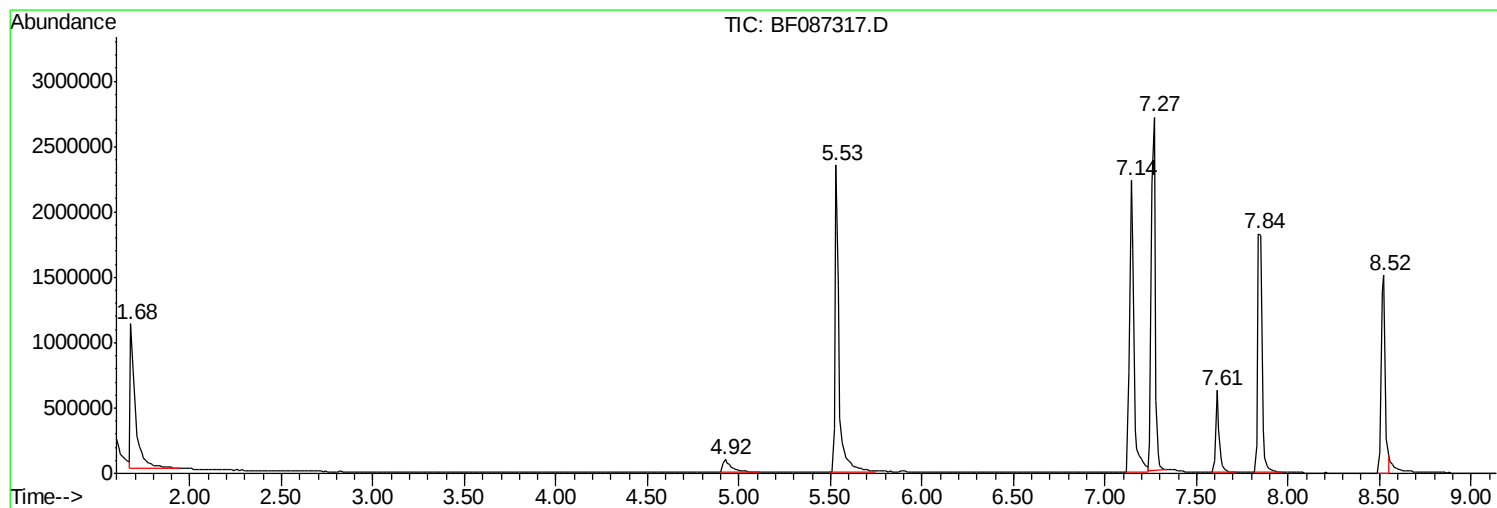

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF052316\
Data File : BF087317.D
Acq On : 24 May 2016 00:32
Operator : UM/SJ
Sample : PB90819BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB90819BL










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 4

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.92	8.14 ng	347813	1,4-Dichlorobenzene-d4	7.61

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	64
2		Acetic acid, 1,1-dimethylethyl e...	116	C6H12O2	000540-88-5	23
3		1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	10
4		Diacetamide	101	C4H7NO2	000625-77-4	9
5		Butane	58	C4H10	000106-97-8	9

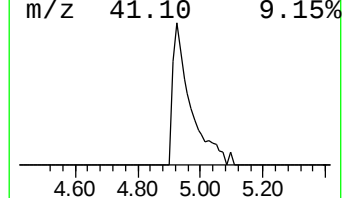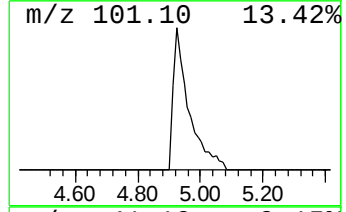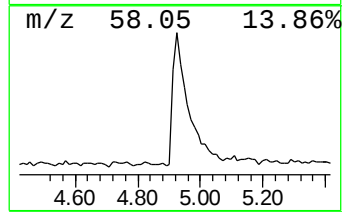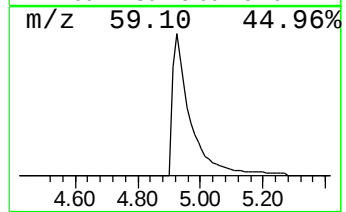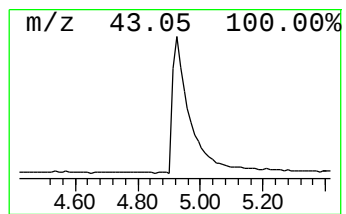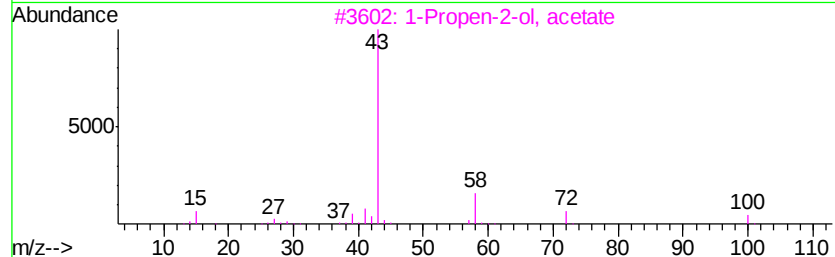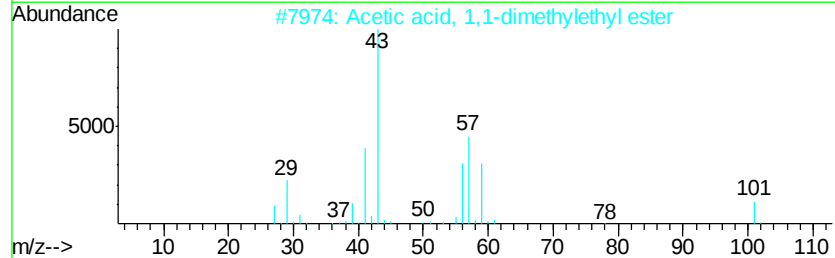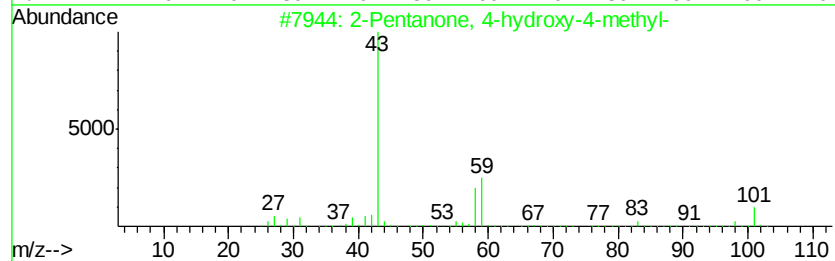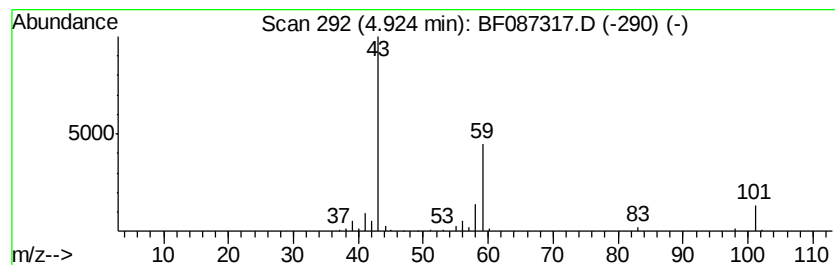

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF052316\
Data File : BF087317.D
Acq On : 24 May 2016 00:32
Operator : UM/SJ
Sample : PB90819BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB90819BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	4.92	8.1 ng		347813	1	7.61	854739	20.0