

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF052316\
 Data File : BF087324.D
 Acq On : 24 May 2016 5:03
 Operator : UM/SJ
 Sample : H3218-03
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 E-2GW

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052316.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.690	7	9	66	rVB	3680184	9754062	100.00%	23.159%
2	5.530	342	345	366	rBV	807543	1920889	19.69%	4.561%
3	7.153	484	487	494	rBV	699930	1335889	13.70%	3.172%
4	7.267	494	497	517	rVB	2405986	3667052	37.60%	8.707%
5	7.610	525	527	537	rVB	590634	836420	8.58%	1.986%
6	7.850	545	548	559	rBV	2200073	3244976	33.27%	7.704%
7	8.525	604	607	624	rBV	2090250	2920644	29.94%	6.934%
8	9.645	702	705	711	rBV	712579	1055711	10.82%	2.507%
9	11.428	857	861	863	rBV	3196601	5060167	51.88%	12.014%
10	12.468	949	952	960	rBV	850539	1246128	12.78%	2.959%
11	13.771	1062	1066	1079	rBV	2243644	3225003	33.06%	7.657%
12	14.880	1160	1163	1172	rVB	771576	1214210	12.45%	2.883%
13	17.211	1364	1367	1370	rBV	3052270	4848454	49.71%	11.511%
14	18.560	1483	1485	1494	rVB	701460	1049023	10.75%	2.491%
15	20.217	1628	1630	1636	rBV	412445	739762	7.58%	1.756%


Sum of corrected areas: 42118390

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF052316\
Data File : BF087324.D
Acq On : 24 May 2016 5:03
Operator : UM/SJ
Sample : H3218-03
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
E-2GW

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

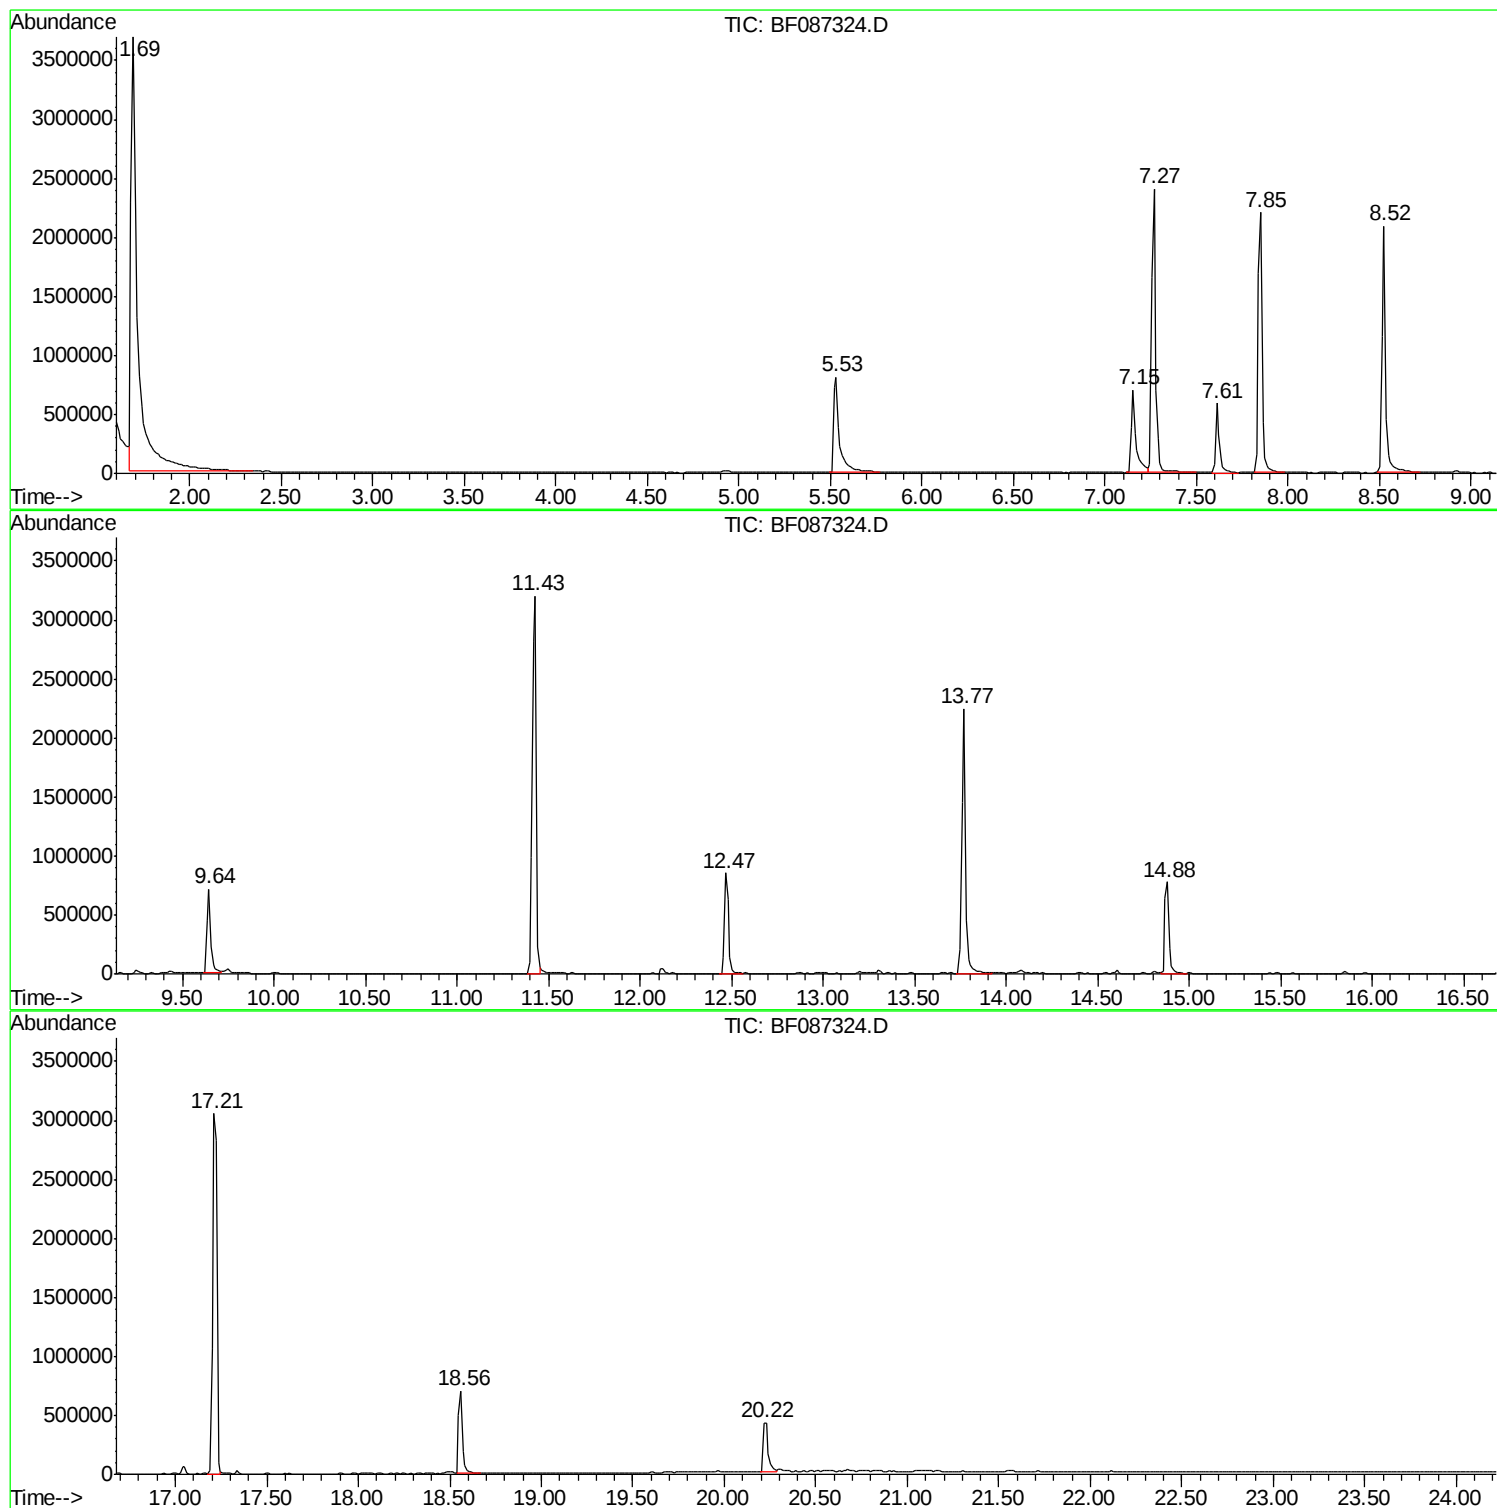

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF052316\
Data File : BF087324.D
Acq On : 24 May 2016 5:03
Operator : UM/SJ
Sample : H3218-03
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
E-2GW










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown7.27 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.27	87.68 ng	3667050	1,4-Dichlorobenzene-d4	7.61

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	22
3		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	12
4		(5-METHYL-2-PYRIDYL)ACETONITRILE	132	C8H8N2	1000241-93-9	10
5		Benzene, 1,2,4-trifluoro-	132	C6H3F3	000367-23-7	9

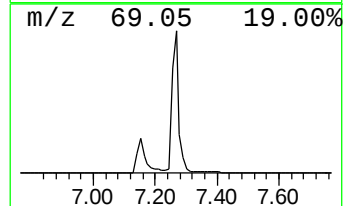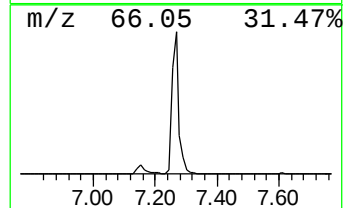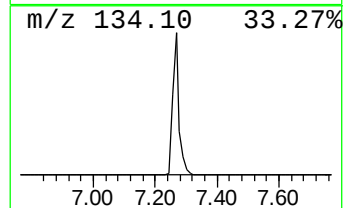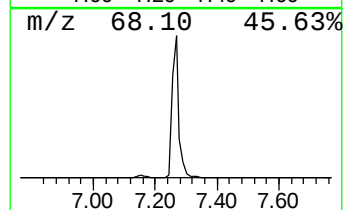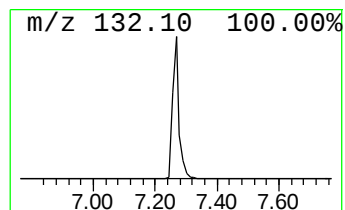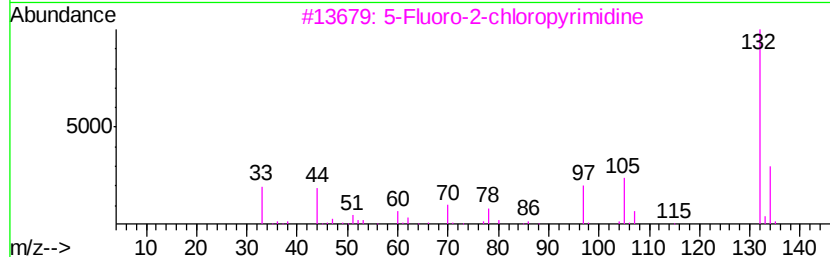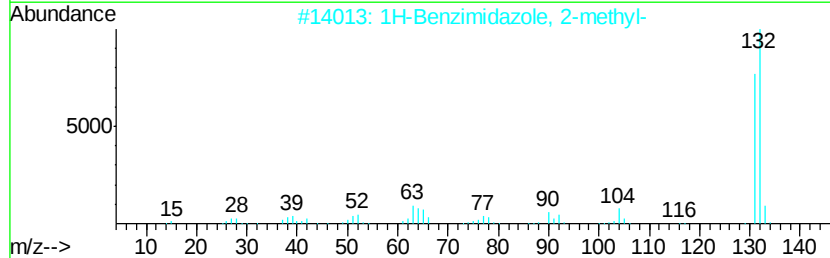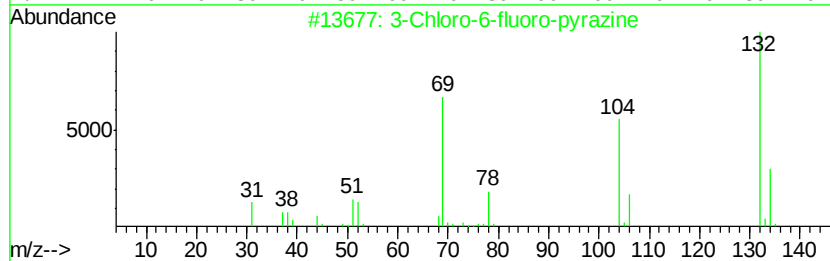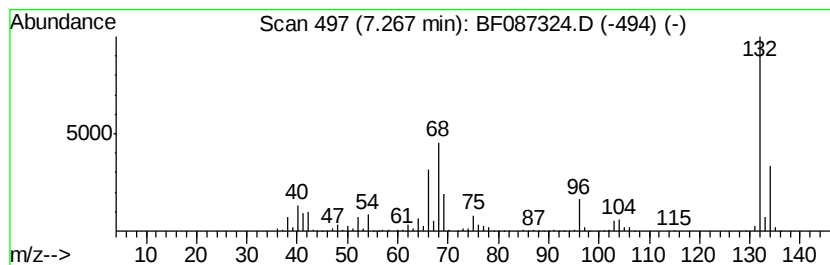

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF052316\
Data File : BF087324.D
Acq On : 24 May 2016 5:03
Operator : UM/SJ
Sample : H3218-03
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
E-2GW

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---			
					#	RT	Resp	Conc
unknown7.27	7.27	87.7	ng	3667050	1	7.61	836420	20.0