


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF052316\
 Data File : BF087300.D
 Acq On : 23 May 2016 14:02
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052316.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue May 24 01:40:43 2016

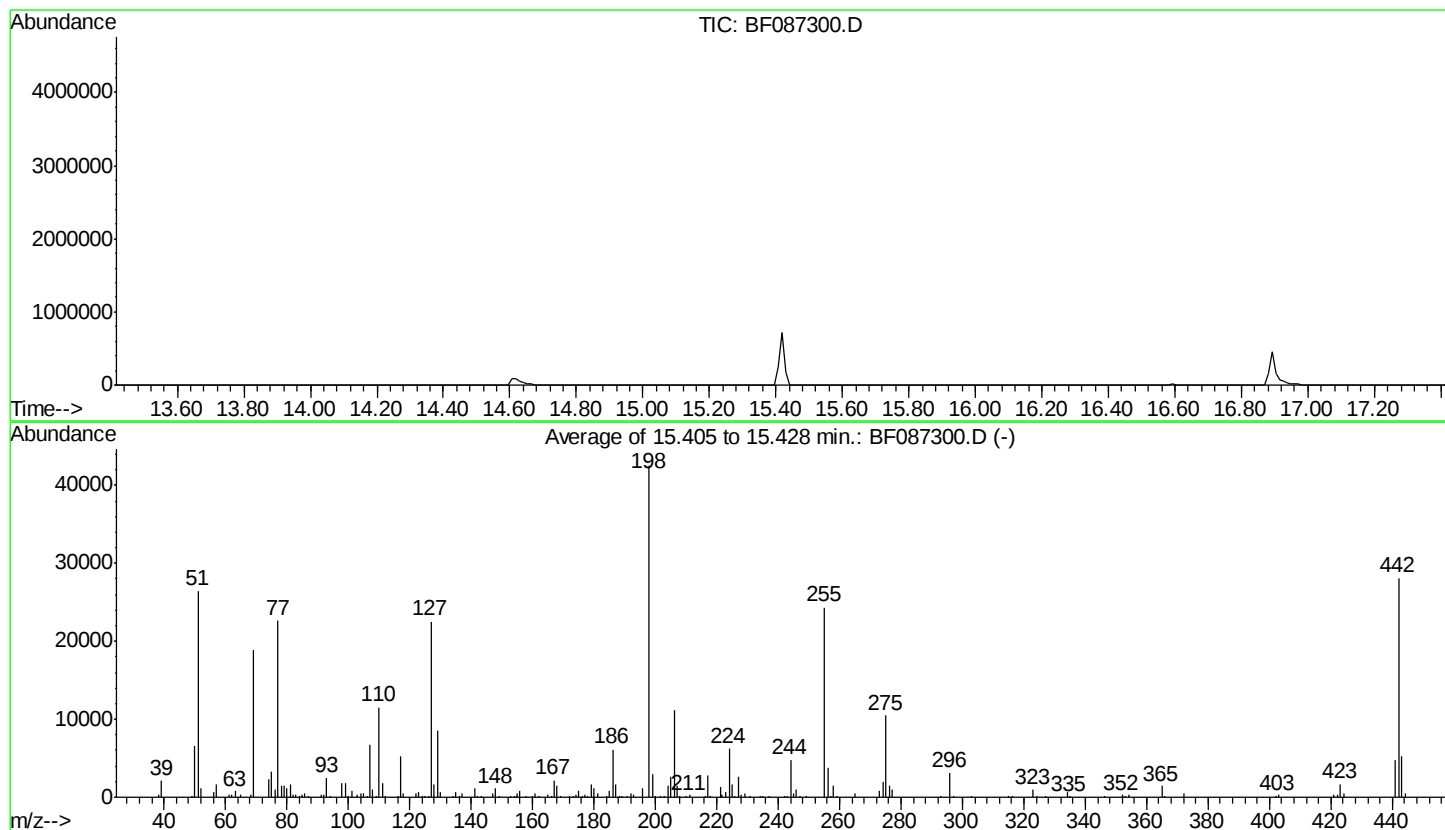

AutoFind: Scans 1209, 1210, 1211; Background Corrected with Scan 1205

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	62.2	26458	PASS
68	69	0.00	2	1.8	337	PASS
69	198	0.00	100	44.4	18863	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	53.0	22561	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	42528	PASS
199	198	5	9	6.9	2915	PASS
275	198	10	60	24.7	10507	PASS
365	198	1	100	3.4	1425	PASS
441	442	0.01	24	16.8	4722	PASS
442	198	50	100	66.1	28123	PASS
443	442	15	24	18.9	5318	PASS