


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF052316\
Data File : BF087320.D
Acq On : 24 May 2016 2:48
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052316.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue May 24 01:40:43 2016

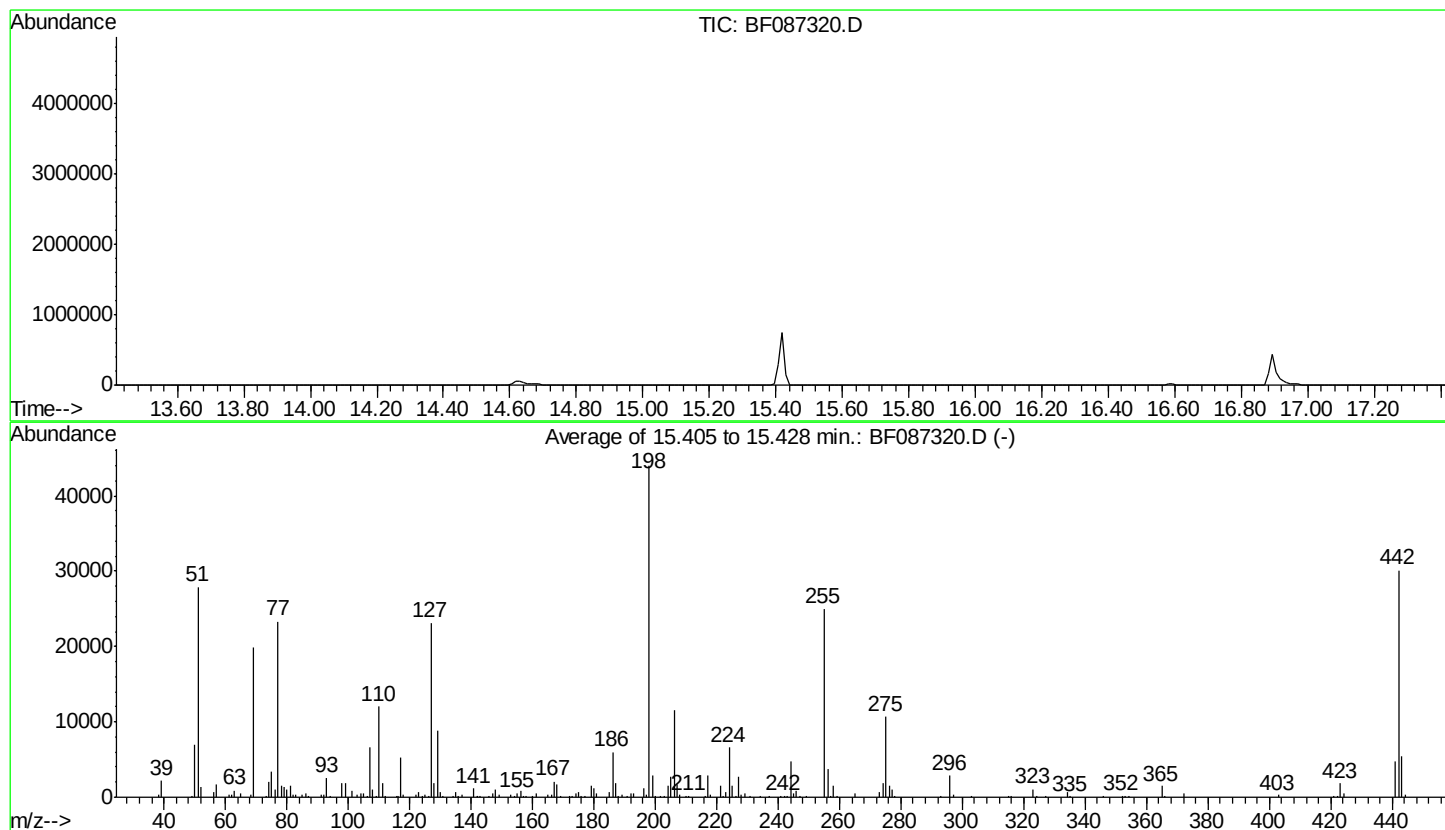

AutoFind: Scans 1209, 1210, 1211; Background Corrected with Scan 1205

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	63.4	27912	PASS
68	69	0.00	2	1.7	348	PASS
69	198	0.00	100	45.3	19933	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.6	23167	PASS
197	198	0.00	2	0.9	397	PASS
198	198	100	100	100.0	44017	PASS
199	198	5	9	6.7	2937	PASS
275	198	10	60	24.3	10690	PASS
365	198	1	100	3.4	1492	PASS
441	442	0.01	24	15.8	4749	PASS
442	198	50	100	68.5	30134	PASS
443	442	15	24	18.2	5492	PASS