

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF052317\
 Data File : BF095359.D
 Acq On : 23 May 2017 19:25
 Operator : SJ/MA
 Sample : I3251-01
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PTS-02

Quant Time: May 24 03:06:01 2017
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu May 18 17:07:53 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.75	152	107728	20.00	ng	-0.01
21) Naphthalene-d8	9.77	136	422280	20.00	ng	-0.01
38) Acenaphthene-d10	12.61	164	202056	20.00	ng	-0.01
63) Phenanthrene-d10	15.01	188	328453	20.00	ng	-0.01
75) Chrysene-d12	18.68	240	189647	20.00	ng	-0.01
86) Perylene-d12	20.36	264	193969	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.72	112	729400	112.88	ng	-0.02
7) Phenol-d6	7.30	99	909129	117.26	ng	-0.02
23) Nitrobenzene-d5	8.65	82	520960	77.79	ng	-0.02
41) 2,4,6-Tribromophenol	13.90	330	170684	103.15	ng	-0.02
44) 2-Fluorobiphenyl	11.54	172	938737	66.87	ng	-0.02
78) Terphenyl-d14	17.32	244	525765	61.06	ng	-0.02
Target Compounds						
49) Dimethylphthalate	12.25	163	140845	8.49	ng	Qvalue 100

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF052317\
Data File : BF095359.D
Acq On : 23 May 2017 19:25
Operator : SJ/MA
Sample : I3251-01
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PTS-02

Quant Time: May 24 03:06:01 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 18 17:07:53 2017
Response via : Initial Calibration

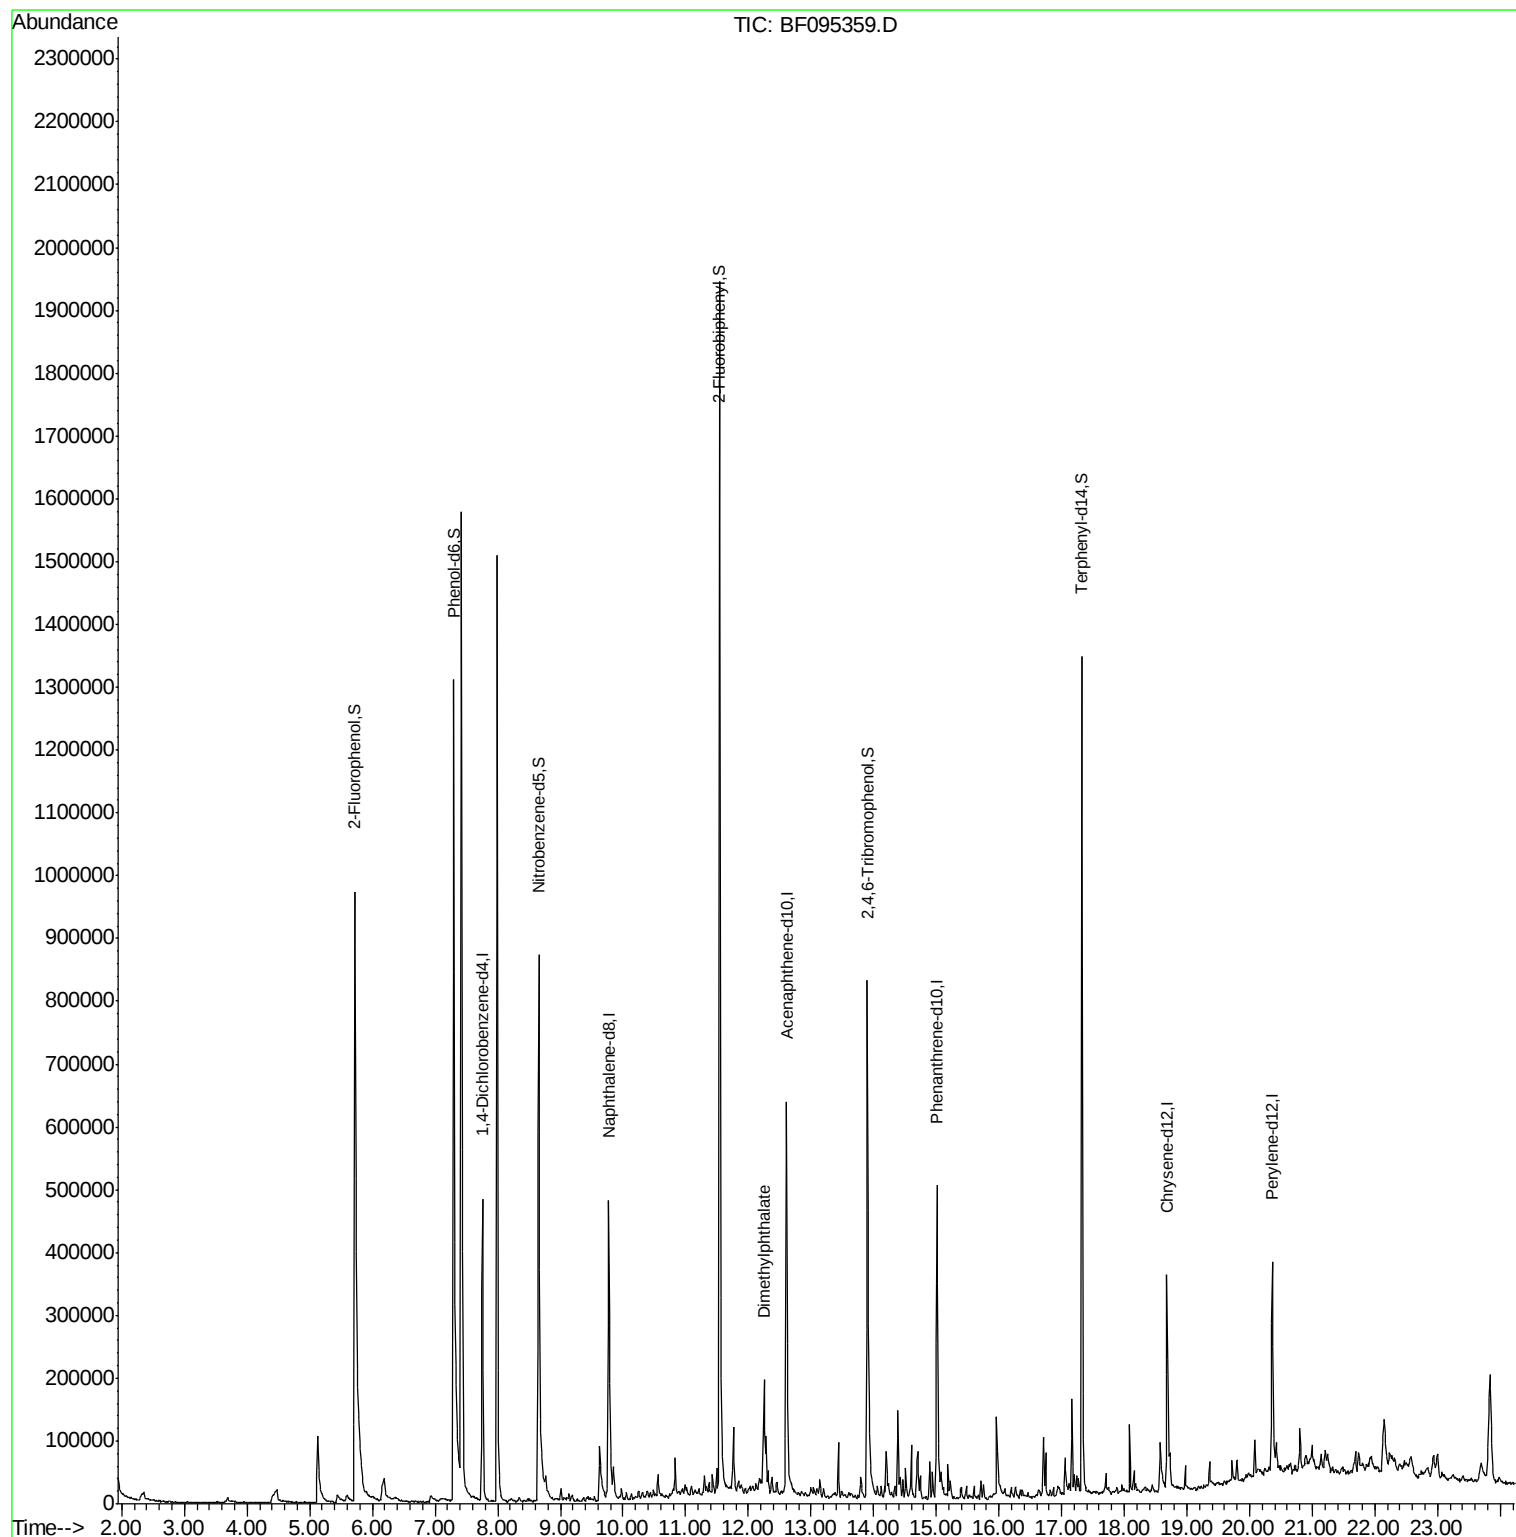




#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 7.75 min Scan# 989
Delta R.T. -0.01 min
Lab File: BF095359.D
Acq: 23 May 2017 19:25

Instrument :
BNA_F
ClientSampleId :
PTS-02

Tgt Ion:152 Resp: 107728
Ion Ratio Lower Upper
152 100
150 158.5 126.2 189.2
115 59.2 52.2 78.2

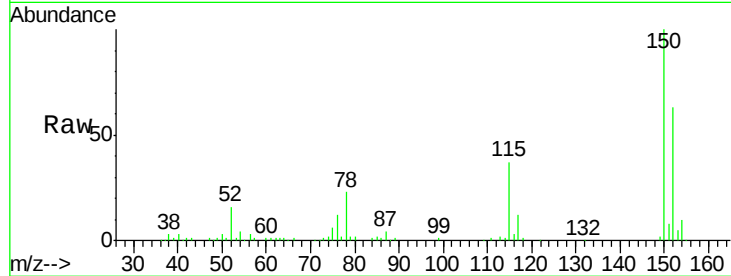


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

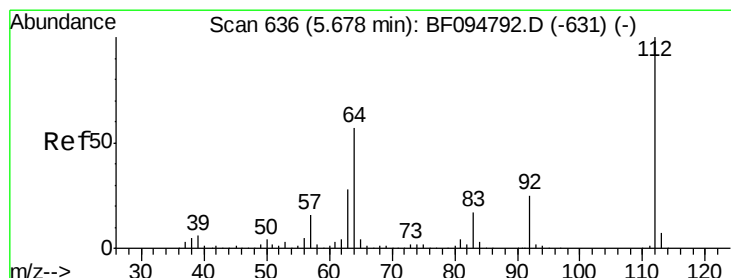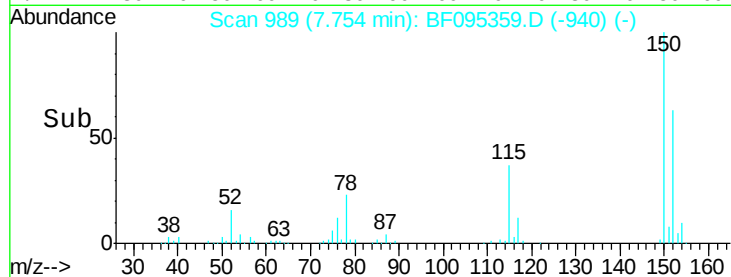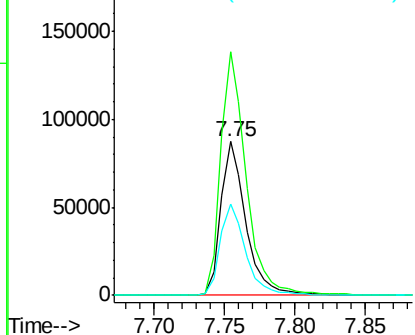



#5


2-Fluorophenol
Concen: 112.88 ng
RT: 5.72 min Scan# 643
Delta R.T. -0.02 min
Lab File: BF095359.D
Acq: 23 May 2017 19:25

Tgt Ion:112 Resp: 729400
Ion Ratio Lower Upper
112 100
64 55.4 46.0 69.0
63 26.2 23.4 35.0

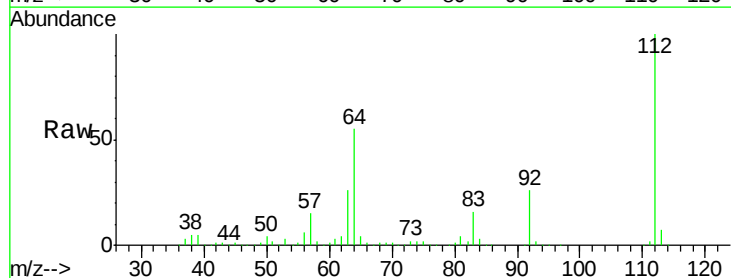

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

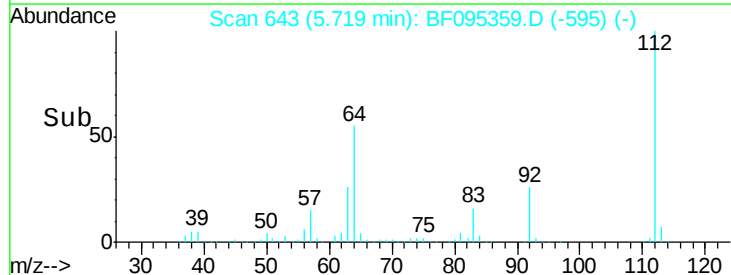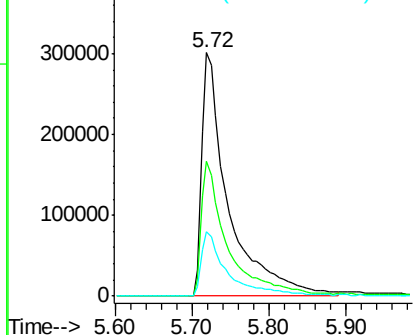

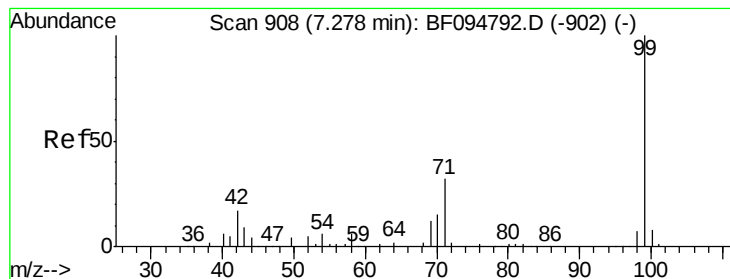

#7

Phenol-d6

Concen: 117.26 ng

RT: 7.30 min Scan# 911

Delta R.T. -0.02 min

Lab File: BF095359.D

Acq: 23 May 2017 19:25

Instrument :

BNA_F

ClientSampleId :

PTS-02


Tgt Ion: 99 Resp: 909129

Ion Ratio Lower Upper

99 100

42 16.2 13.5 20.3




71 32.1 24.5 36.7

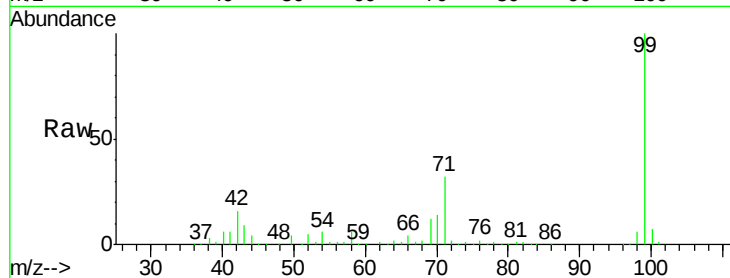

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

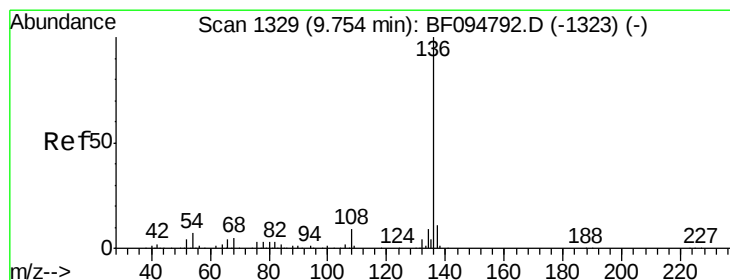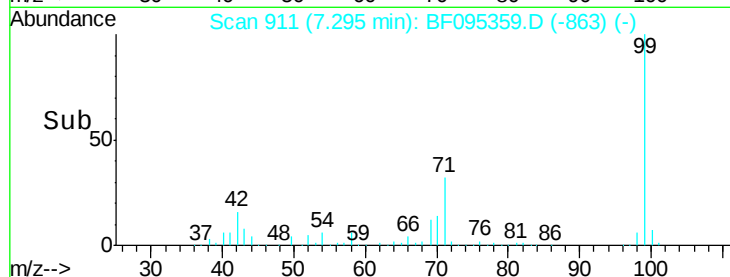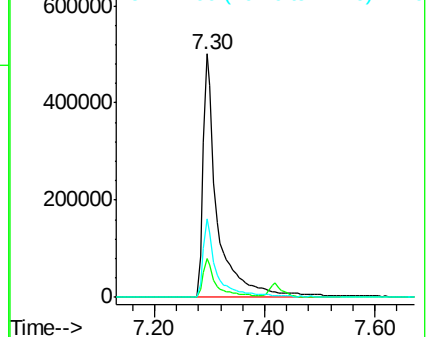

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 9.77 min Scan# 1332

Delta R.T. -0.01 min

Lab File: BF095359.D

Acq: 23 May 2017 19:25

Tgt Ion: 136 Resp: 422280


Ion Ratio Lower Upper

136 100

137 10.8 8.5 12.7

54 7.0 4.9 7.3

68 6.0 4.1 6.1


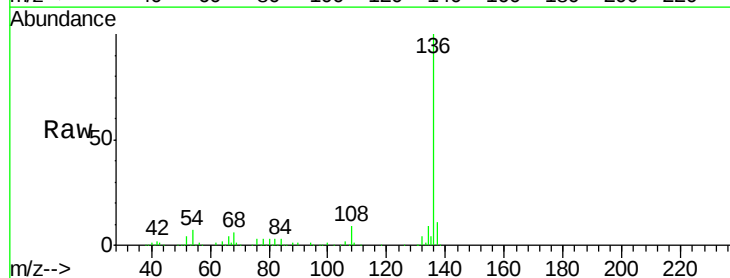



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

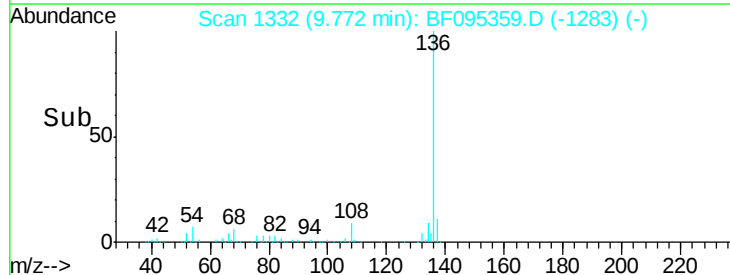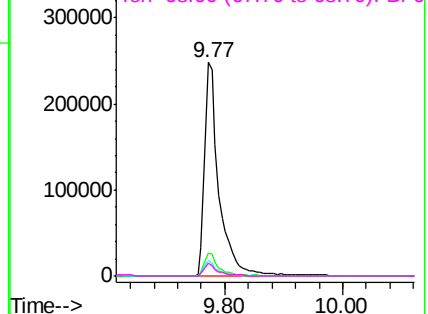

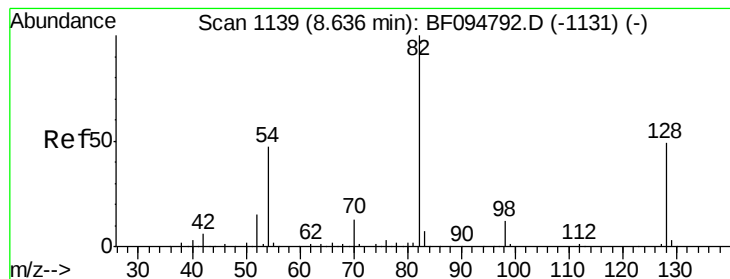

#23

Nitrobenzene-d5

Concen: 77.79 ng

RT: 8.65 min Scan# 1142

Delta R.T. -0.02 min

Lab File: BF095359.D

Acq: 23 May 2017 19:25

Instrument :

BNA_F

ClientSampled :

PTS-02


Tgt Ion: 82 Resp: 520960

Ion Ratio Lower Upper

82 100

128 47.2 34.0 51.0




54 46.8 42.2 63.2

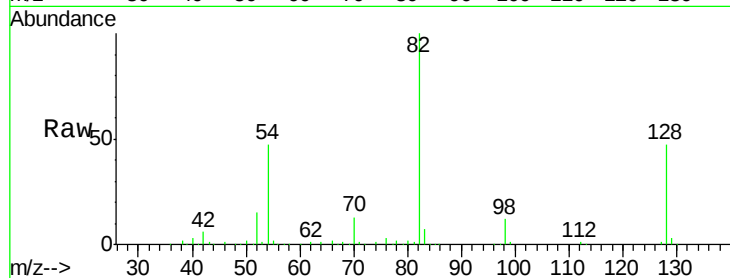

Abundance Ion 82.00 (81.70 to 82.70): BF0

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BF0

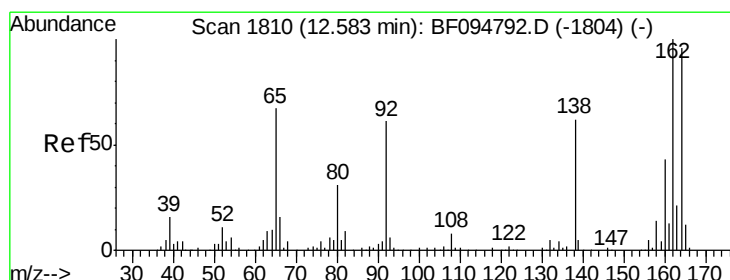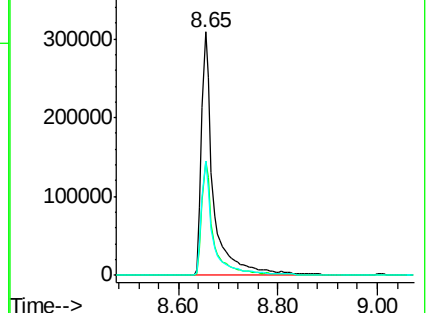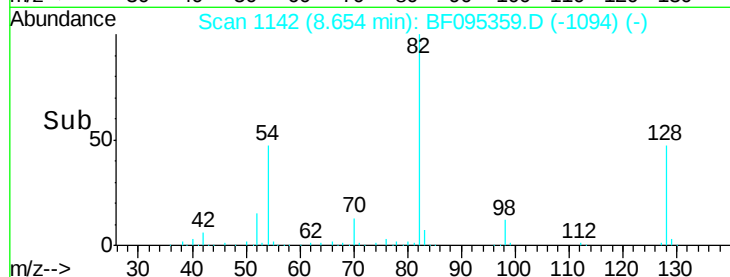

#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 12.61 min Scan# 1814

Delta R.T. -0.01 min

Lab File: BF095359.D

Acq: 23 May 2017 19:25


Tgt Ion: 164 Resp: 202056

Ion Ratio Lower Upper

164 100

162 102.8 82.6 123.8



160 44.8 36.2 54.2

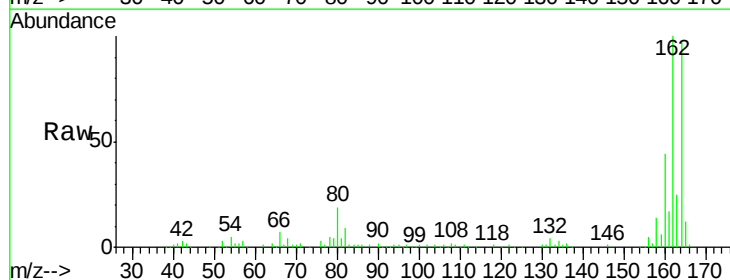


Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

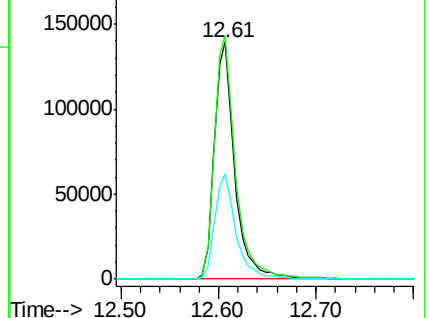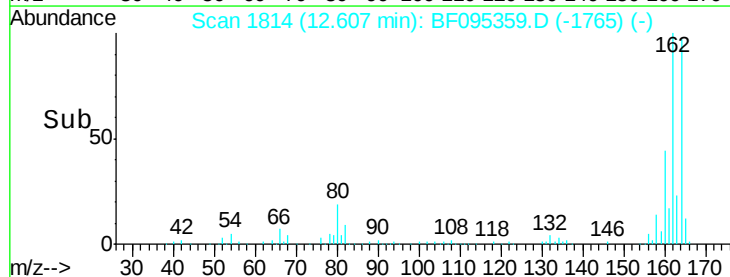


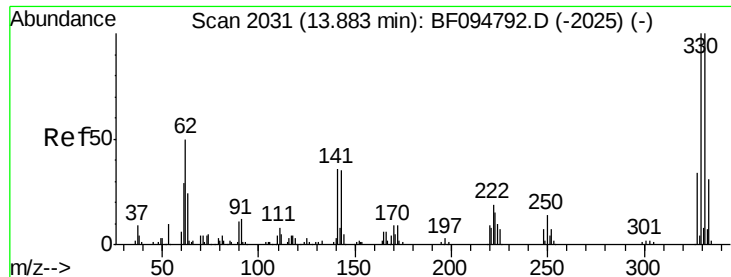




#41
 2,4,6-Tribromophenol
 Concen: 103.15 ng
 RT: 13.90 min Scan# 2034
 Delta R.T. -0.02 min
 Lab File: BF095359.D
 Acq: 23 May 2017 19:25

Instrument :
 BNA_F
 ClientSampleId :
 PTS-02

Tgt Ion: 330 Resp: 170684
 Ion Ratio Lower Upper
 330 100
 332 96.5 76.6 115.0
 141 38.7 31.4 47.2

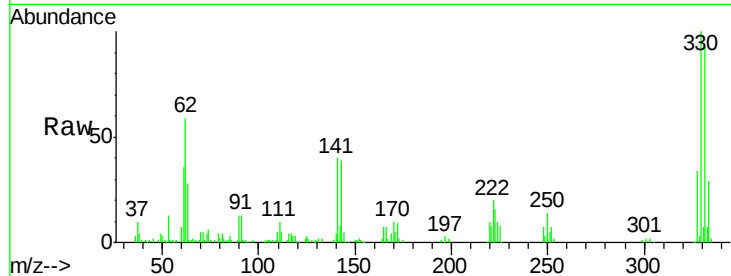


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

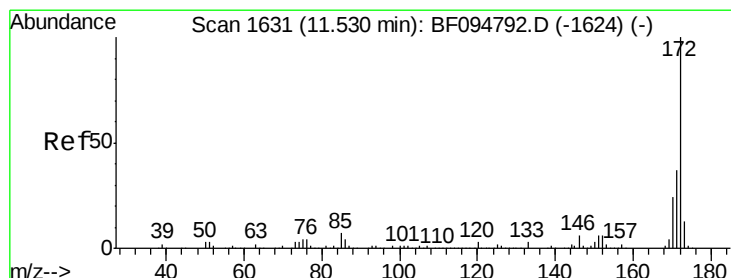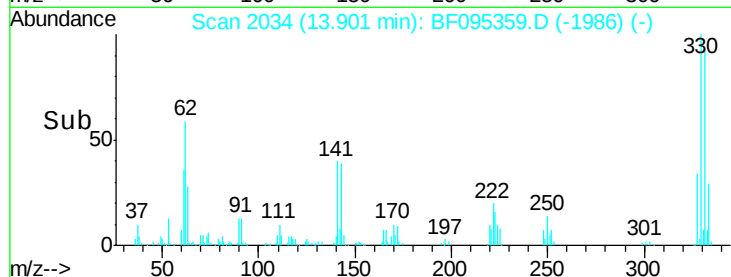
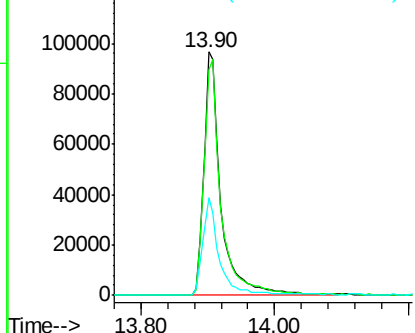


#44
 2-Fluorobiphenyl
 Concen: 66.87 ng
 RT: 11.54 min Scan# 1633
 Delta R.T. -0.02 min
 Lab File: BF095359.D
 Acq: 23 May 2017 19:25

Tgt Ion: 172 Resp: 938737
 Ion Ratio Lower Upper
 172 100
 171 35.5 29.6 44.4
 170 23.7 19.8 29.8

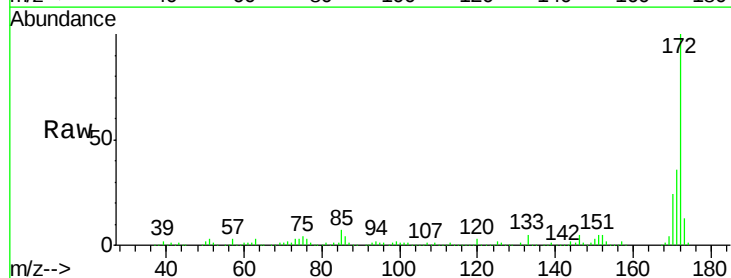

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

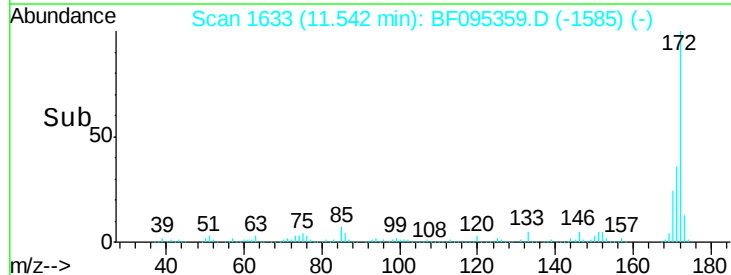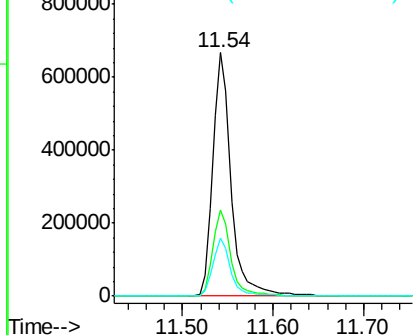



#49

Dimethylphthalate

Concen: 8.49 ng

RT: 12.25 min Scan# 1753

Delta R.T. -0.01 min

Lab File: BF095359.D

Acq: 23 May 2017 19:25

Instrument :

BNA_F

ClientSampleId :

PTS-02


Tgt Ion:163 Resp: 140845

Ion Ratio Lower Upper

163 100

194 3.4 2.6 4.0




164 10.5 8.4 12.6

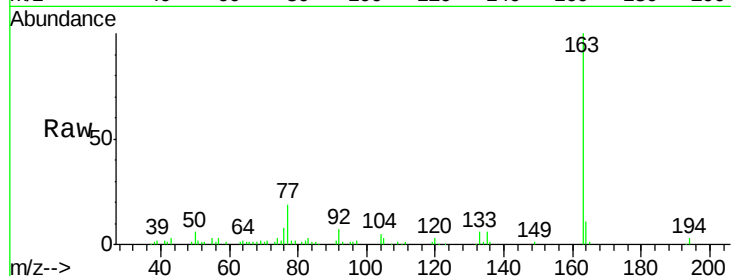

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

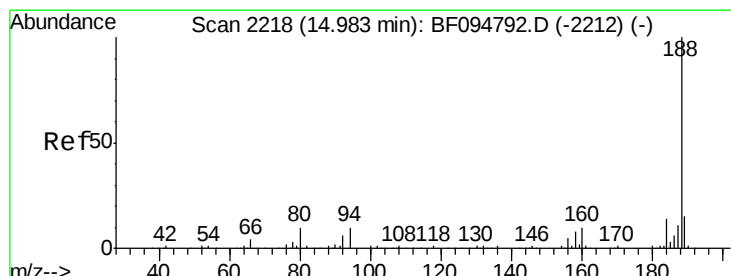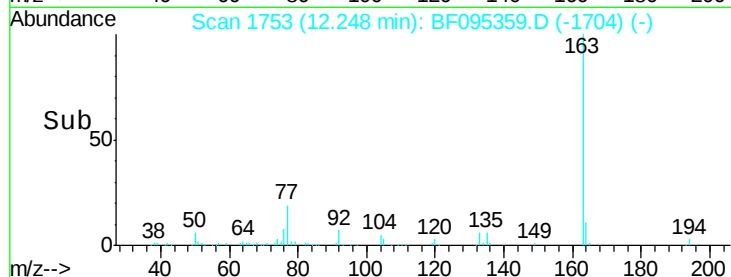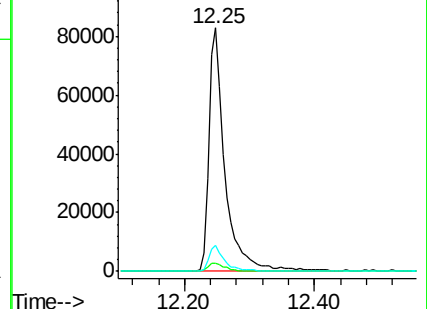

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 15.01 min Scan# 2223

Delta R.T. -0.01 min

Lab File: BF095359.D

Acq: 23 May 2017 19:25


Tgt Ion:188 Resp: 328453

Ion Ratio Lower Upper

188 100

94 9.8 9.4 14.2



80 11.0 10.2 15.2

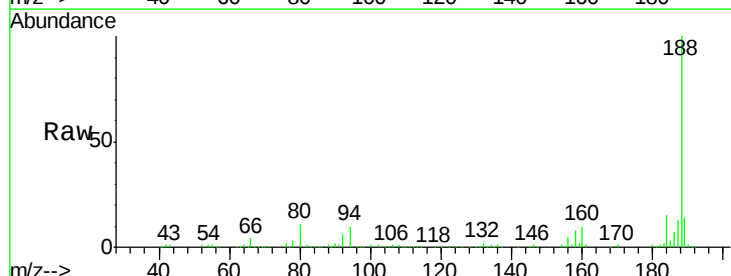


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0



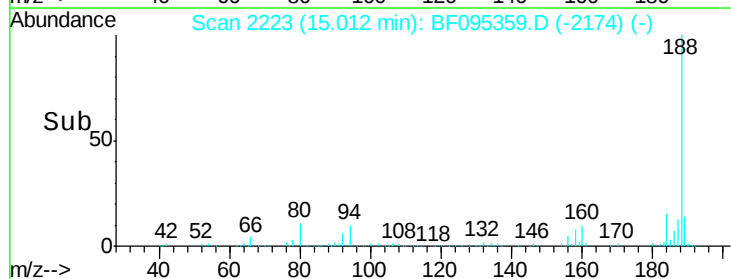
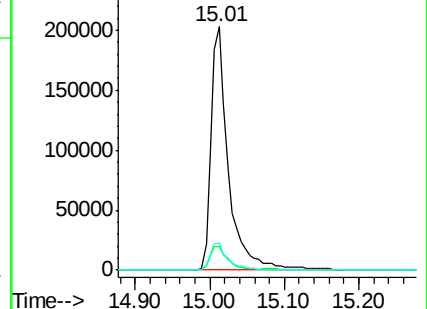


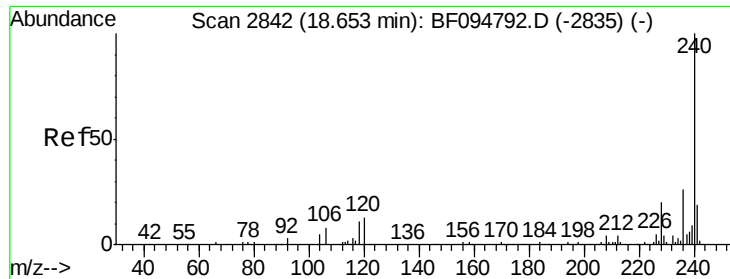

#75
Chrysene-d12
Concen: 20.00 ng
RT: 18.68 min Scan# 2847
Delta R.T. -0.01 min
Lab File: BF095359.D
Acq: 23 May 2017 19:25




Instrument :
BNA_F
ClientSampleId :
PTS-02


Tgt Ion:240 Resp: 189647
Ion Ratio Lower Upper
240 100
120 13.6 5.8 8.8#
236 25.0 20.5 30.7

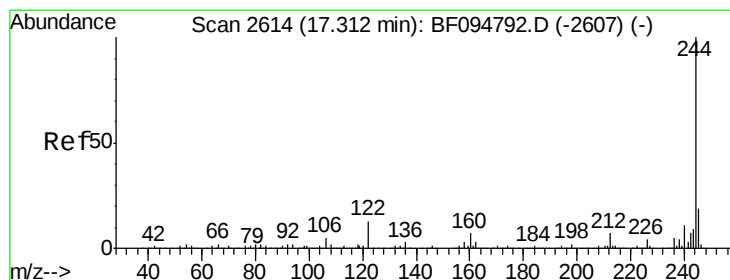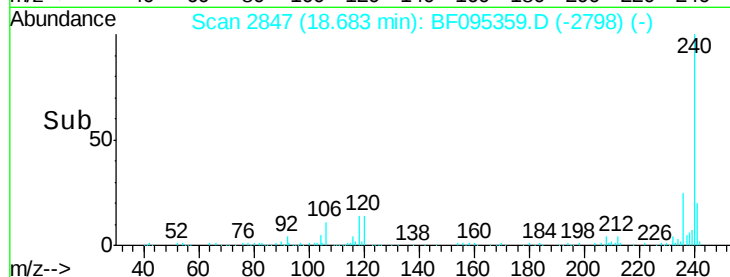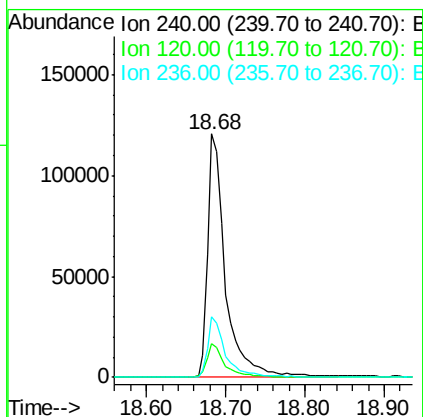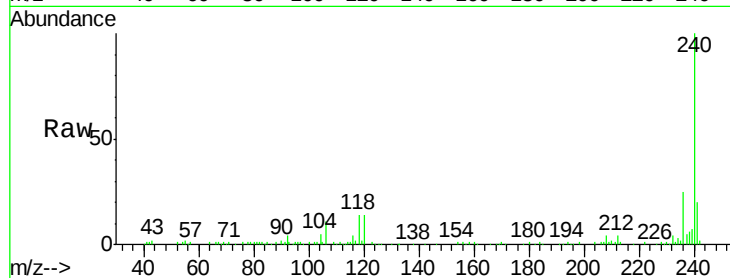

#78
Terphenyl-d14
Concen: 61.06 ng
RT: 17.32 min Scan# 2616
Delta R.T. -0.02 min
Lab File: BF095359.D
Acq: 23 May 2017 19:25

Tgt Ion:244 Resp: 525765
Ion Ratio Lower Upper
244 100
212 6.8 6.0 9.0
122 14.7 10.3 15.5

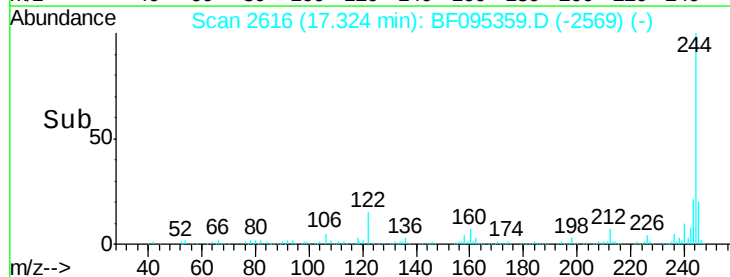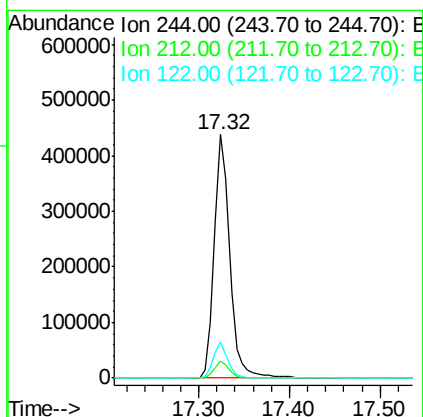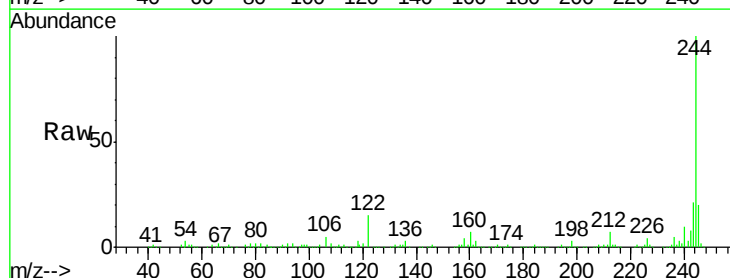

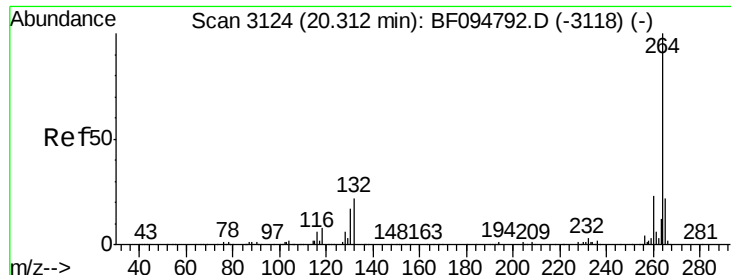

#86
Perylene-d12
Concen: 20.00 ng
RT: 20.36 min Scan# 3132
Delta R.T. -0.01 min
Lab File: BF095359.D
Acq: 23 May 2017 19:25

Instrument :
BNA_F
ClientSampleId :
PTS-02

Tgt Ion	Ratio	Lower	Upper
264	100		
260	24.6	19.5	29.3
265	20.9	17.2	25.8

