


Data Path : Z:\HPCHEM1\BNA_F\Data\BF052317\
 Data File : BF095368.D
 Acq On : 24 May 2017 2:42
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu May 18 17:07:53 2017

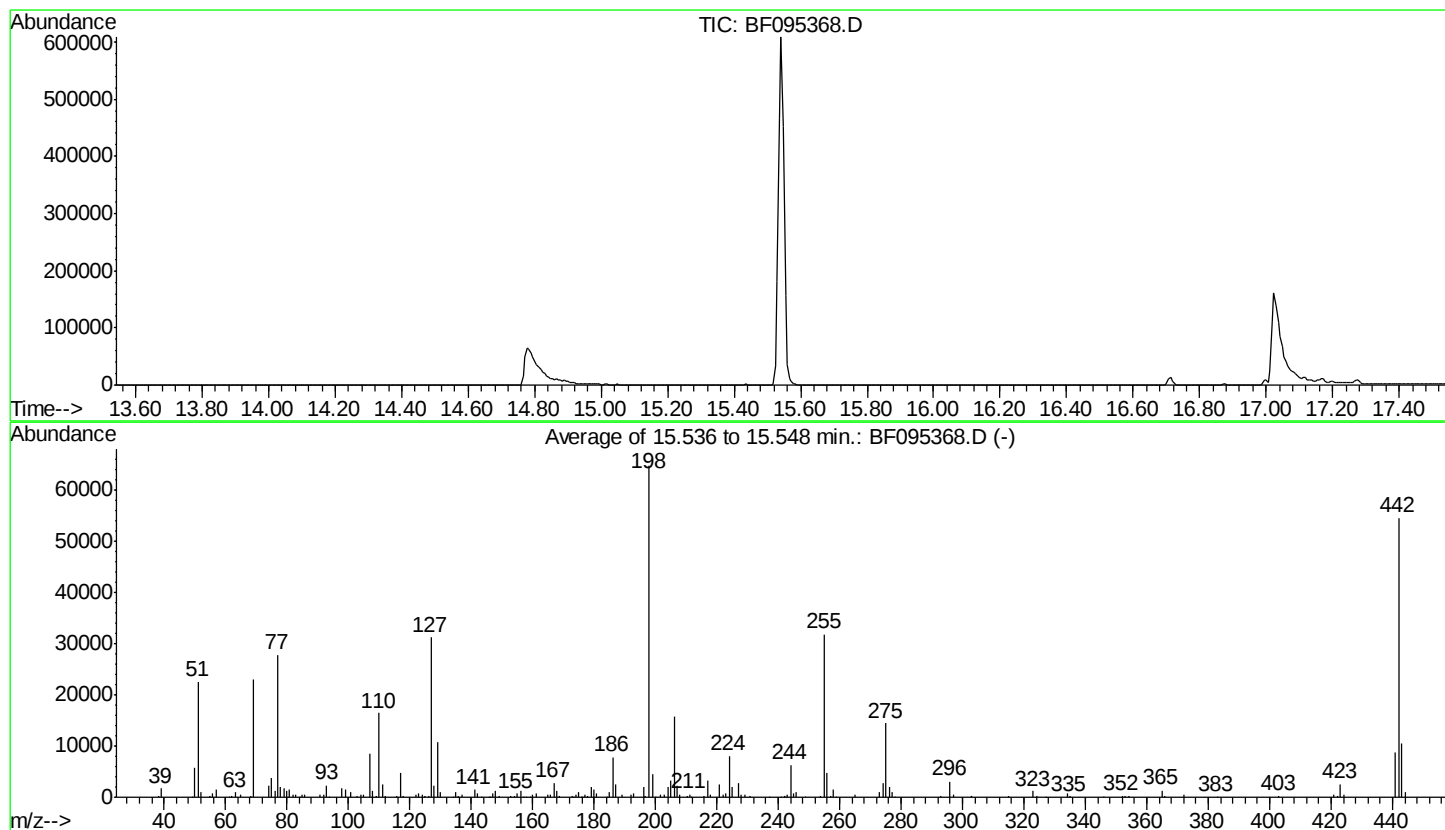

AutoFind: Scans 2312, 2313, 2314; Background Corrected with Scan 2306

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.9	22581	PASS
68	69	0.00	2	1.5	355	PASS
69	198	0.00	100	35.5	22944	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.1	31090	PASS
197	198	0.00	2	0.5	306	PASS
198	198	100	100	100.0	64664	PASS
199	198	5	9	6.8	4404	PASS
275	198	10	60	22.2	14377	PASS
365	198	1	100	2.1	1331	PASS
441	442	0.01	24	15.8	8620	PASS
442	198	50	100	84.3	54538	PASS
443	442	15	24	19.3	10499	PASS