
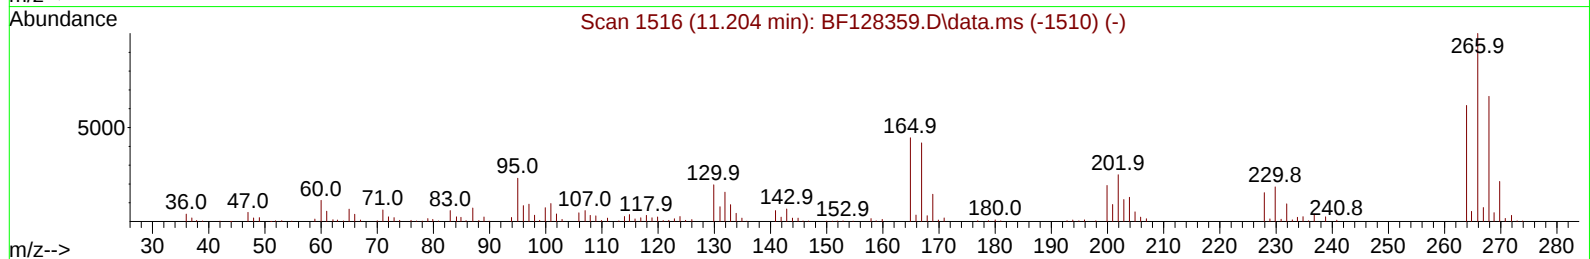
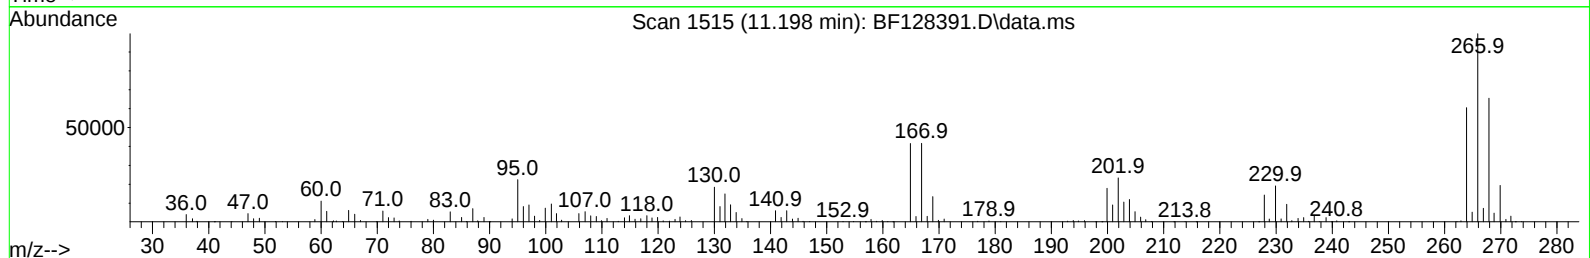


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052322\
Data File : BF128391.D
Acq On : 23 May 2022 10:01
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 24 08:31:12 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 21 05:28:09 2022
Response via : Initial Calibration

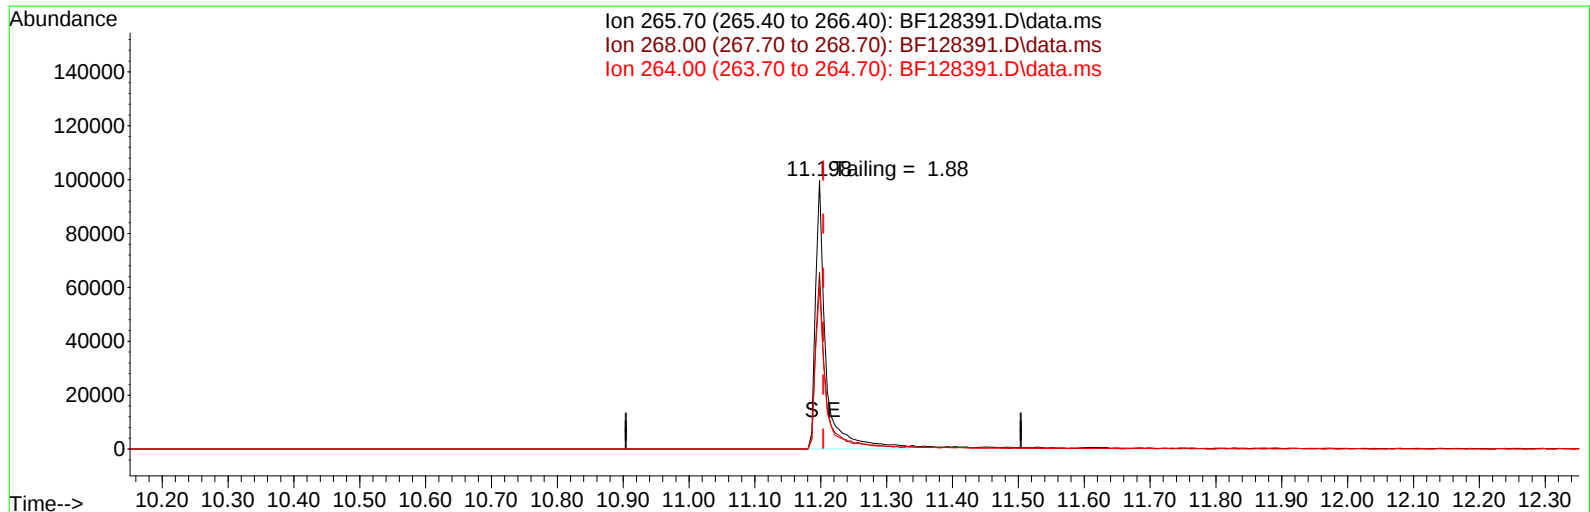

TIC: BF128391.D\data.ms




(70) Pentachlorophenol (C)

11.198min (-0.006) 167898.05 ng

response 111331

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.30	65.75
264.00	66.40	60.72
0.00	0.00	0.00

Quant Time: May 24 08:31:12 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 21 05:28:09 2022
Response via : Initial Calibration

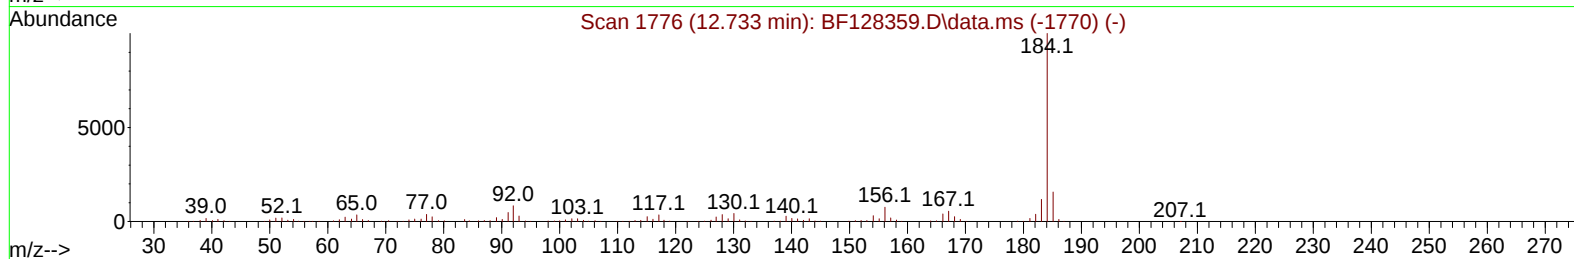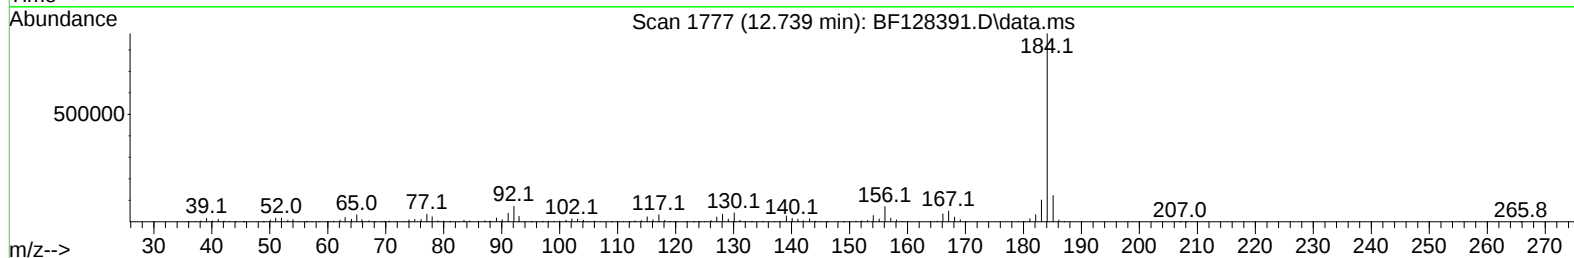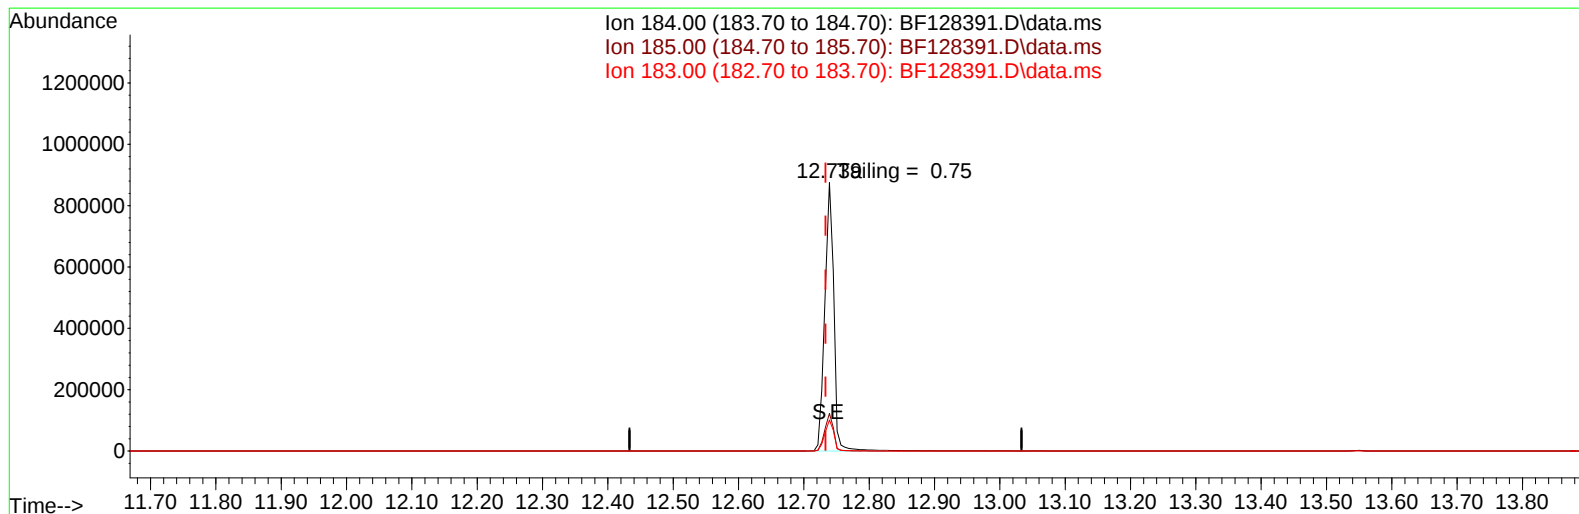

TIC: BF128391.D\data.ms

(77) Benzidine

12.739min (+ 0.006) 526465.04 ng

response **843132**

Ion	Exp%	Act%
-----	------	------

184.00	100.00	100.00
--------	--------	--------

185.00	15.10	14.01
--------	-------	-------

183.00	11.20	11.58
--------	-------	-------

0.00 0.00 0.00