
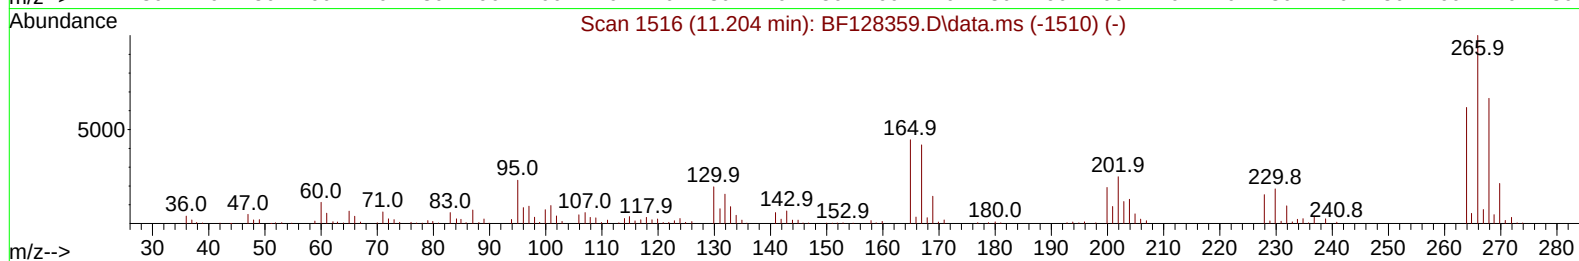
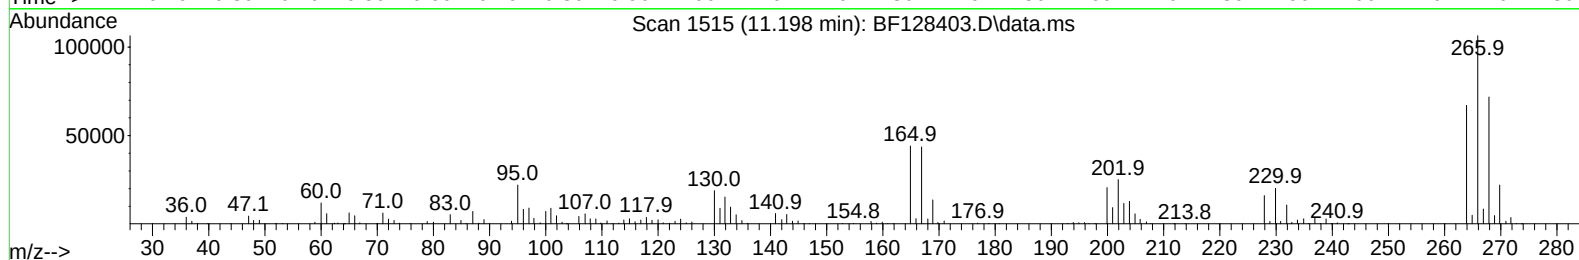


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052322\
Data File : BF128403.D
Acq On : 23 May 2022 16:37
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 24 08:33:45 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 21 05:28:09 2022
Response via : Initial Calibration

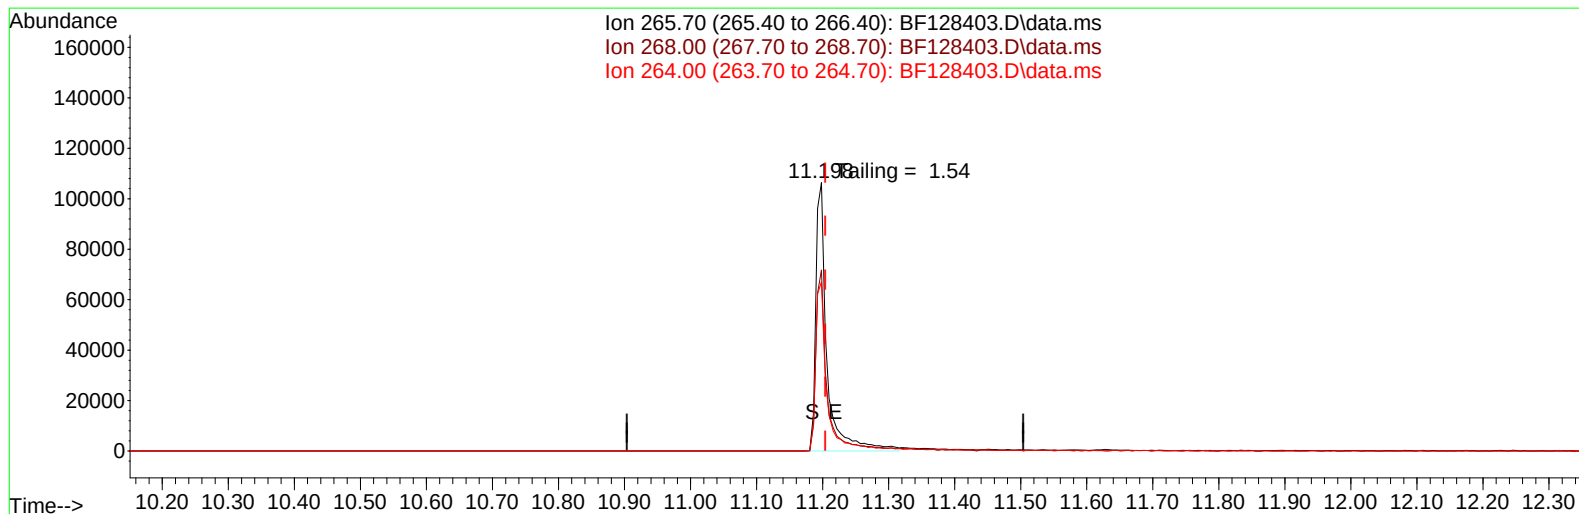

TIC: BF128403.D\data.ms

(70) Pentachlorophenol (C)




11.198min (-0.006) 192327.72 ng

response 127530

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.30	67.43
264.00	66.40	63.04
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052322\  
Data File : BF128403.D  
Acq On    : 23 May 2022  16:37  
Operator  : CG\JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: May 24 08:33:45 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 21 05:28:09 2022
Response via : Initial Calibration

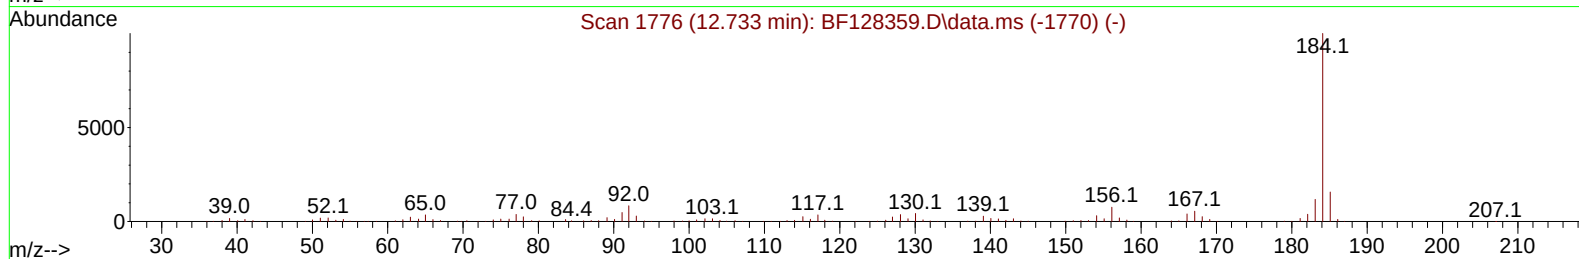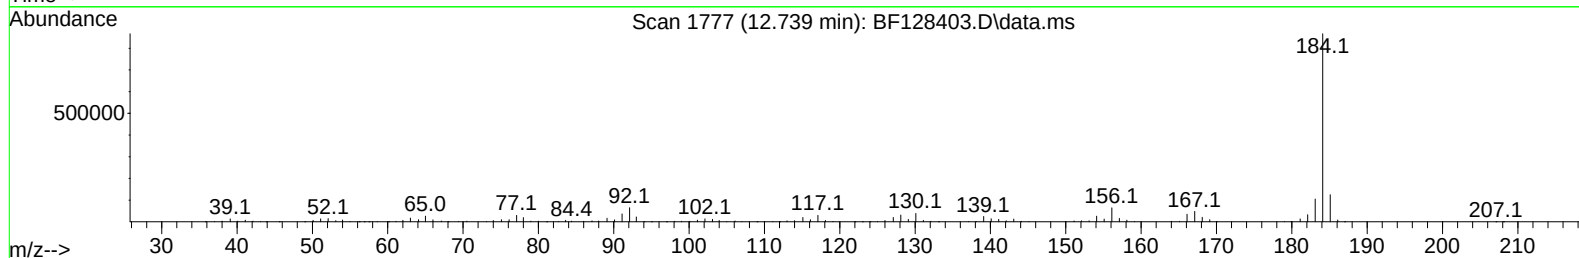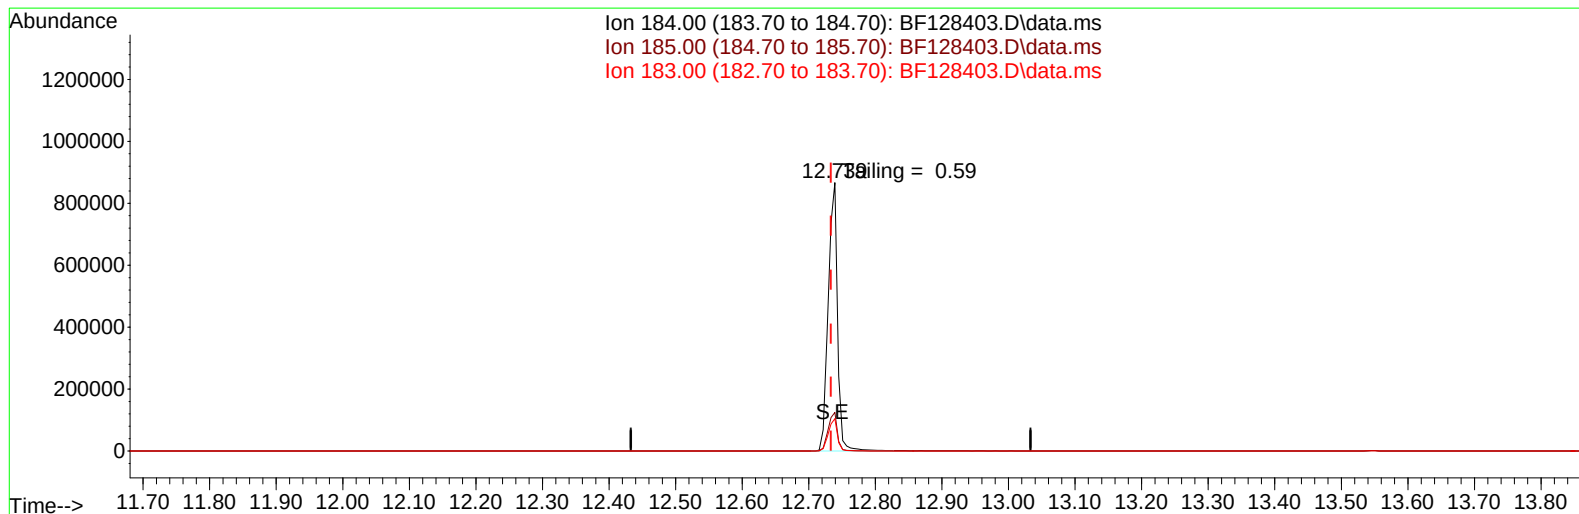

TIC: BF128403.D\data.ms

(77) Benzidine

12.739min (+ 0.006) 341819.89 ng

response **846018**

Ion	Exp%	Act%
-----	------	------

184.00	100.00	100.00
--------	--------	--------

185.00	15.10	14.40
--------	-------	-------

183.00	11.20	12.08
--------	-------	-------

0.00 0.00 0.00