

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052322\
 Data File : BF128410.D
 Acq On : 23 May 2022 20:10
 Operator : CG\JU
 Sample : N2873-08
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 P031-SS001-1824-01

Quant Time: May 24 01:23:45 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat May 21 05:28:09 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.857	152	121450	20.000	ng	0.00
21) Naphthalene-d8	8.139	136	449259	20.000	ng	0.00
39) Acenaphthene-d10	9.892	164	251346	20.000	ng	-0.01
64) Phenanthrene-d10	11.386	188	482260	20.000	ng	0.00
76) Chrysene-d12	14.039	240	244210	20.000	ng	-0.01
86) Perylene-d12	15.527	264	229261	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.481	112	646241	84.678	ng	0.00
7) Phenol-d6	6.492	99	823516	81.947	ng	0.00
23) Nitrobenzene-d5	7.422	82	580052	57.849	ng	-0.01
42) 2,4,6-Tribromophenol	10.692	330	208585	80.469	ng	0.00
45) 2-Fluorobiphenyl	9.210	172	884049	57.519	ng	-0.01
79) Terphenyl-d14	12.974	244	888187	70.209	ng	0.00


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052322\
Data File : BF128410.D
Acq On : 23 May 2022 20:10
Operator : CG\JU
Sample : N2873-08
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P031-SS001-1824-01


Quant Time: May 24 01:23:45 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 21 05:28:09 2022
Response via : Initial Calibration

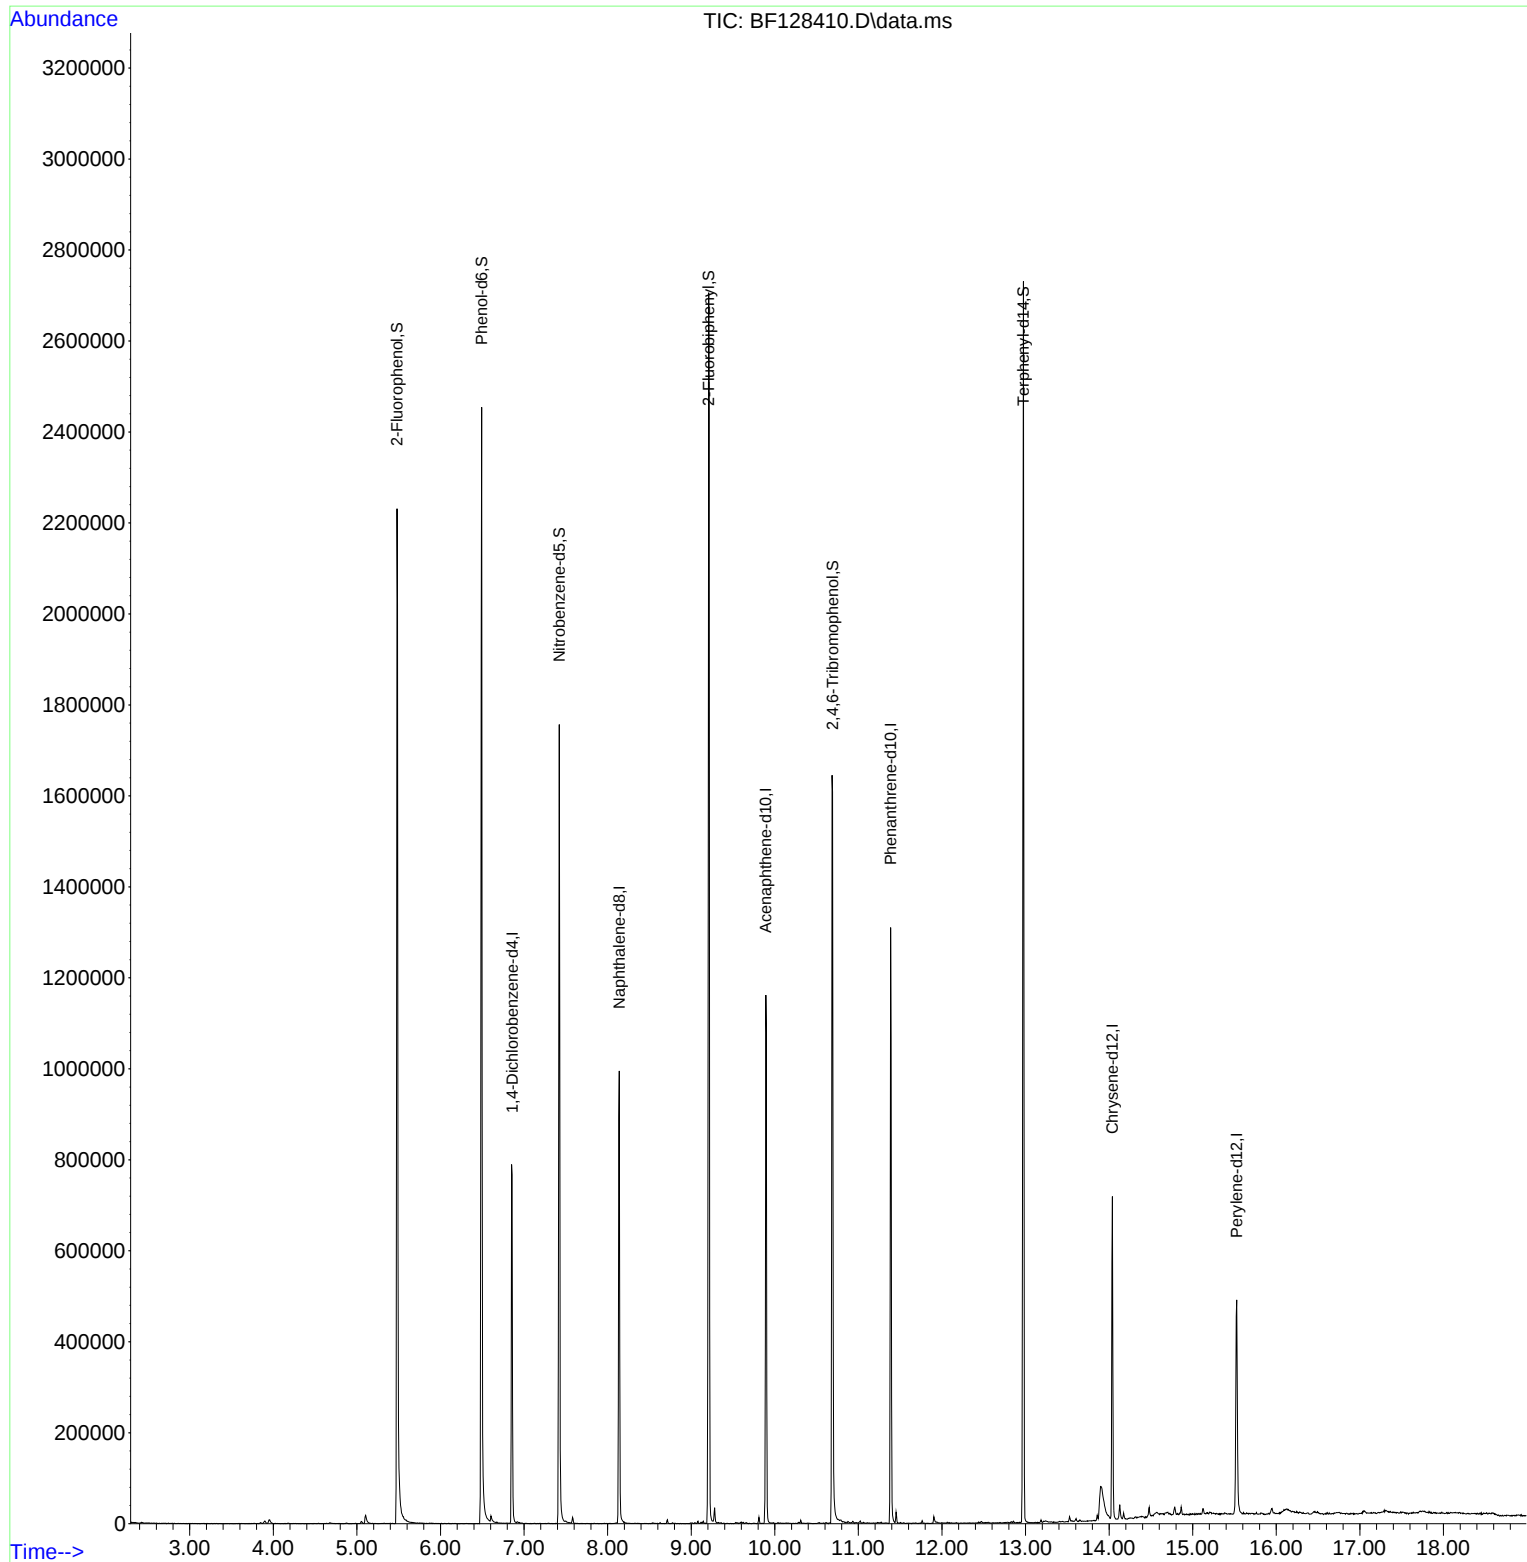






#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.857 min Scan# 71
Delta R.T. 0.000 min
Lab File: BF128410.D
Acq: 23 May 2022 20:10

Instrument :
BNA_F
ClientSampleId :
P031-SS001-1824-01



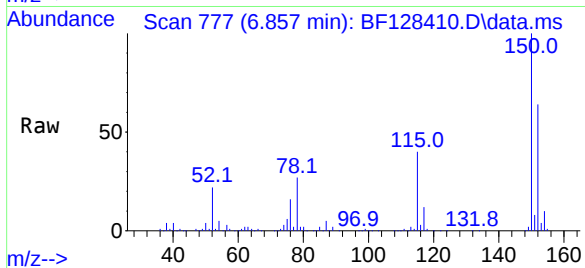



Tgt Ion:152 Resp: 121450
Ion Ratio Lower Upper
152 100
150 156.0 125.3 187.9
115 62.3 48.8 73.2

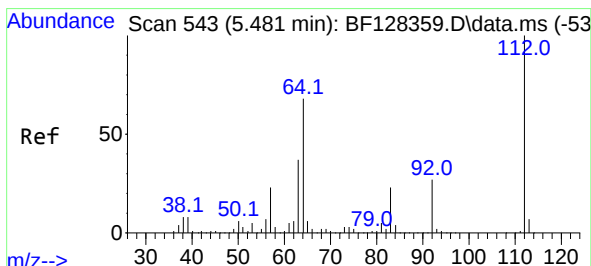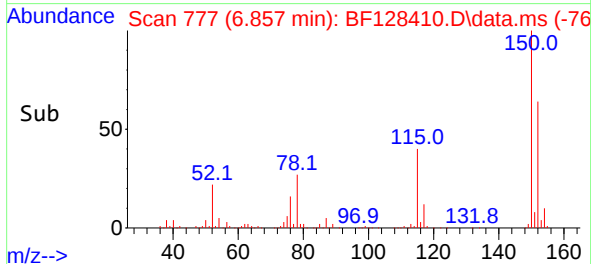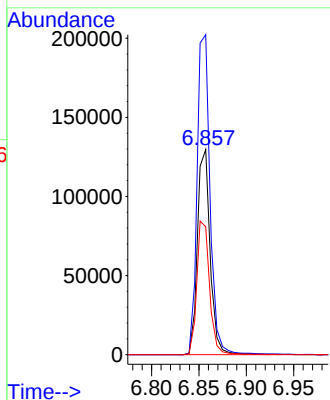

#5
2-Fluorophenol
Concen: 84.678 ng
RT: 5.481 min Scan# 543
Delta R.T. 0.000 min
Lab File: BF128410.D
Acq: 23 May 2022 20:10

Tgt Ion:112 Resp: 646241
Ion Ratio Lower Upper
112 100
64 67.3 49.5 74.3
63 35.6 26.3 39.5


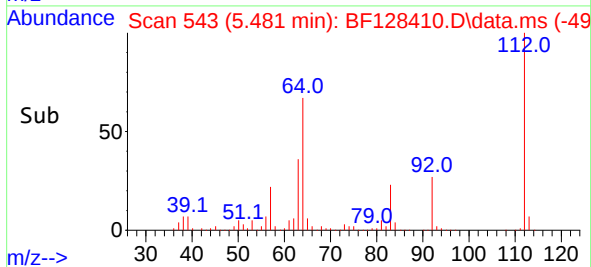
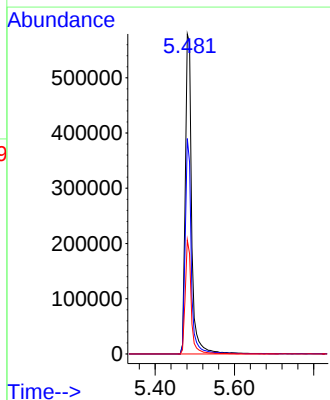
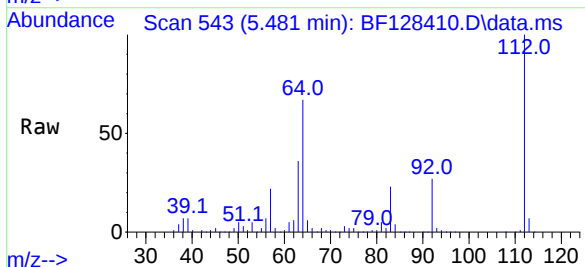


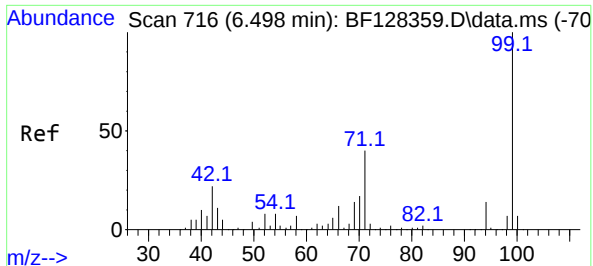

#7
Phenol-d6
Concen: 81.947 ng
RT: 6.492 min Scan# 716
Delta R.T. -0.006 min
Lab File: BF128410.D
Acq: 23 May 2022 20:10




Instrument :
BNA_F
ClientSampleId :
P031-SS001-1824-01


Tgt Ion: 99 Resp: 823516
Ion Ratio Lower Upper
99 100
42 20.0 16.6 24.8
71 37.5 30.0 45.0

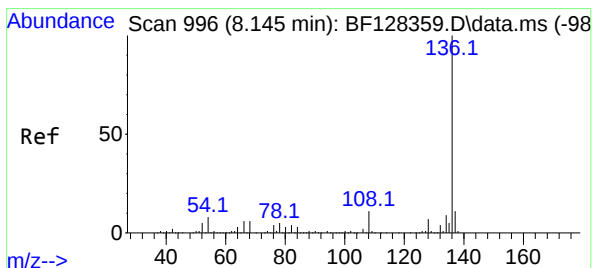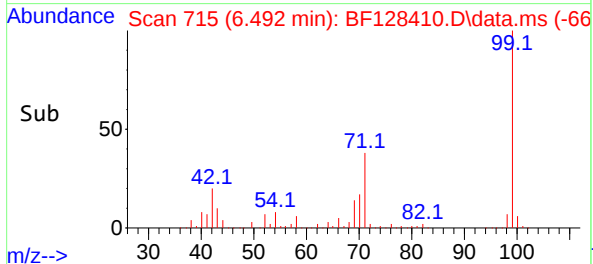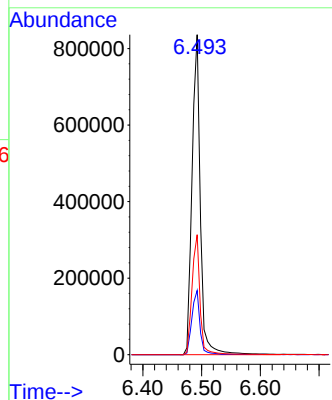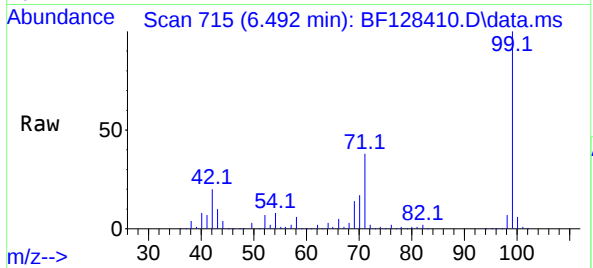

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.139 min Scan# 995
Delta R.T. -0.006 min
Lab File: BF128410.D
Acq: 23 May 2022 20:10

Tgt Ion: 136 Resp: 449259
Ion Ratio Lower Upper
136 100
137 10.6 8.6 13.0
54 8.1 6.8 10.2
68 6.2 5.1 7.7

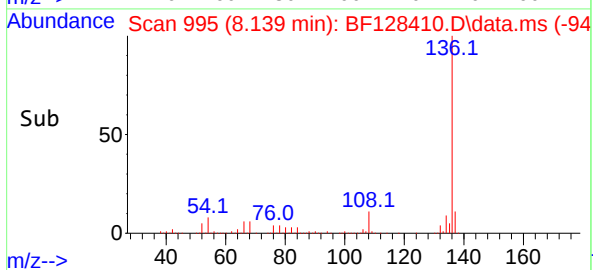
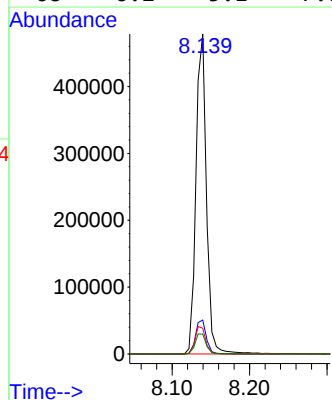
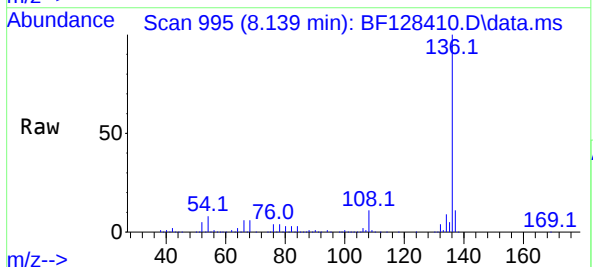


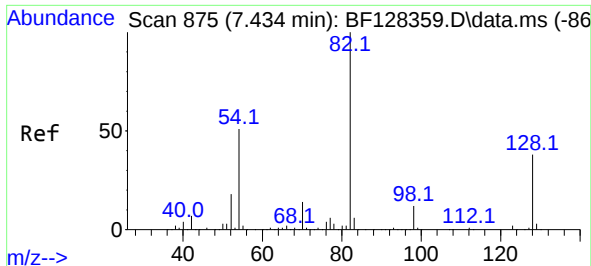

#23
Nitrobenzene-d5
Concen: 57.849 ng
RT: 7.422 min Scan# 81
Delta R.T. -0.012 min
Lab File: BF128410.D
Acq: 23 May 2022 20:10




Instrument :
BNA_F
ClientSampleId :
P031-SS001-1824-01


Tgt Ion: 82 Resp: 580052
Ion Ratio Lower Upper
82 100
128 38.8 30.0 45.0
54 51.6 41.3 61.9

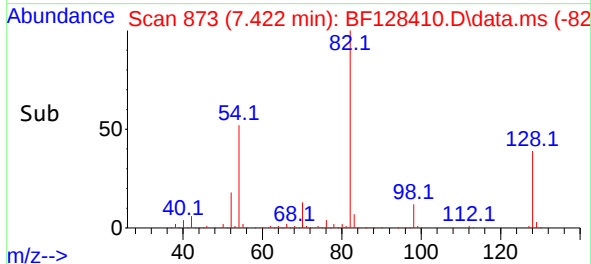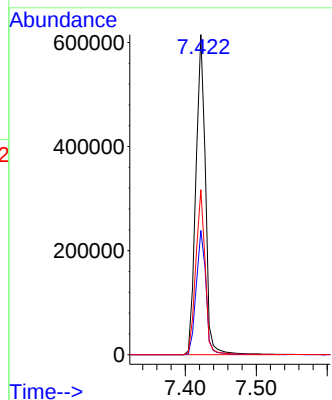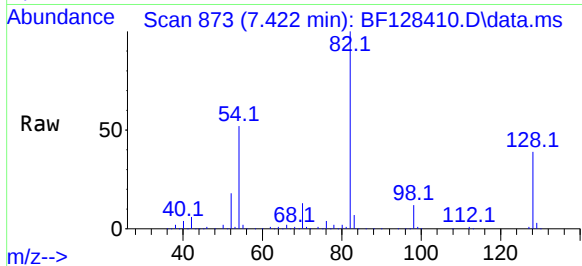

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.892 min Scan# 1293
Delta R.T. -0.012 min
Lab File: BF128410.D
Acq: 23 May 2022 20:10

Tgt Ion:164 Resp: 251346
Ion Ratio Lower Upper
164 100
162 95.9 76.0 114.0
160 43.5 34.8 52.2


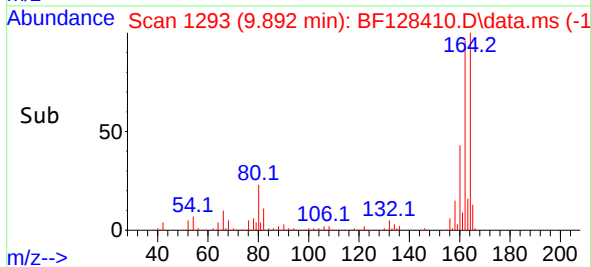
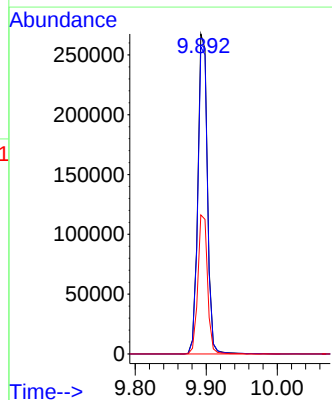
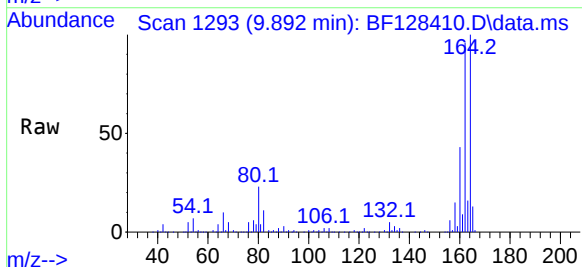


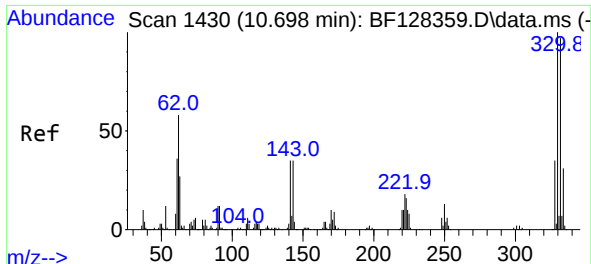

#42
2,4,6-Tribromophenol
Concen: 80.469 ng
RT: 10.692 min Scan# 1429
Delta R.T. -0.006 min
Lab File: BF128410.D
Acq: 23 May 2022 20:10




Instrument :
BNA_F
ClientSampleId :
P031-SS001-1824-01

Tgt Ion:330 Resp: 208585
Ion Ratio Lower Upper
330 100
332 96.7 79.0 118.4
141 33.5 28.9 43.3

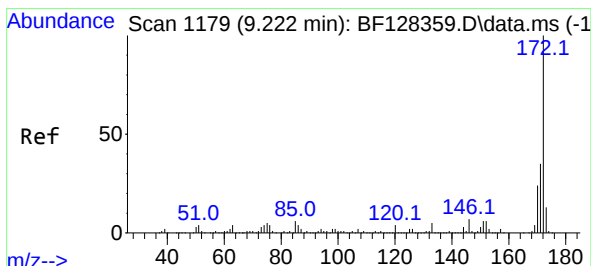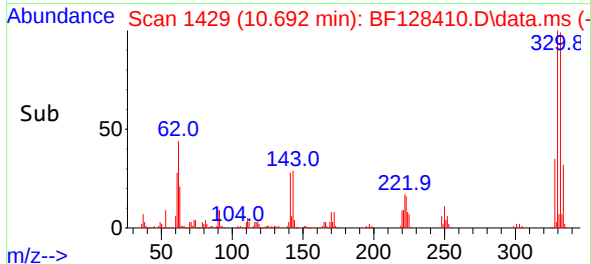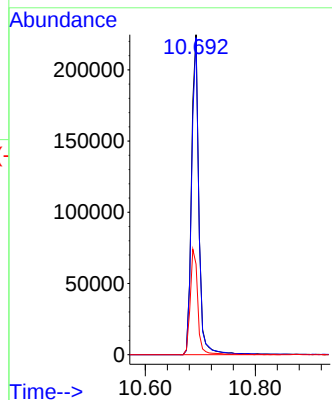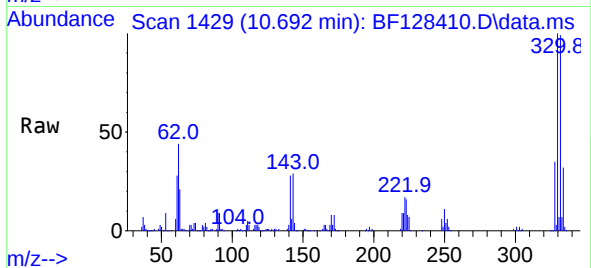

#45
2-Fluorobiphenyl
Concen: 57.519 ng
RT: 9.210 min Scan# 1177
Delta R.T. -0.012 min
Lab File: BF128410.D
Acq: 23 May 2022 20:10

Tgt Ion:172 Resp: 884049
Ion Ratio Lower Upper
172 100
171 35.6 28.6 42.8
170 23.9 19.1 28.7


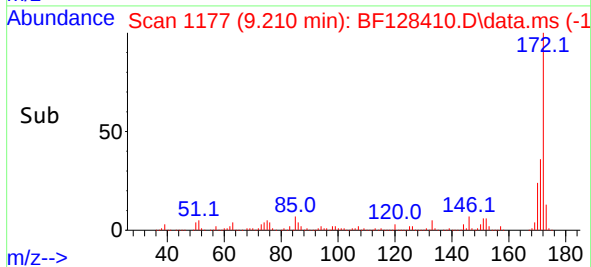
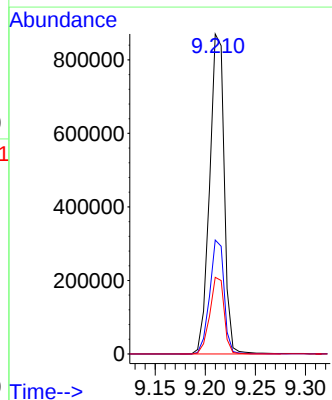
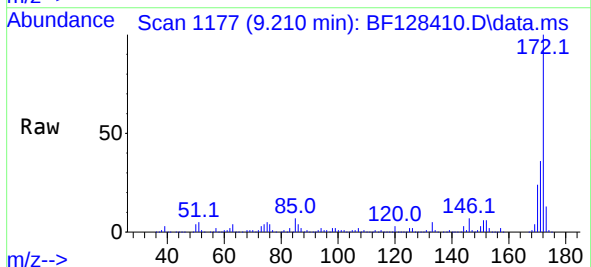




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.386 min Scan# 11
Delta R.T. -0.006 min
Lab File: BF128410.D
Acq: 23 May 2022 20:10




Instrument :
BNA_F
ClientSampleId :
P031-SS001-1824-01

Tgt Ion:188 Resp: 482260
Ion Ratio Lower Upper
188 100
94 9.8 8.0 12.0
80 11.1 8.9 13.3

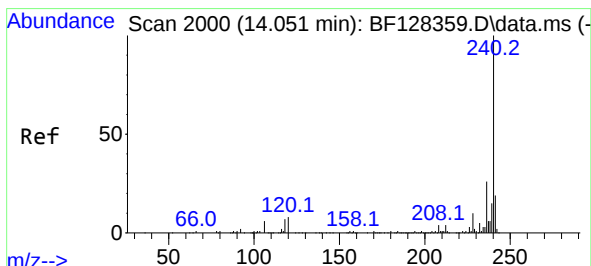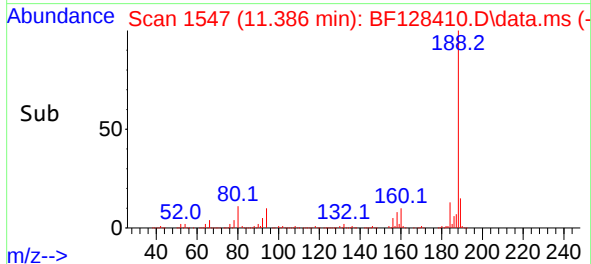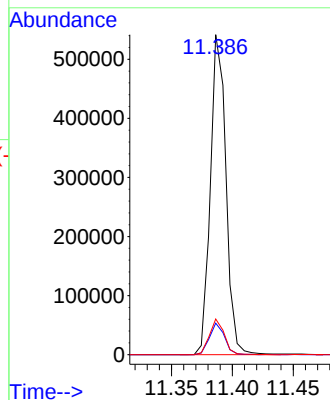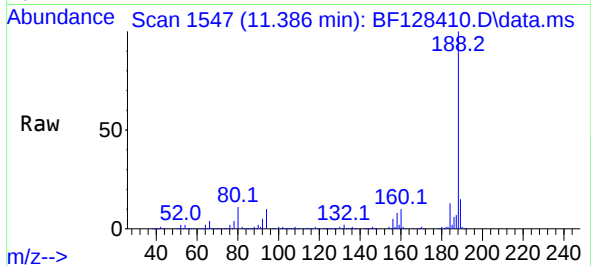

#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.039 min Scan# 1998
Delta R.T. -0.012 min
Lab File: BF128410.D
Acq: 23 May 2022 20:10


Tgt Ion:240 Resp: 244210
Ion Ratio Lower Upper
240 100
120 9.5 7.0 10.6
236 25.2 20.3 30.5

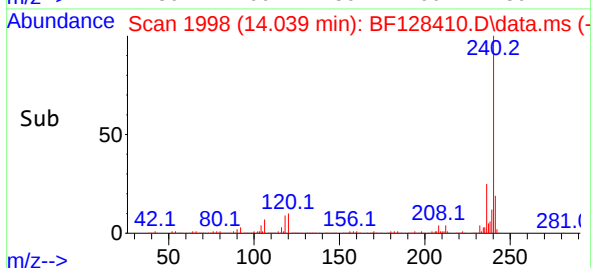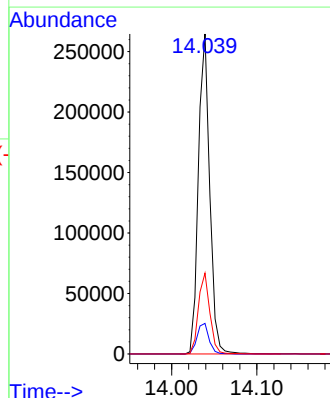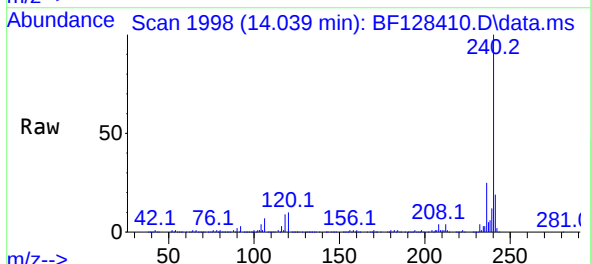






#79
 Terphenyl-d14
 Concen: 70.209 ng
 RT: 12.974 min Scan# 11
 Delta R.T. -0.006 min
 Lab File: BF128410.D
 Acq: 23 May 2022 20:10

Instrument :
 BNA_F
 ClientSampleId :
 P031-SS001-1824-01

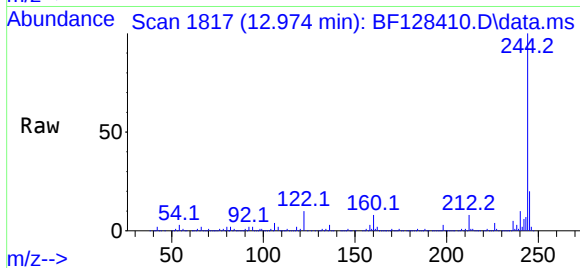

Tgt Ion:244 Resp: 888187
 Ion Ratio Lower Upper
 244 100
 212 7.5 6.2 9.4
 122 9.9 8.6 12.8

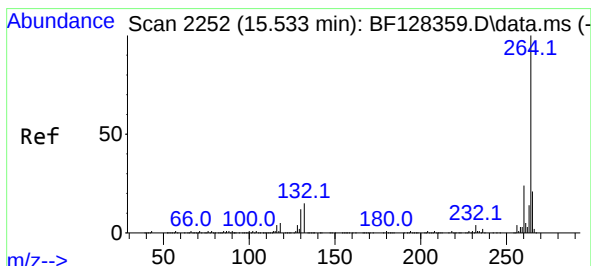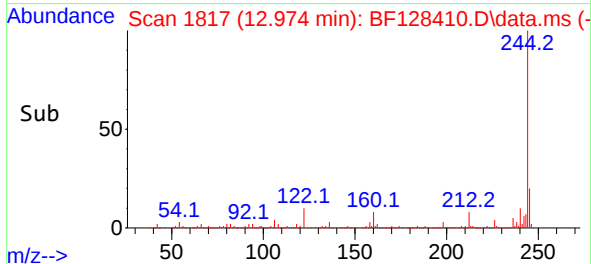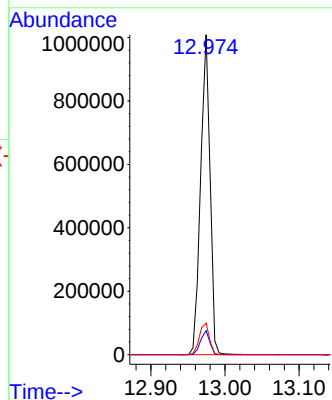

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.527 min Scan# 2251
 Delta R.T. -0.006 min
 Lab File: BF128410.D
 Acq: 23 May 2022 20:10

Tgt Ion:264 Resp: 229261
 Ion Ratio Lower Upper
 264 100
 260 23.1 20.1 30.1
 265 21.5 17.5 26.3

