

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052322\
 Data File : BF128422.D
 Acq On : 24 May 2022 02:04
 Operator : CG\JU
 Sample : N2875-11
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 P007-SS008-0006-01

Quant Time: May 24 02:38:10 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat May 21 05:28:09 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.857	152	113236	20.000	ng	0.00
21) Naphthalene-d8	8.139	136	415857	20.000	ng	0.00
39) Acenaphthene-d10	9.892	164	200969	20.000	ng	-0.01
64) Phenanthrene-d10	11.386	188	297986	20.000	ng	0.00
76) Chrysene-d12	14.039	240	249079	20.000	ng	-0.01
86) Perylene-d12	15.521	264	199907	20.000	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.481	112	562674	79.076	ng	0.00
7) Phenol-d6	6.492	99	704883	75.230	ng	0.00
23) Nitrobenzene-d5	7.422	82	487660	52.541	ng	-0.01
42) 2,4,6-Tribromophenol	10.686	330	129321	62.396	ng	-0.01
45) 2-Fluorobiphenyl	9.210	172	731756	59.545	ng	-0.01
79) Terphenyl-d14	12.969	244	613589	47.555	ng	-0.01


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052322\
Data File : BF128422.D
Acq On : 24 May 2022 02:04
Operator : CG\JU
Sample : N2875-11
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P007-SS008-0006-01

Quant Time: May 24 02:38:10 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 21 05:28:09 2022
Response via : Initial Calibration




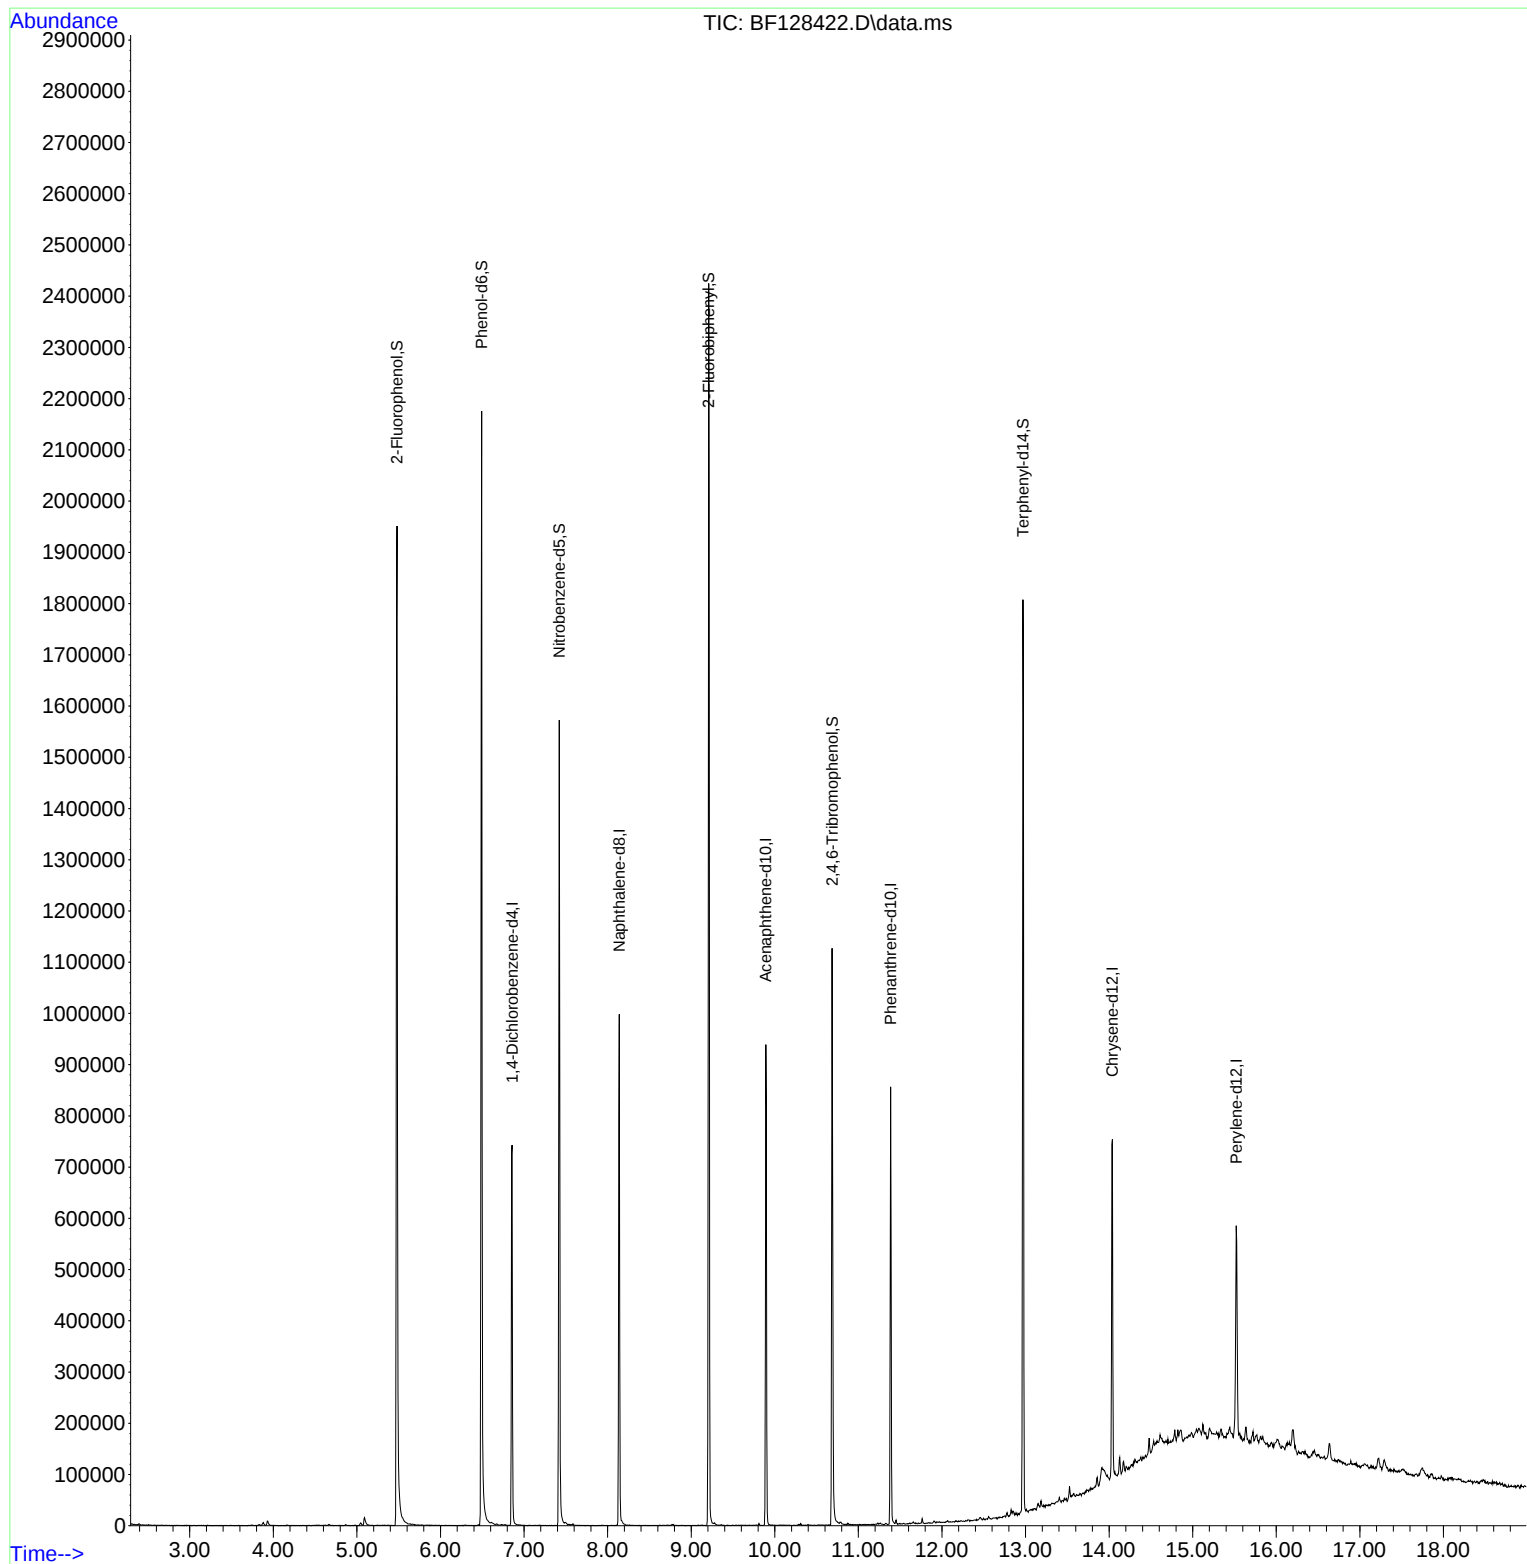


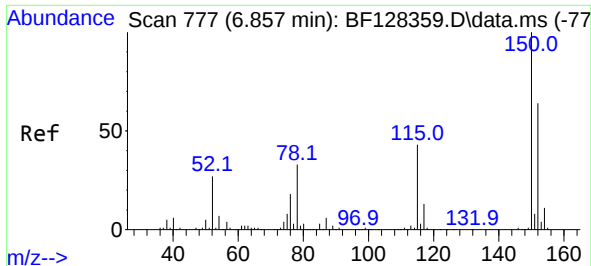

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.857 min Scan# 71
Delta R.T. 0.000 min
Lab File: BF128422.D
Acq: 24 May 2022 02:04




Instrument :
BNA_F
ClientSampleId :
P007-SS008-0006-01


Tgt Ion:152 Resp: 113236
Ion Ratio Lower Upper
152 100
150 157.6 125.3 187.9
115 60.5 48.8 73.2

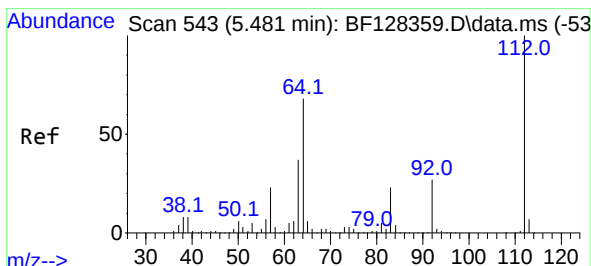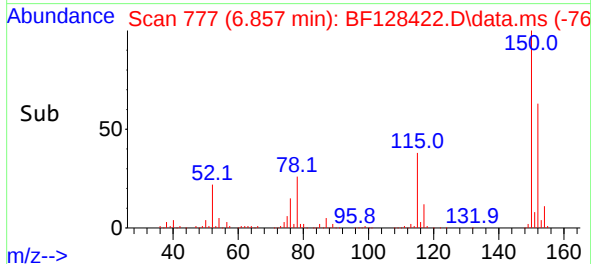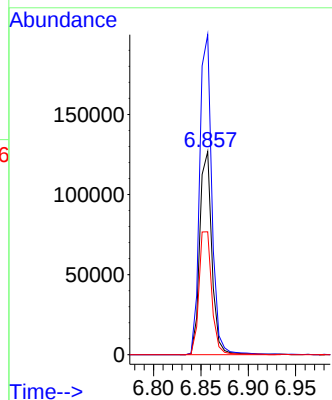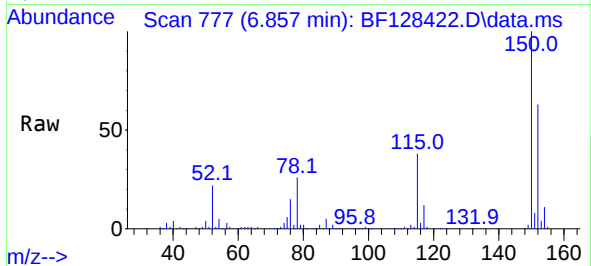

#5
2-Fluorophenol
Concen: 79.076 ng
RT: 5.481 min Scan# 543
Delta R.T. 0.000 min
Lab File: BF128422.D
Acq: 24 May 2022 02:04

Tgt Ion:112 Resp: 562674
Ion Ratio Lower Upper
112 100
64 62.1 49.5 74.3
63 32.9 26.3 39.5


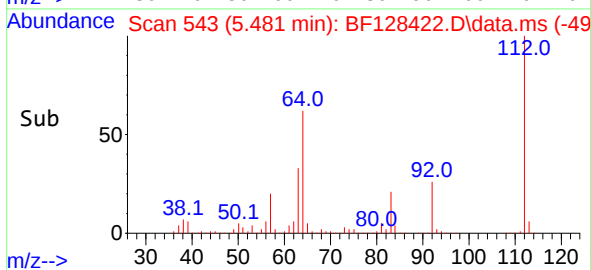
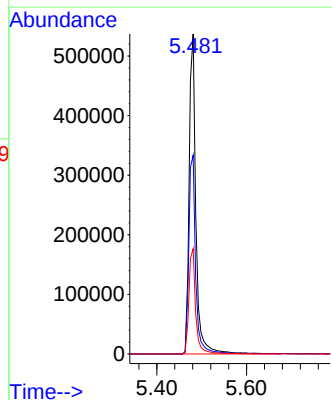
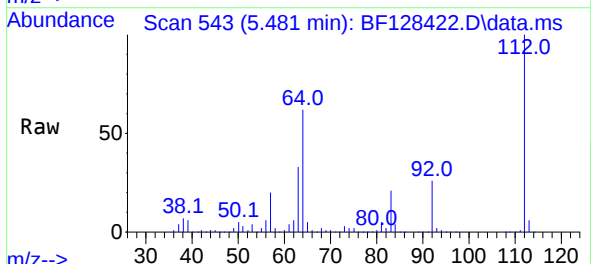


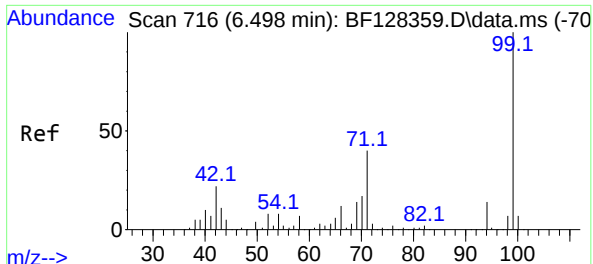

#7
Phenol-d6
Concen: 75.230 ng
RT: 6.492 min Scan# 716
Delta R.T. -0.006 min
Lab File: BF128422.D
Acq: 24 May 2022 02:04




Instrument :
BNA_F
ClientSampleId :
P007-SS008-0006-01


Tgt Ion: 99 Resp: 704883
Ion Ratio Lower Upper
99 100
42 19.8 16.6 24.8
71 37.4 30.0 45.0

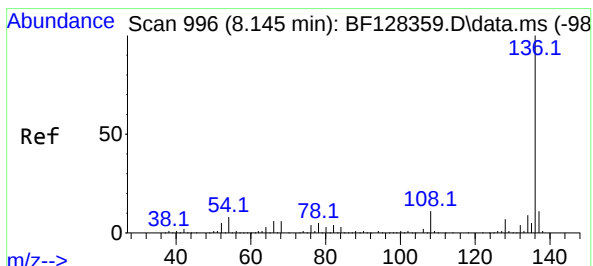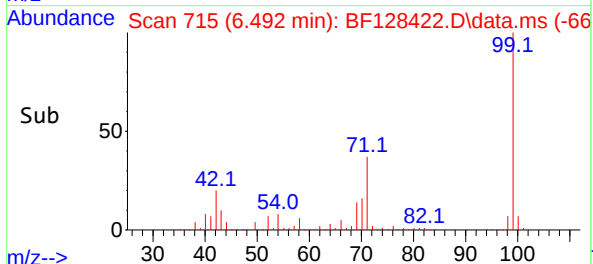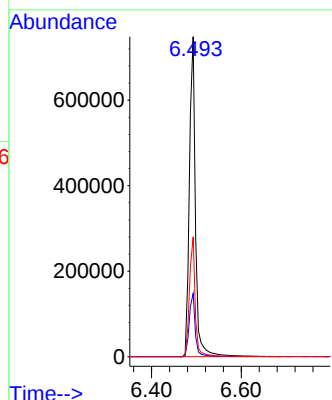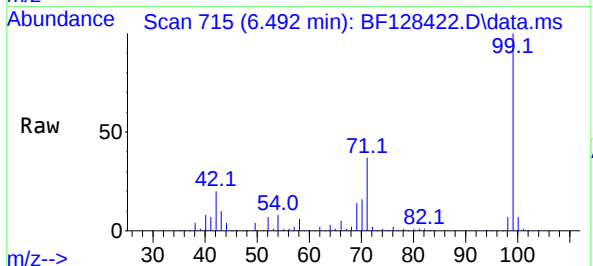

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.139 min Scan# 995
Delta R.T. -0.006 min
Lab File: BF128422.D
Acq: 24 May 2022 02:04

Tgt Ion: 136 Resp: 415857
Ion Ratio Lower Upper
136 100
137 10.4 8.6 13.0
54 8.2 6.8 10.2
68 6.0 5.1 7.7


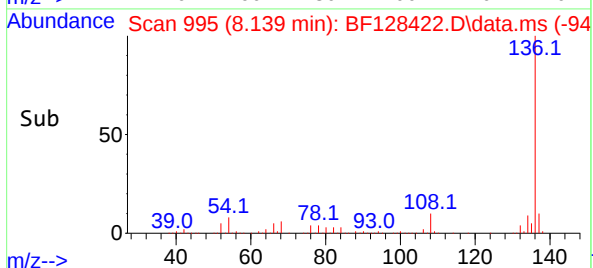
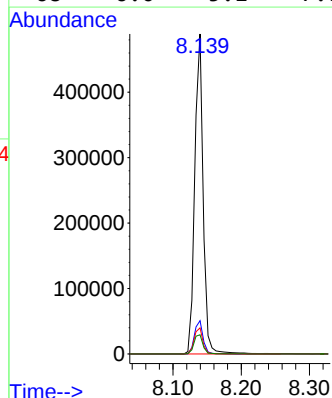
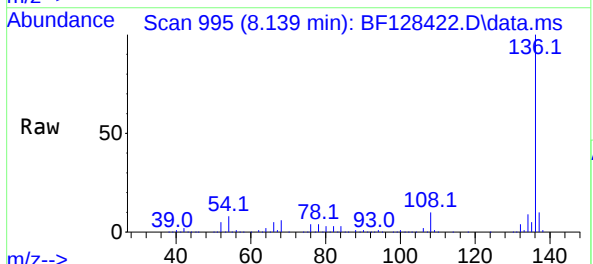


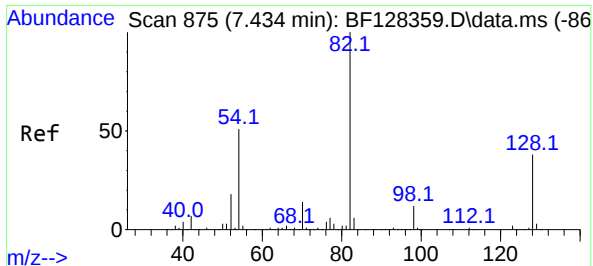

#23
Nitrobenzene-d5
Concen: 52.541 ng
RT: 7.422 min Scan# 81
Delta R.T. -0.012 min
Lab File: BF128422.D
Acq: 24 May 2022 02:04




Instrument :
BNA_F
ClientSampleId :
P007-SS008-0006-01


Tgt Ion: 82 Resp: 487660
Ion Ratio Lower Upper
82 100
128 37.9 30.0 45.0
54 50.0 41.3 61.9

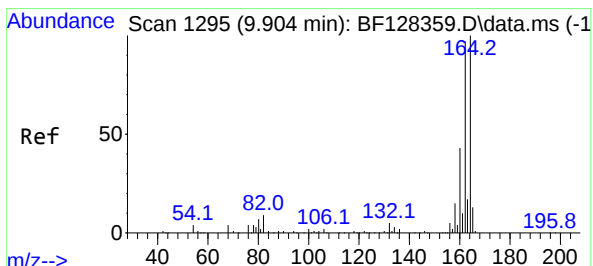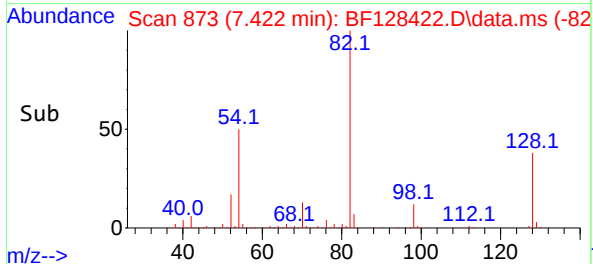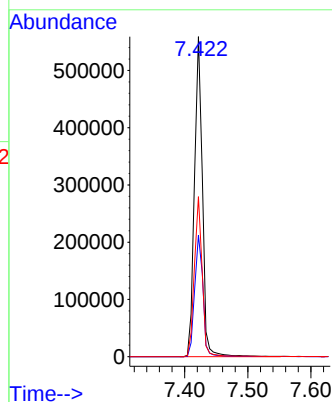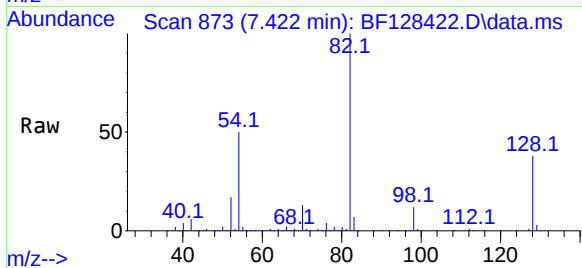

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.892 min Scan# 1293
Delta R.T. -0.012 min
Lab File: BF128422.D
Acq: 24 May 2022 02:04

Tgt Ion:164 Resp: 200969
Ion Ratio Lower Upper
164 100
162 93.9 76.0 114.0
160 42.1 34.8 52.2

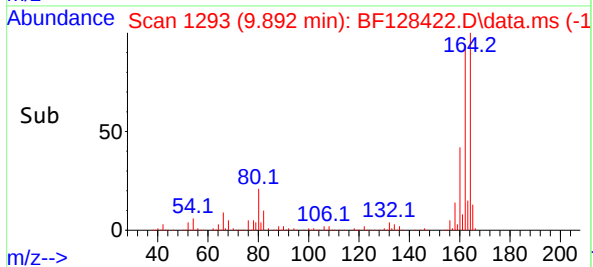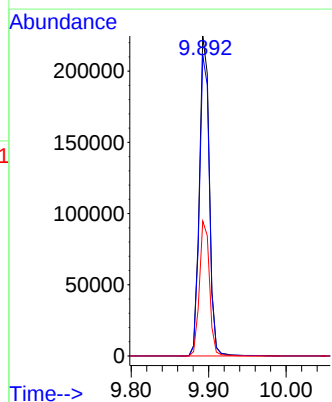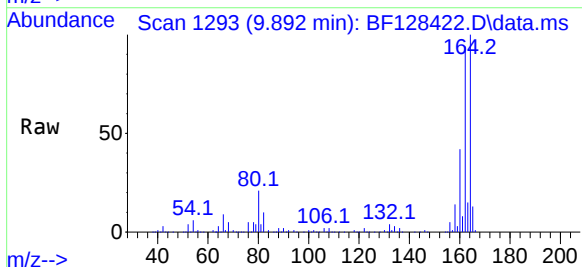

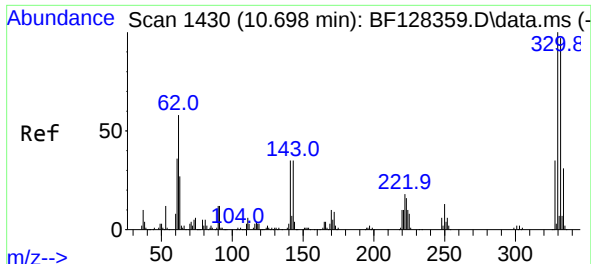

#42

2,4,6-Tribromophenol

Concen: 62.396 ng

RT: 10.686 min Scan# 1428

Delta R.T. -0.012 min

Lab File: BF128422.D

Acq: 24 May 2022 02:04

Instrument :

BNA_F

ClientSampleId :

P007-SS008-0006-01





Tgt Ion:330 Resp: 129321

Ion Ratio Lower Upper

330 100

332 96.7 79.0 118.4

141 32.6 28.9 43.3

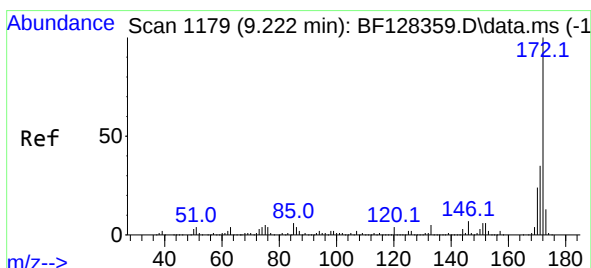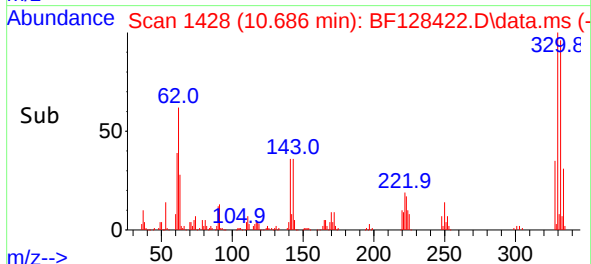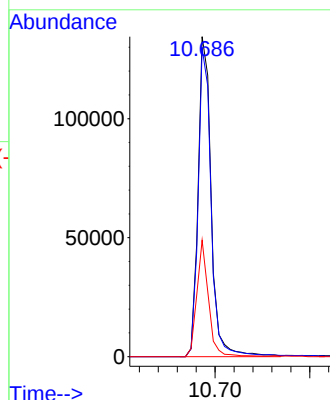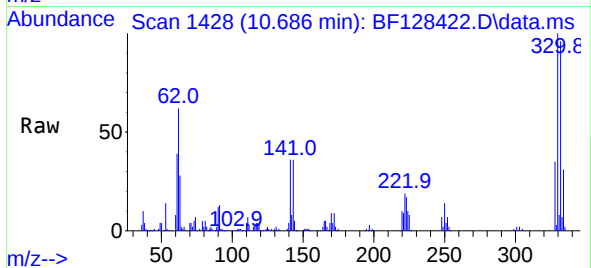

#45

2-Fluorobiphenyl

Concen: 59.545 ng

RT: 9.210 min Scan# 1177

Delta R.T. -0.012 min

Lab File: BF128422.D

Acq: 24 May 2022 02:04




Tgt Ion:172 Resp: 731756


Ion Ratio Lower Upper

172 100

171 34.7 28.6 42.8

170 23.2 19.1 28.7


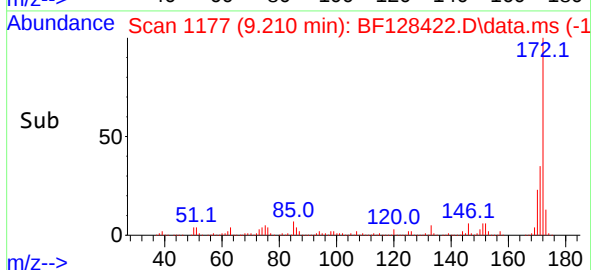
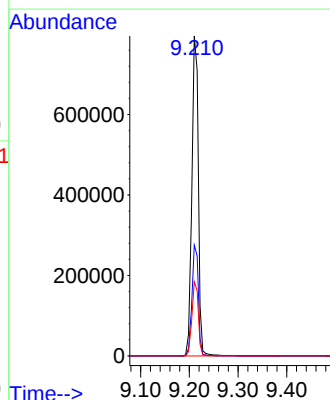
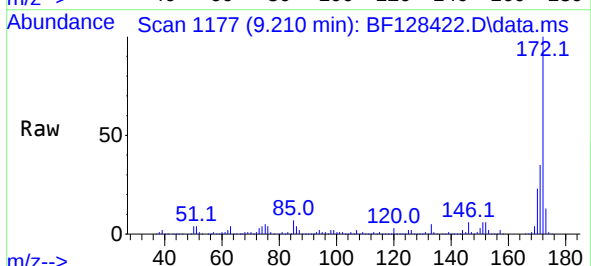


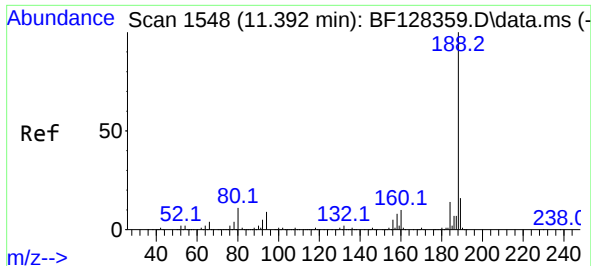

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.386 min Scan# 11
Delta R.T. -0.006 min
Lab File: BF128422.D
Acq: 24 May 2022 02:04




Instrument :
BNA_F
ClientSampleId :
P007-SS008-0006-01


Tgt Ion:188 Resp: 297986
Ion Ratio Lower Upper
188 100
94 9.7 8.0 12.0
80 10.7 8.9 13.3

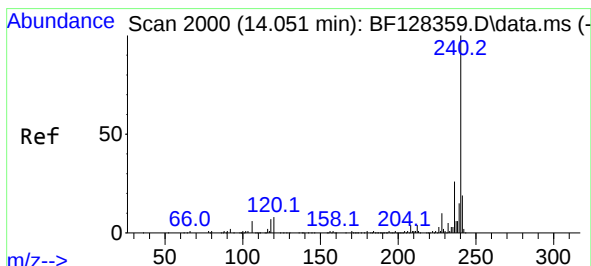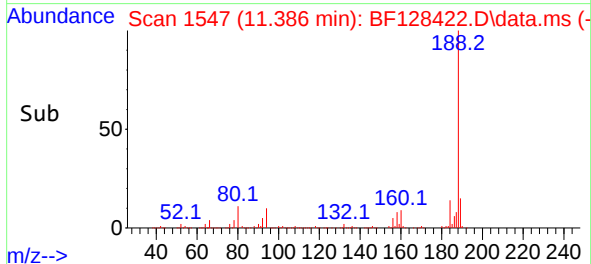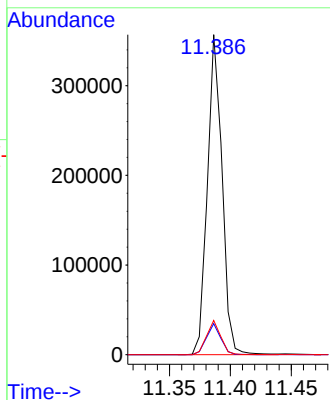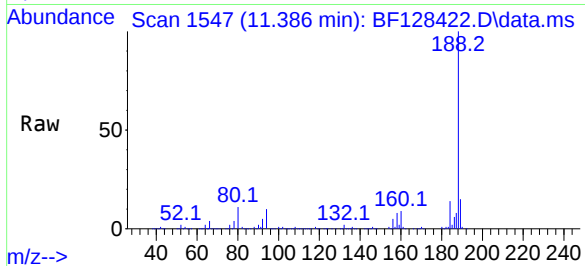

#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.039 min Scan# 1998
Delta R.T. -0.012 min
Lab File: BF128422.D
Acq: 24 May 2022 02:04

Tgt Ion:240 Resp: 249079
Ion Ratio Lower Upper
240 100
120 9.1 7.0 10.6
236 24.9 20.3 30.5


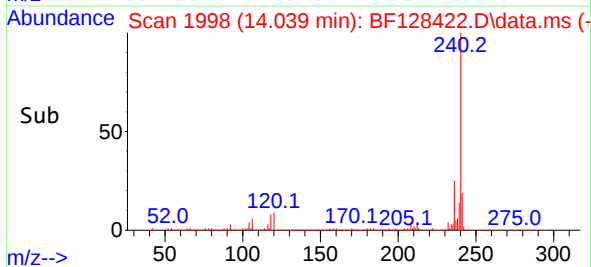
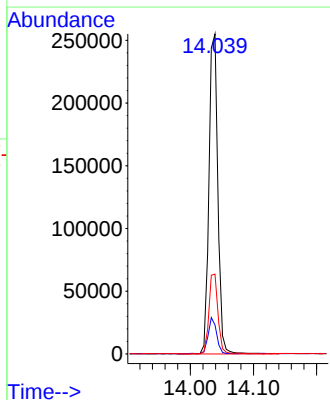
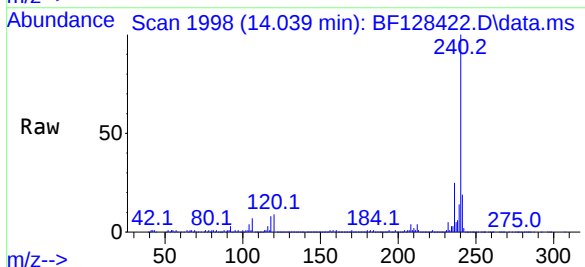


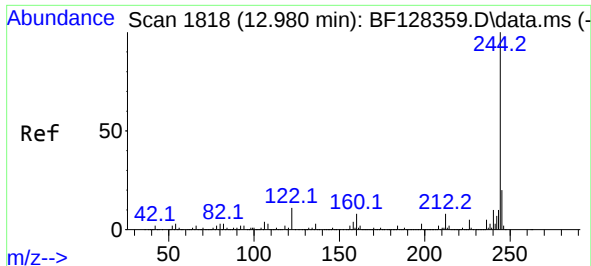

#79
 Terphenyl-d14
 Concen: 47.555 ng
 RT: 12.969 min Scan# 1818
 Delta R.T. -0.012 min
 Lab File: BF128422.D
 Acq: 24 May 2022 02:04

Instrument :
 BNA_F
 ClientSampleId :
 P007-SS008-0006-01

Tgt Ion:244 Resp: 613589
 Ion Ratio Lower Upper
 244 100
 212 7.4 6.2 9.4
 122 11.3 8.6 12.8

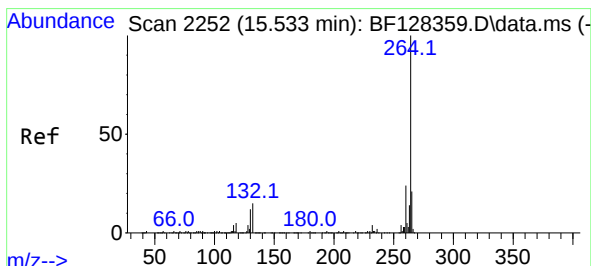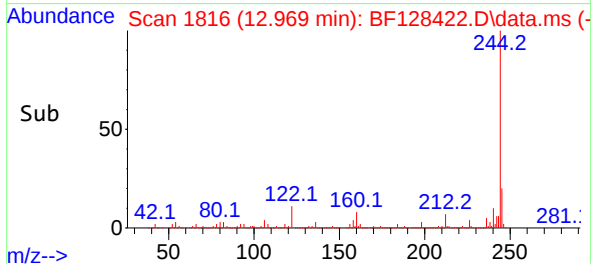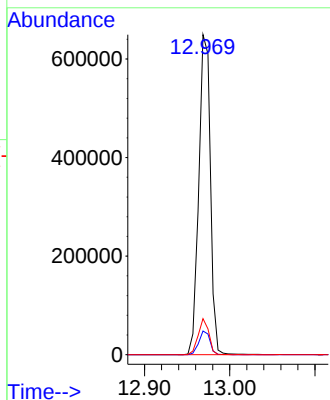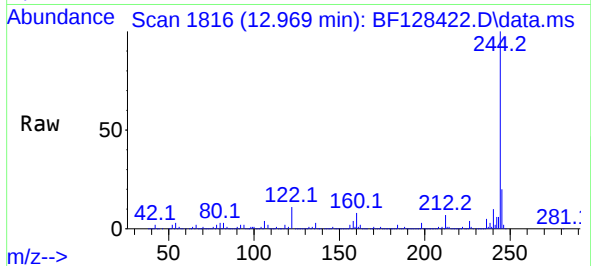

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.521 min Scan# 2250
 Delta R.T. -0.012 min
 Lab File: BF128422.D
 Acq: 24 May 2022 02:04

Tgt Ion:264 Resp: 199907
 Ion Ratio Lower Upper
 264 100
 260 24.0 20.1 30.1
 265 22.5 17.5 26.3

