

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052322\
 Data File : BF128399.D
 Acq On : 23 May 2022 14:34
 Operator : CG\JU
 Sample : N2873-04
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 P029-SS001-2430-01

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128399.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.481	539	543	566	rBV	1853428	1834992	89.00%	13.160%
2	6.492	711	715	733	rBV	2094208	1865033	90.46%	13.375%
3	6.857	774	777	786	rBV	578625	496903	24.10%	3.564%
4	7.422	869	873	890	rBV	1371678	1244029	60.34%	8.922%
5	8.139	991	995	1013	rBV	841064	692966	33.61%	4.970%
6	9.210	1174	1177	1181	rBV	2341629	2061803	100.00%	14.786%
7	9.898	1290	1294	1302	rBV	862820	763795	37.05%	5.478%
8	10.692	1425	1429	1438	rBV	1319396	1327190	64.37%	9.518%
9	11.386	1544	1547	1555	rBV	819467	778743	37.77%	5.585%
10	12.974	1813	1817	1820	rBV	2074382	1741333	84.46%	12.488%
11	13.904	1969	1975	1986	rBV6	15641	44234	2.15%	0.317%
12	14.039	1994	1998	2006	rVB	579089	506468	24.56%	3.632%
13	14.127	2009	2013	2020	rBV	142325	145731	7.07%	1.045%
14	15.527	2246	2251	2263	rVB2	342206	440700	21.37%	3.161%

Sum of corrected areas: 13943920

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052322\
Data File : BF128399.D
Acq On : 23 May 2022 14:34
Operator : CG\JU
Sample : N2873-04
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P029-SS001-2430-01










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Triphenylphosphine oxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
14.127	5.75 ng	145731	Chrysene-d12	14.039

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Triphenylphosphine oxide	278	C18H15OP	000791-28-6	92
2			(E)-7-Benzylidene-1-azabicyclo[3...]	293	C15H19NO3S	1000483-83-4	70
3			Formaldehyde, (triphenylphosphor...]	304	C19H17N2P	015990-54-2	50
4			Carbazol-1-one, 1,2,3,4-tetrahyd...	277	C18H15NO2	299962-12-2	25
5			Vanadium, cycloheptatrienyl-(pen...	277	C17H22V	1000155-20-5	23

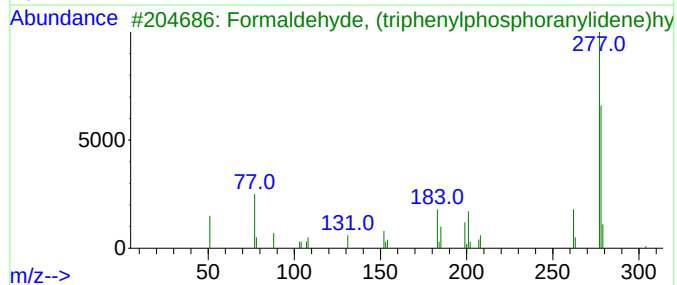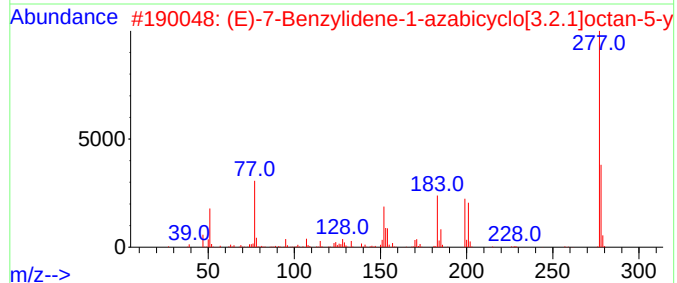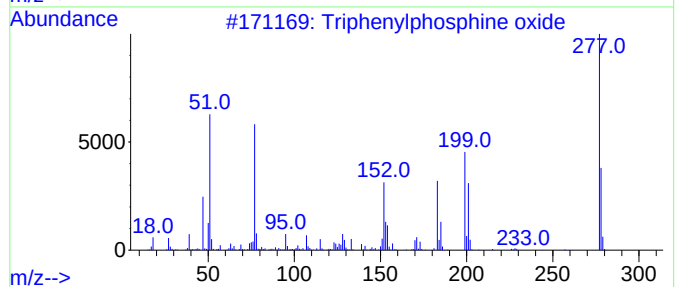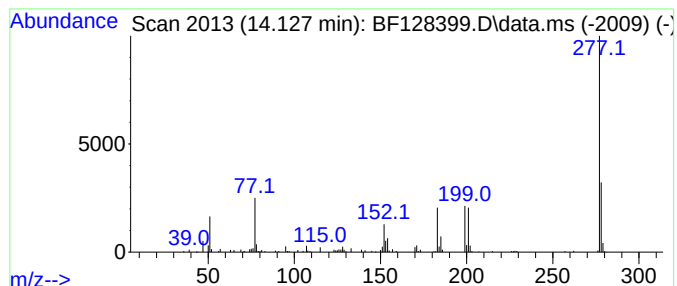

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052322\
Data File : BF128399.D
Acq On : 23 May 2022 14:34
Operator : CG\JU
Sample : N2873-04
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P029-SS001-2430-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Triphenylphosph...	14.127	5.8	ng	145731	5	14.039	506468	20.0