

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052322\
 Data File : BF128400.D
 Acq On : 23 May 2022 15:04
 Operator : CG\JU
 Sample : N2873-11
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 P032-SS001-0612-01

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128400.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.481	539	543	560	rBV	1645198	1799921	86.96%	12.566%
2	6.493	711	715	730	rBV	2022469	1805090	87.21%	12.602%
3	6.857	773	777	786	rBV	612480	535906	25.89%	3.741%
4	7.422	869	873	890	rBV	1423899	1211294	58.52%	8.457%
5	8.139	991	995	1014	rBV	797797	682450	32.97%	4.764%
6	9.210	1174	1177	1181	rBV	2230273	2069901	100.00%	14.451%
7	9.892	1290	1293	1302	rBV	823333	751537	36.31%	5.247%
8	10.686	1425	1428	1443	rBV	1257480	1270239	61.37%	8.868%
9	11.386	1544	1547	1556	rBV	820071	776374	37.51%	5.420%
10	12.974	1813	1817	1820	rBV	2325352	1999115	96.58%	13.957%
11	13.898	1969	1974	1989	rVB3	45692	137393	6.64%	0.959%
12	14.039	1994	1998	2007	rVB	669197	606359	29.29%	4.233%
13	14.127	2009	2013	2019	rBV	144507	144596	6.99%	1.009%
14	15.527	2246	2251	2261	rVB	405730	533586	25.78%	3.725%




Sum of corrected areas: 14323761

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052322\
Data File : BF128400.D
Acq On : 23 May 2022 15:04
Operator : CG\JU
Sample : N2873-11
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P032-SS001-0612-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

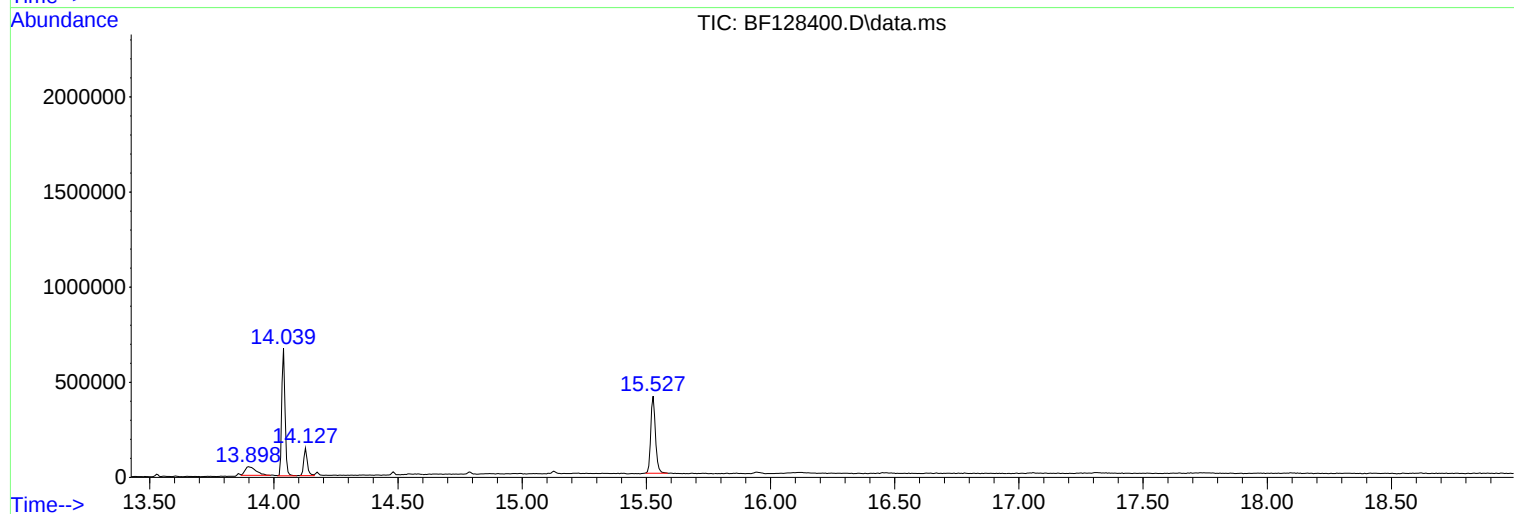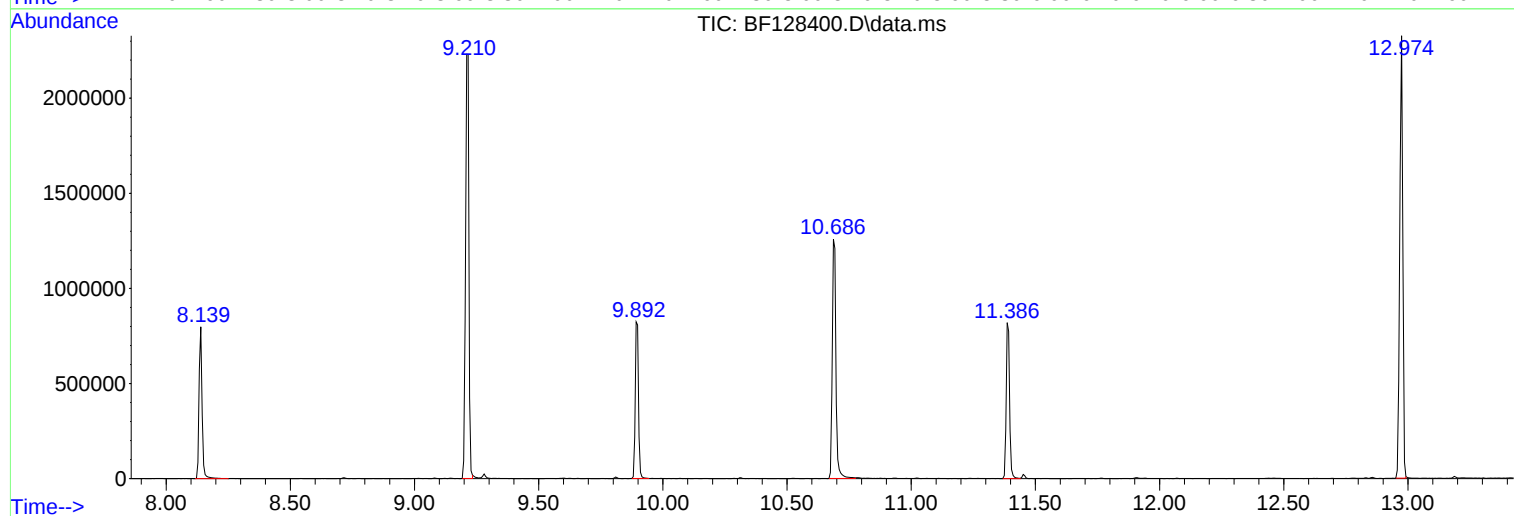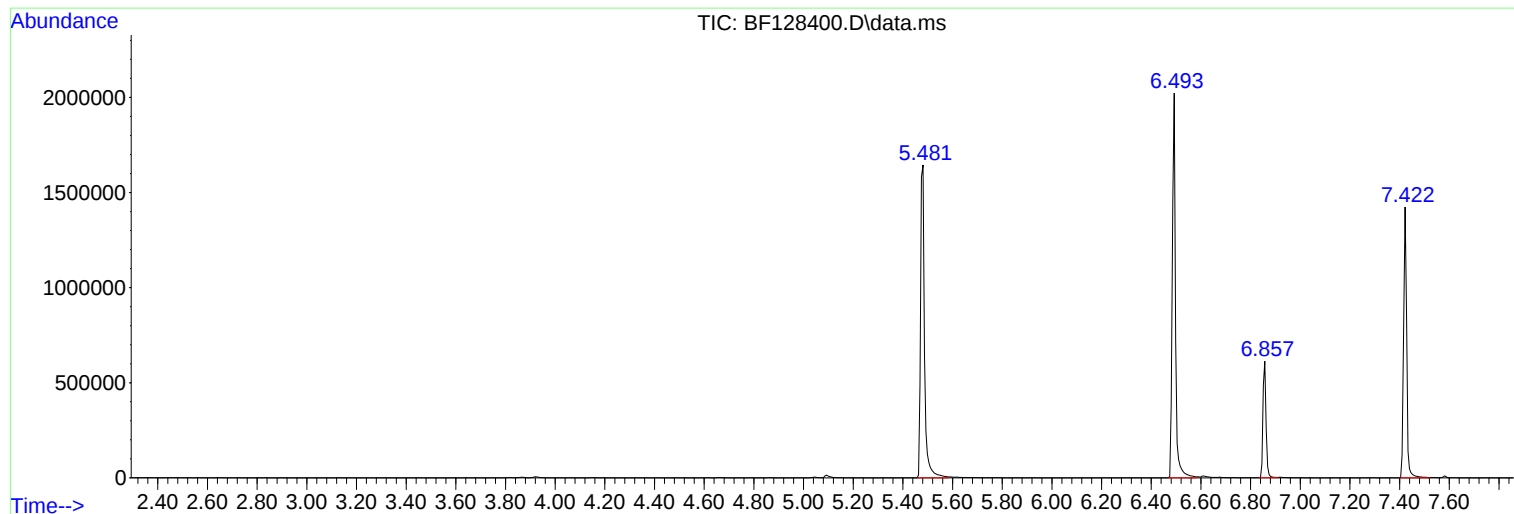

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052322\
Data File : BF128400.D
Acq On : 23 May 2022 15:04
Operator : CG\JU
Sample : N2873-11
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P032-SS001-0612-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052322\
Data File : BF128400.D
Acq On : 23 May 2022 15:04
Operator : CG\JU
Sample : N2873-11
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P032-SS001-0612-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------