

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052322\
 Data File : BF128401.D
 Acq On : 23 May 2022 15:34
 Operator : CG\JU
 Sample : N2982-02
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 P-2

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128401.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.092	474	477	488	rBV	17389	24253	1.16%	0.160%
2	5.481	539	543	564	rBV	1976213	1951995	93.23%	12.847%
3	6.492	711	715	733	rBV	2159294	1957083	93.47%	12.881%
4	6.857	773	777	786	rBV	653691	574625	27.45%	3.782%
5	7.422	869	873	886	rBV	1483956	1307179	62.43%	8.603%
6	8.139	991	995	1004	rBV	882468	729463	34.84%	4.801%
7	9.210	1174	1177	1181	rBV	2246317	2093719	100.00%	13.780%
8	9.280	1186	1189	1194	rVB	27112	22661	1.08%	0.149%
9	9.898	1290	1294	1306	rBV	906156	828460	39.57%	5.452%
10	10.692	1425	1429	1443	rBV	1414862	1377948	65.81%	9.069%
11	11.392	1544	1548	1555	rBV	906255	864470	41.29%	5.689%
12	12.974	1813	1817	1820	rBV	2324564	2083352	99.50%	13.712%
13	13.915	1970	1977	1989	rBV10	12477	43693	2.09%	0.288%
14	14.039	1994	1998	2009	rBV	749653	688845	32.90%	4.534%
15	14.127	2009	2013	2019	rBV	128653	130053	6.21%	0.856%
16	15.527	2246	2251	2262	rVB2	393141	516346	24.66%	3.398%




Sum of corrected areas: 15194145

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052322\
Data File : BF128401.D
Acq On : 23 May 2022 15:34
Operator : CG\JU
Sample : N2982-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P-2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

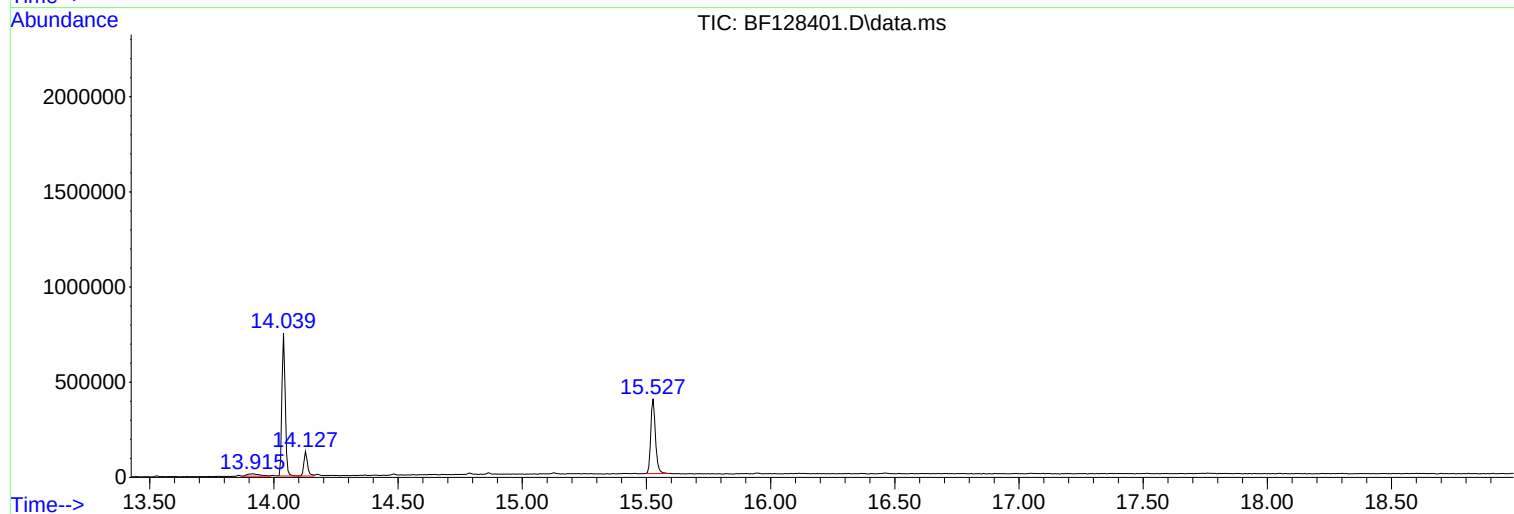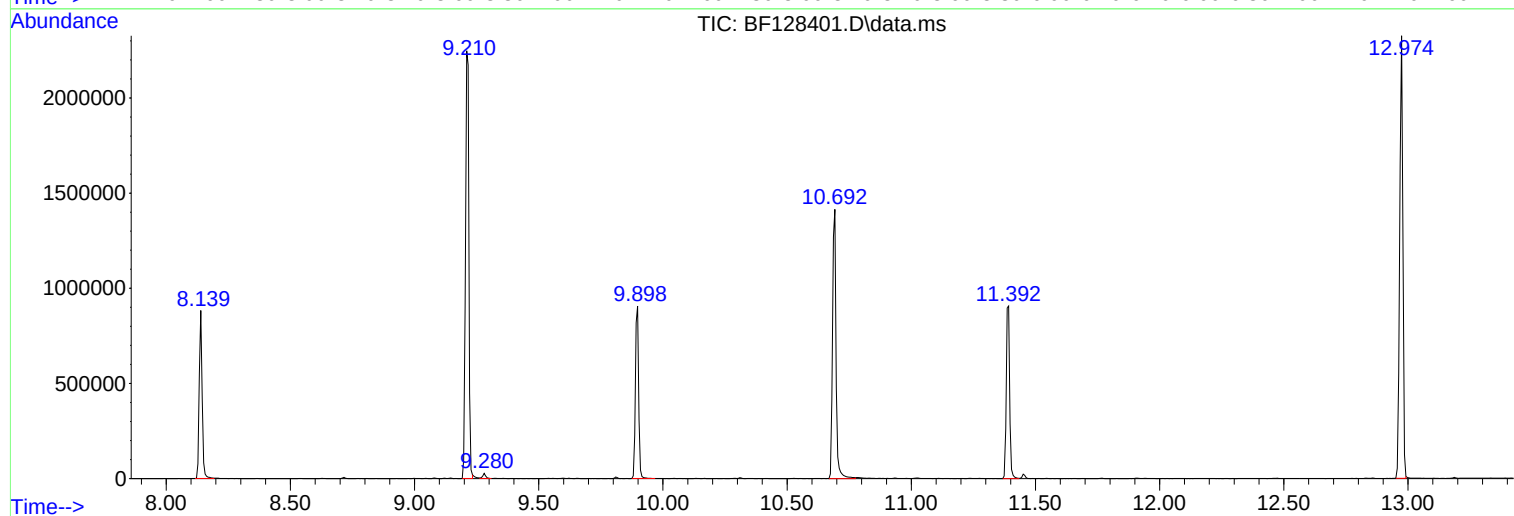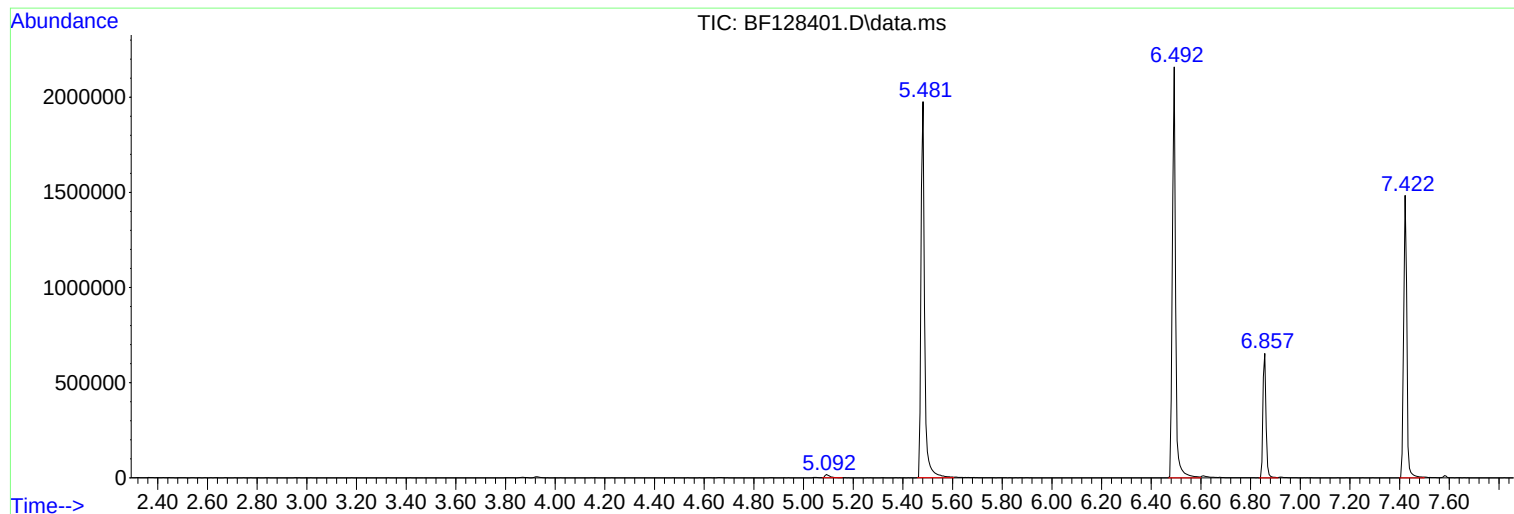

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052322\
Data File : BF128401.D
Acq On : 23 May 2022 15:34
Operator : CG\JU
Sample : N2982-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P-2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052322\
Data File : BF128401.D
Acq On : 23 May 2022 15:34
Operator : CG\JU
Sample : N2982-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P-2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------