

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052322\
 Data File : BF128402.D
 Acq On : 23 May 2022 16:04
 Operator : CG\JU
 Sample : N2873-14
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 P032-SS001-2430-01

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128402.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.481	539	543	568	rBV	1840322	1842810	88.59%	12.359%
2	6.492	711	715	733	rBV	1984709	1857799	89.31%	12.460%
3	6.857	773	777	786	rBV	649982	580732	27.92%	3.895%
4	7.422	869	873	886	rBV	1419720	1241590	59.69%	8.327%
5	8.139	991	995	1008	rBV	856478	750290	36.07%	5.032%
6	9.210	1173	1177	1181	rBV	2295746	2016614	96.95%	13.525%
7	9.892	1290	1293	1302	rBV	910458	846254	40.68%	5.676%
8	10.686	1425	1428	1443	rBV	1330594	1339838	64.41%	8.986%
9	11.386	1544	1547	1556	rBV	966628	895471	43.05%	6.006%
10	12.974	1813	1817	1820	rBV	2387398	2080130	100.00%	13.951%
11	13.910	1969	1976	1986	rBV6	26046	86719	4.17%	0.582%
12	14.039	1994	1998	2009	rBV	840730	716487	34.44%	4.805%
13	14.127	2009	2013	2019	rBV	108664	107597	5.17%	0.722%
14	15.527	2246	2251	2260	rVB	422443	548193	26.35%	3.677%

Sum of corrected areas: 14910524

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052322\
Data File : BF128402.D
Acq On : 23 May 2022 16:04
Operator : CG\JU
Sample : N2873-14
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P032-SS001-2430-01










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 n-Nonadecanol-1 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.910	2.42 ng	86719	Chrysene-d12	14.039

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	n-Nonadecanol-1	284	C19H40O	001454-84-8	95		
2	1-Heneicosanol	312	C21H44O	015594-90-8	95		
3	Trifluoroacetic acid, pentadecyl...	324	C17H31F3O2	959010-23-2	95		
4	Pentafluoropropionic acid, penta...	374	C18H31F5O2	959092-08-1	95		
5	Behenic alcohol	326	C22H46O	000661-19-8	94		

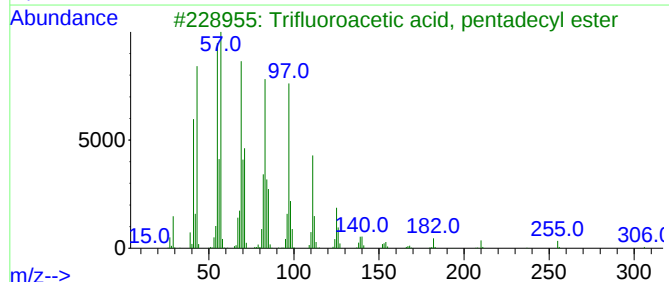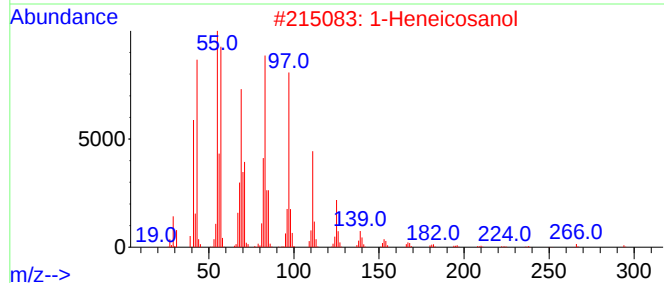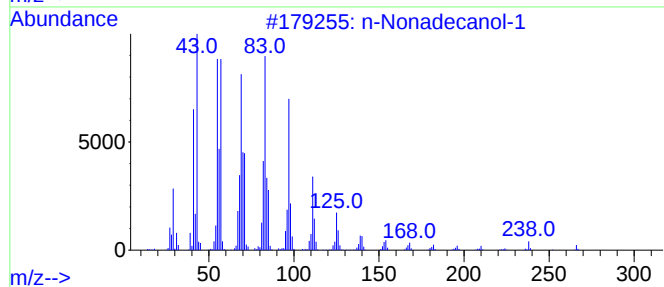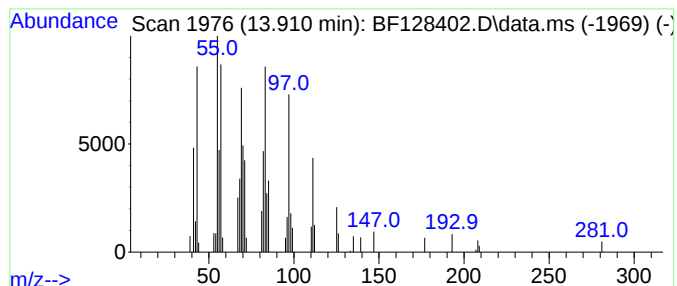

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052322\
Data File : BF128402.D
Acq On : 23 May 2022 16:04
Operator : CG\JU
Sample : N2873-14
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P032-SS001-2430-01









Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Triphenylphosphine oxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
14.127	3.00 ng	107597	Chrysene-d12	14.039

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Triphenylphosphine oxide	278	C18H15OP	000791-28-6	98
2			(E)-7-Benzylidene-1-azabicyclo[3...]	293	C15H19N03S	1000483-83-4	91
3			Formaldehyde, (triphenylphosphor...]	304	C19H17N2P	015990-54-2	64
4			Cobalt,(.eta.<5>-2,4-cyclopentad...	277	C16H15BCo	036682-12-9	38
5			2-Phenyl-6-(trifluoromethyl)-1H-...	277	C15H10F3NO	1000387-59-3	37

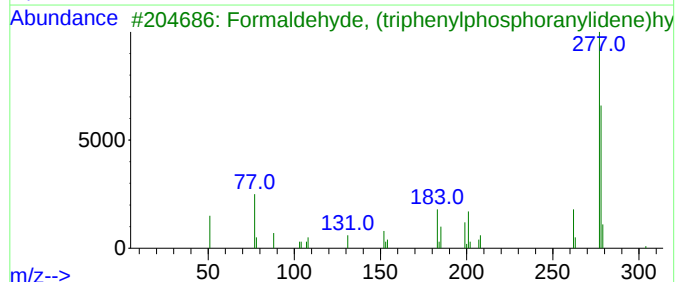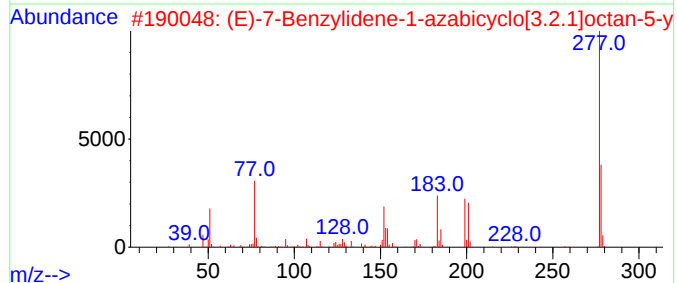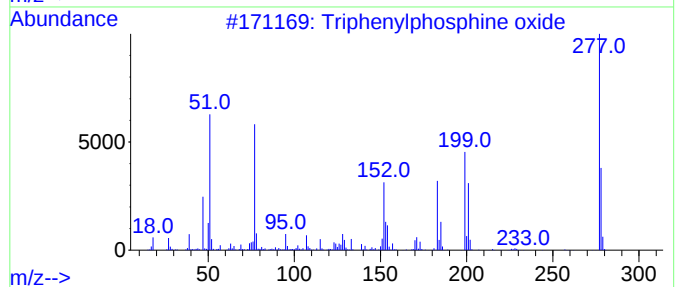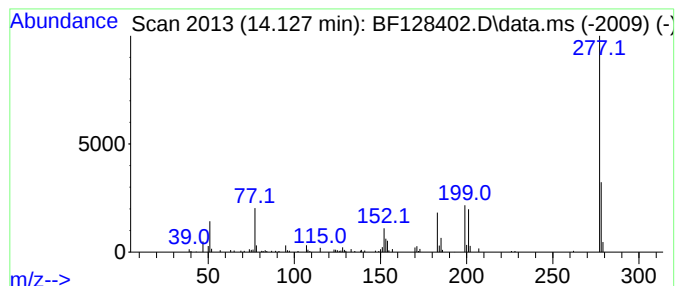

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052322\
Data File : BF128402.D
Acq On : 23 May 2022 16:04
Operator : CG\JU
Sample : N2873-14
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P032-SS001-2430-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
n-Nonadecanol-1	13.910	2.4	ng	86719	5	14.039	716487	20.0
Triphenylphosph...	14.127	3.0	ng	107597	5	14.039	716487	20.0