

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052322\
 Data File : BF128407.D
 Acq On : 23 May 2022 18:40
 Operator : CG\JU
 Sample : N2873-02
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 P029-SS001-1218-01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128407.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.481	540	543	567	rBV	2203136	2308643	87.04%	12.158%
2	6.492	711	715	732	rBV	2452810	2338016	88.15%	12.313%
3	6.857	773	777	787	rBV	758099	726861	27.41%	3.828%
4	7.422	869	873	876	rBV	1715065	1563166	58.94%	8.232%
5	8.139	991	995	1010	rBV	992254	942247	35.53%	4.962%
6	9.210	1173	1177	1181	rBV	2691672	2652250	100.00%	13.968%
7	9.892	1290	1293	1297	rBV	1189776	1068984	40.30%	5.630%
8	10.686	1425	1428	1442	rBV	1708800	1700008	64.10%	8.953%
9	11.386	1544	1547	1556	rBV	1238300	1131874	42.68%	5.961%
10	11.904	1630	1635	1640	rBV	26166	28663	1.08%	0.151%
11	12.974	1813	1817	1820	rBV	2930600	2633650	99.30%	13.870%
12	13.910	1969	1976	1987	rBV3	106278	313272	11.81%	1.650%
13	14.039	1994	1998	2005	rVB	910617	839142	31.64%	4.419%
14	14.127	2009	2013	2018	rBV	33097	39173	1.48%	0.206%
15	14.780	2120	2124	2132	rBV3	38749	58063	2.19%	0.306%
16	15.521	2245	2250	2260	rBV	480378	644153	24.29%	3.392%




Sum of corrected areas: 18988165

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052322\
Data File : BF128407.D
Acq On : 23 May 2022 18:40
Operator : CG\JU
Sample : N2873-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P029-SS001-1218-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

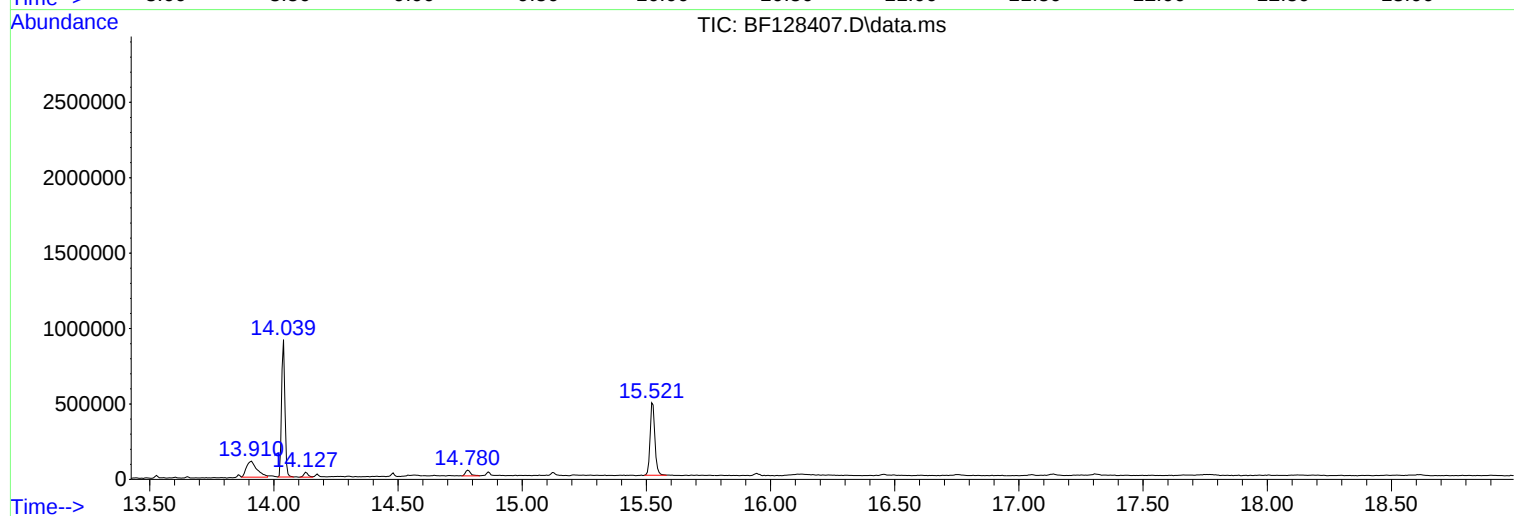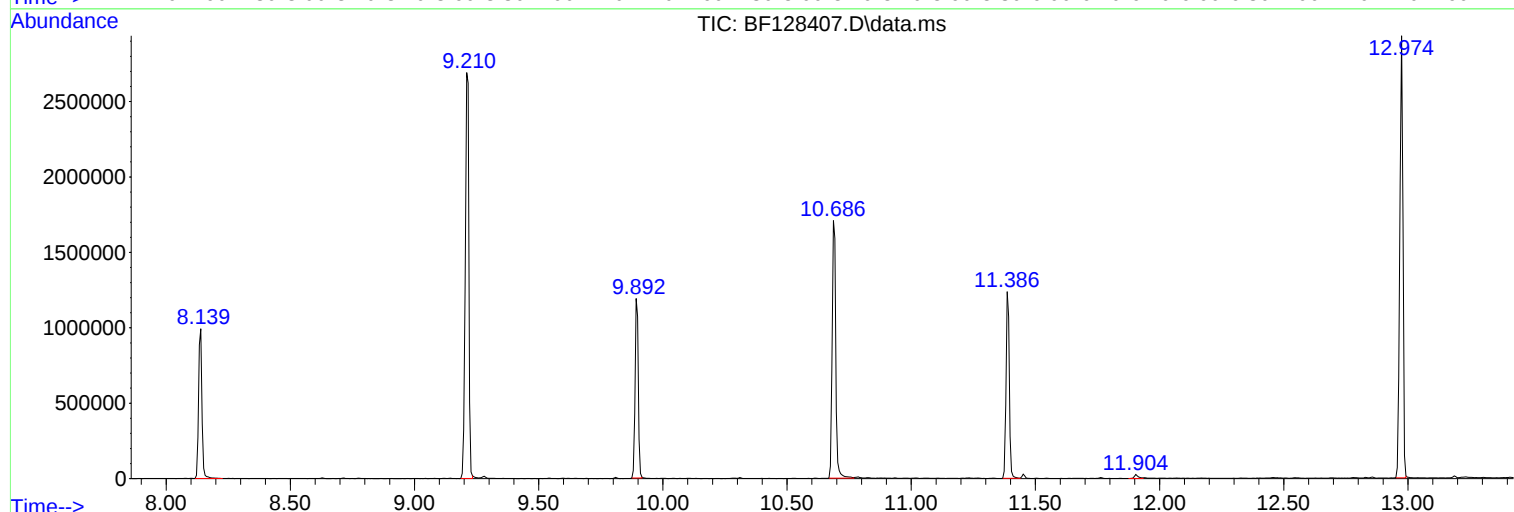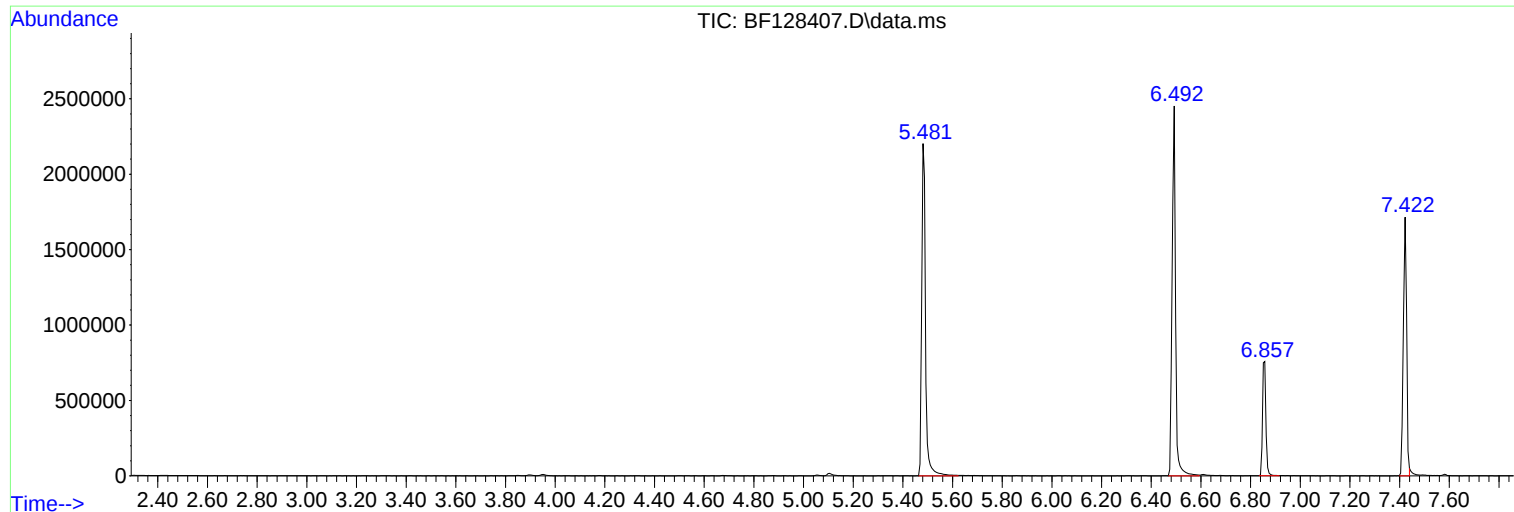

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052322\
Data File : BF128407.D
Acq On : 23 May 2022 18:40
Operator : CG\JU
Sample : N2873-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P029-SS001-1218-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052322\
Data File : BF128407.D
Acq On : 23 May 2022 18:40
Operator : CG\JU
Sample : N2873-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P029-SS001-1218-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------