

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052322\
 Data File : BF128408.D
 Acq On : 23 May 2022 19:10
 Operator : CG\JU
 Sample : N2876-21
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 P007-SS014-0006-01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128408.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.092	474	477	487	rBV	24576	34075	1.44%	0.198%
2	5.481	539	543	559	rBV	2045622	1990134	84.24%	11.557%
3	6.492	711	715	729	rBV	2075181	2002403	84.76%	11.628%
4	6.857	773	777	785	rBV	768209	723696	30.63%	4.203%
5	7.422	869	873	885	rBV	1506861	1355834	57.39%	7.873%
6	7.581	896	900	905	rVB	56502	50202	2.12%	0.292%
7	8.139	991	995	1011	rBV	1052629	950825	40.25%	5.521%
8	9.210	1173	1177	1181	rBV	2460740	2321482	98.26%	13.481%
9	9.280	1185	1189	1194	rVB	33300	30087	1.27%	0.175%
10	9.898	1290	1294	1297	rBV	1159327	1074597	45.48%	6.240%
11	10.686	1425	1428	1437	rBV	1434989	1424426	60.29%	8.272%
12	11.386	1544	1547	1555	rBV	1286123	1143820	48.41%	6.642%
13	12.974	1813	1817	1820	rBV	2619973	2362548	100.00%	13.719%
14	13.904	1969	1975	1994	rBV6	67423	240073	10.16%	1.394%
15	14.039	1994	1998	2005	rBV	914905	829022	35.09%	4.814%
16	14.127	2009	2013	2018	rBV	31042	34829	1.47%	0.202%
17	15.521	2246	2250	2264	rVB	466590	652531	27.62%	3.789%




Sum of corrected areas: 17220584

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052322\
Data File : BF128408.D
Acq On : 23 May 2022 19:10
Operator : CG\JU
Sample : N2876-21
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P007-SS014-0006-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

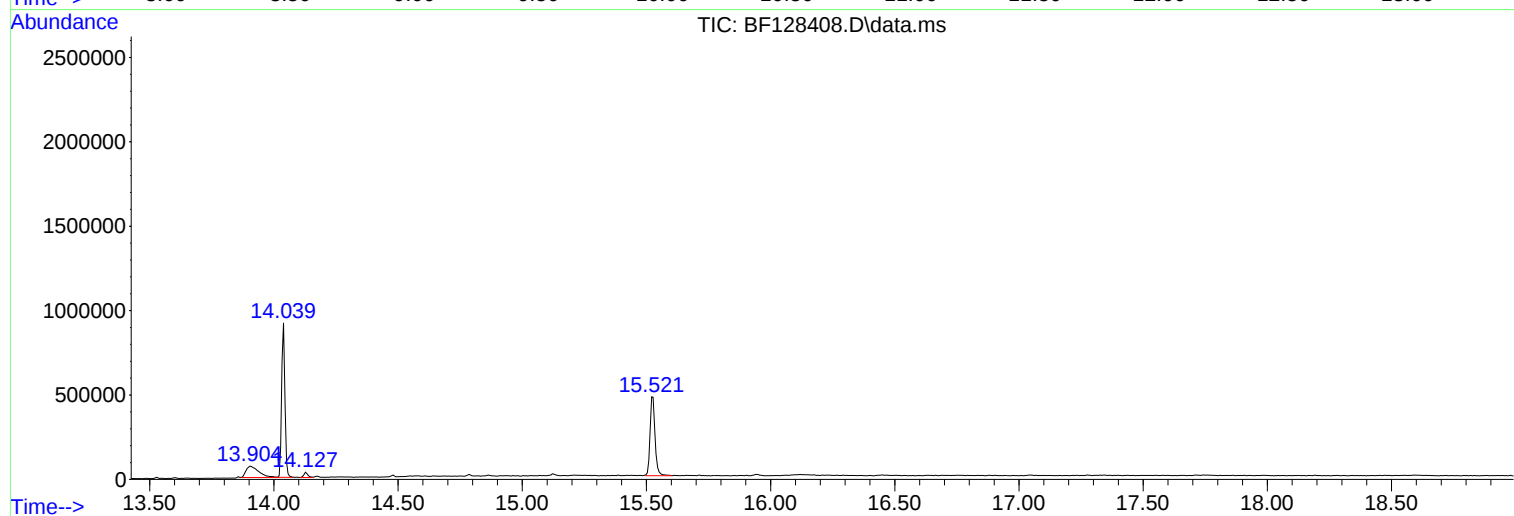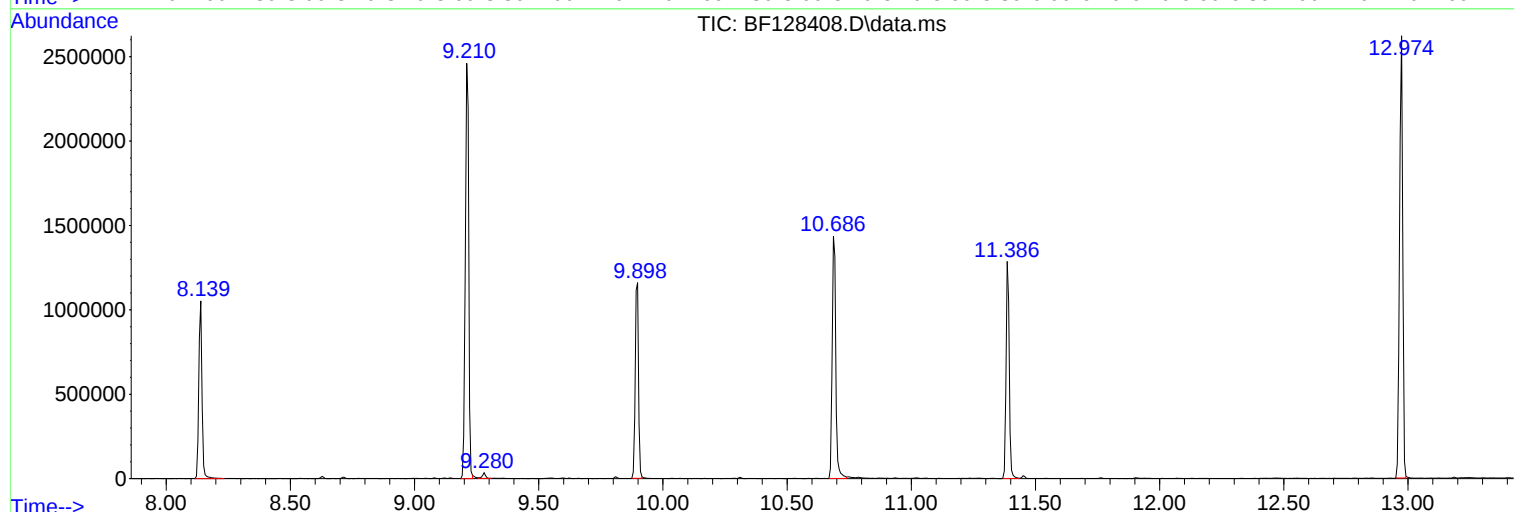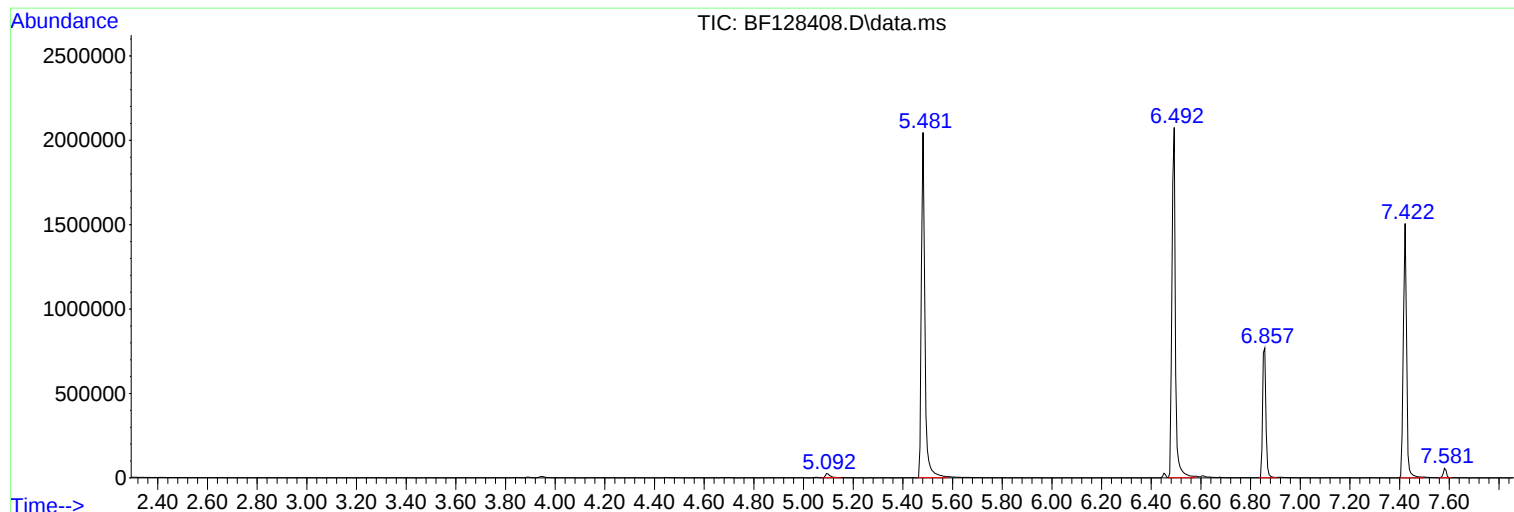

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052322\
Data File : BF128408.D
Acq On : 23 May 2022 19:10
Operator : CG\JU
Sample : N2876-21
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P007-SS014-0006-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052322\
Data File : BF128408.D
Acq On : 23 May 2022 19:10
Operator : CG\JU
Sample : N2876-21
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P007-SS014-0006-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------