

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052322\
 Data File : BF128409.D
 Acq On : 23 May 2022 19:40
 Operator : CG\JU
 Sample : N2873-13
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 P032-SS001-1824-01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128409.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.104	476	479	488	rVB	20473	31145	1.14%	0.164%
2	5.481	540	543	575	rBV	2309145	2396177	87.57%	12.580%
3	6.492	711	715	732	rBV	2564254	2447752	89.45%	12.851%
4	6.857	773	777	785	rBV	779218	732197	26.76%	3.844%
5	7.422	869	873	876	rBV	1792527	1628943	59.53%	8.552%
6	8.139	991	995	1007	rBV	1001000	955175	34.91%	5.015%
7	9.210	1173	1177	1181	rBV	2765167	2736363	100.00%	14.366%
8	9.898	1290	1294	1297	rBV	1121703	1073910	39.25%	5.638%
9	10.692	1425	1429	1443	rBV	1702765	1757692	64.23%	9.228%
10	11.386	1544	1547	1555	rBV	1243824	1122867	41.04%	5.895%
11	11.451	1555	1558	1565	rVB2	34317	28983	1.06%	0.152%
12	12.974	1813	1817	1820	rBV	2934326	2605147	95.20%	13.678%
13	13.910	1969	1976	1977	rBV3	29261	43478	1.59%	0.228%
14	14.039	1994	1998	2006	rVB	834128	795770	29.08%	4.178%
15	14.127	2009	2013	2018	rBV	34789	38250	1.40%	0.201%
16	15.521	2245	2250	2264	rVB	470791	652996	23.86%	3.428%




Sum of corrected areas: 19046845

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052322\
Data File : BF128409.D
Acq On : 23 May 2022 19:40
Operator : CG\JU
Sample : N2873-13
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P032-SS001-1824-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

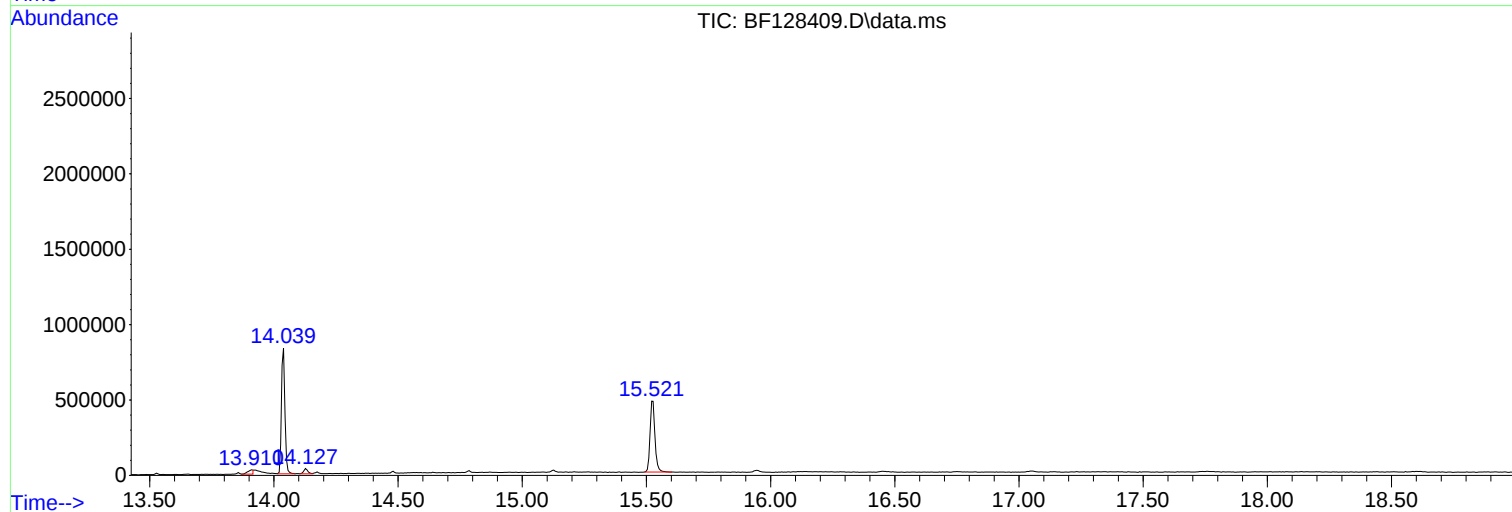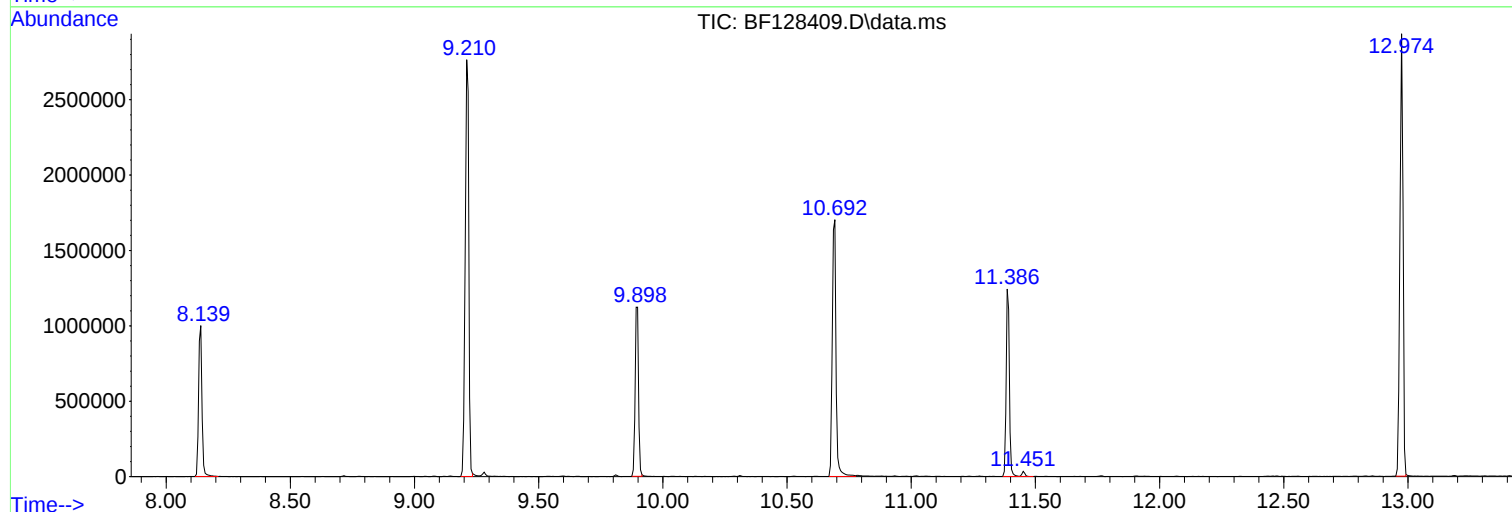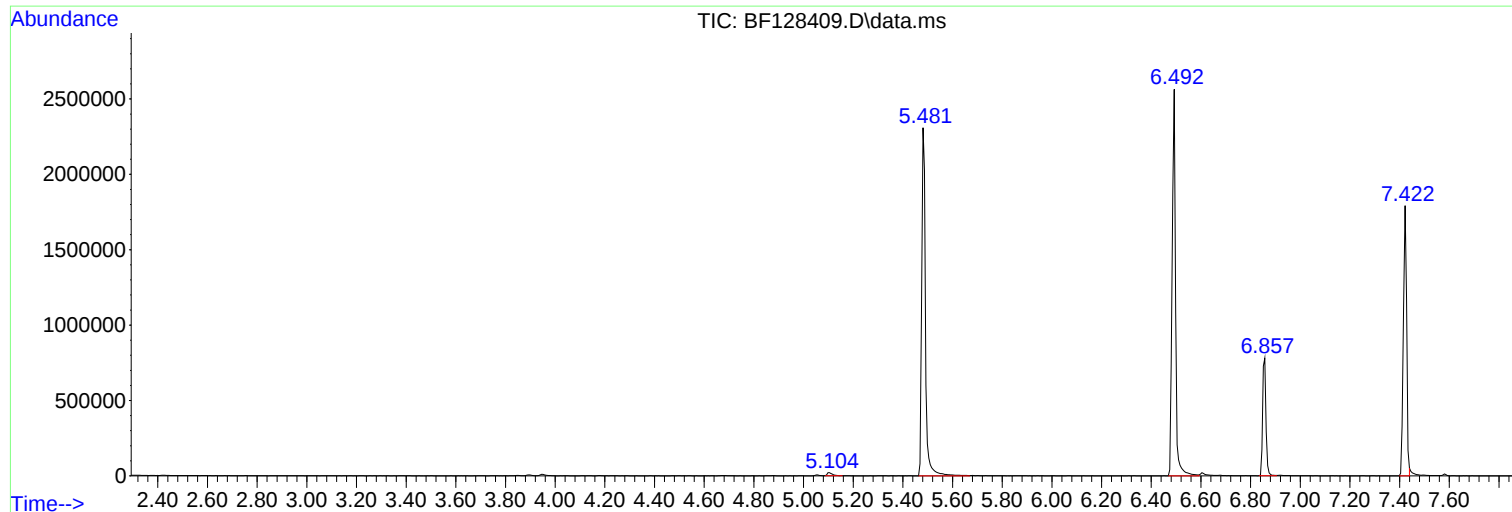

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052322\
Data File : BF128409.D
Acq On : 23 May 2022 19:40
Operator : CG\JU
Sample : N2873-13
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P032-SS001-1824-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052322\
Data File : BF128409.D
Acq On : 23 May 2022 19:40
Operator : CG\JU
Sample : N2873-13
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P032-SS001-1824-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------