

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052322\
 Data File : BF128411.D
 Acq On : 23 May 2022 20:40
 Operator : CG\JU
 Sample : N2873-07
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 P031-SS001-1218-01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128411.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.098	475	478	492	rBV	44801	63173	2.28%	0.332%
2	5.481	540	543	572	rBV	2362974	2478165	89.52%	13.038%
3	6.492	711	715	718	rBV	2677742	2469209	89.20%	12.991%
4	6.857	773	777	783	rBV	788752	732851	26.47%	3.856%
5	7.422	869	873	876	rBV	1789677	1678709	60.64%	8.832%
6	8.139	991	995	1008	rBV	1010895	916761	33.12%	4.823%
7	9.210	1173	1177	1181	rBV	2787144	2768275	100.00%	14.565%
8	9.892	1290	1293	1297	rBV	1175413	1075548	38.85%	5.659%
9	10.692	1425	1429	1443	rBV	1779509	1768842	63.90%	9.306%
10	11.386	1544	1547	1555	rBV	1182737	1064147	38.44%	5.599%
11	12.974	1813	1817	1820	rBV	2821956	2497493	90.22%	13.140%
12	13.921	1970	1978	1990	rBV8	25138	98552	3.56%	0.519%
13	14.039	1994	1998	2007	rVB	781360	712571	25.74%	3.749%
14	14.127	2009	2013	2018	rVV	33336	35731	1.29%	0.188%
15	15.527	2244	2251	2264	rVB	480410	646776	23.36%	3.403%

Sum of corrected areas: 19006803

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052322\
Data File : BF128411.D
Acq On : 23 May 2022 20:40
Operator : CG\JU
Sample : N2873-07
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P031-SS001-1218-01










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Acetic acid, chloro-, octad... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.921	2.77 ng	98552	Chrysene-d12	14.039

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Acetic acid, chloro-, octadecyl ...	346	C20H39ClO2	005348-82-3	94
2			1-Nonadecene	266	C19H38	018435-45-5	91
3			3-Chloropropionic acid, heptadec...	346	C20H39ClO2	1000283-05-1	91
4			9-Eicosene, (E)-	280	C20H40	074685-29-3	87
5			Pentadecafluorooctanoic acid, oc...	666	C26H37F15O2	1000406-04-8	87

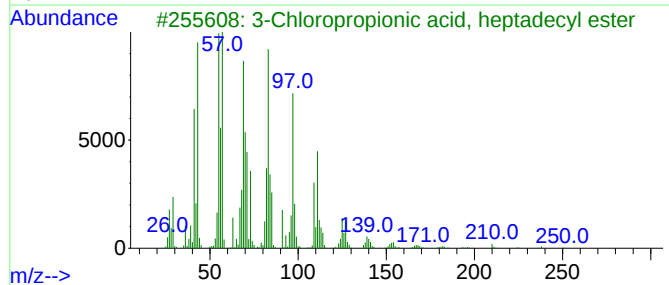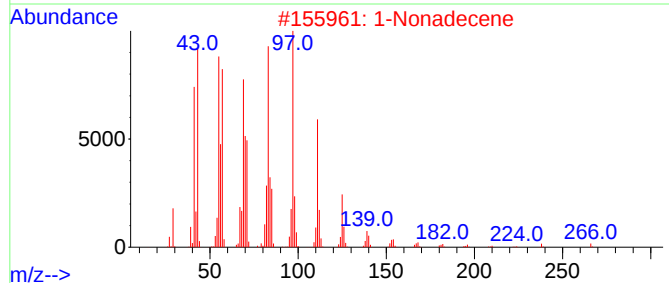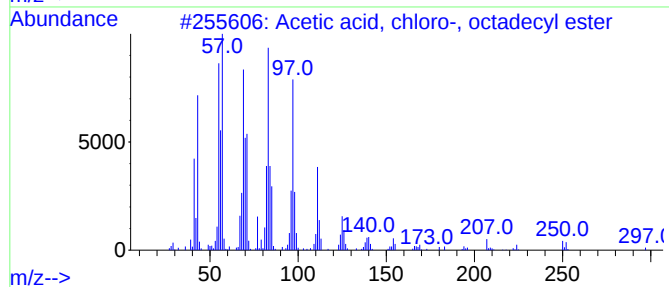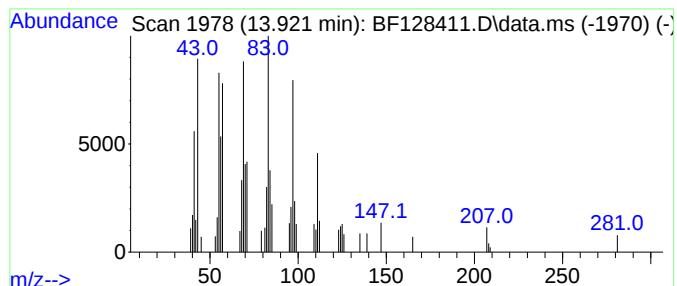

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052322\
Data File : BF128411.D
Acq On : 23 May 2022 20:40
Operator : CG\JU
Sample : N2873-07
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P031-SS001-1218-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Acetic acid, ch...	13.921	2.8	ng	98552	5	14.039	712571	20.0