

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052322\
 Data File : BF128412.D
 Acq On : 23 May 2022 21:10
 Operator : CG\JU
 Sample : N2873-06
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 P031-SS001-0612-01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128412.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.104	476	479	489	rBV	18012	28321	1.08%	0.153%
2	5.481	540	543	572	rBV	2331444	2376696	90.26%	12.832%
3	6.492	711	715	732	rBV	2509430	2421410	91.95%	13.073%
4	6.857	773	777	785	rBV	765675	718394	27.28%	3.879%
5	7.422	869	873	885	rBV	1764333	1652140	62.74%	8.920%
6	8.139	991	995	1011	rBV	1007321	940361	35.71%	5.077%
7	9.210	1173	1177	1181	rBV	2757125	2633277	100.00%	14.217%
8	9.280	1186	1189	1194	rVB	36827	32538	1.24%	0.176%
9	9.892	1290	1293	1297	rBV	1125317	1054899	40.06%	5.695%
10	10.686	1425	1428	1443	rBV	1665007	1719192	65.29%	9.282%
11	11.386	1544	1547	1556	rBV	1247917	1086401	41.26%	5.865%
12	12.974	1812	1817	1820	rBV	2651679	2383014	90.50%	12.866%
13	13.915	1970	1977	1989	rBV	21992	85416	3.24%	0.461%
14	14.039	1994	1998	2005	rVV	716817	685330	26.03%	3.700%
15	14.127	2009	2013	2018	rBV	30284	34576	1.31%	0.187%
16	15.521	2245	2250	2261	rVB	493005	670272	25.45%	3.619%




Sum of corrected areas: 18522237

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052322\
Data File : BF128412.D
Acq On : 23 May 2022 21:10
Operator : CG\JU
Sample : N2873-06
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P031-SS001-0612-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

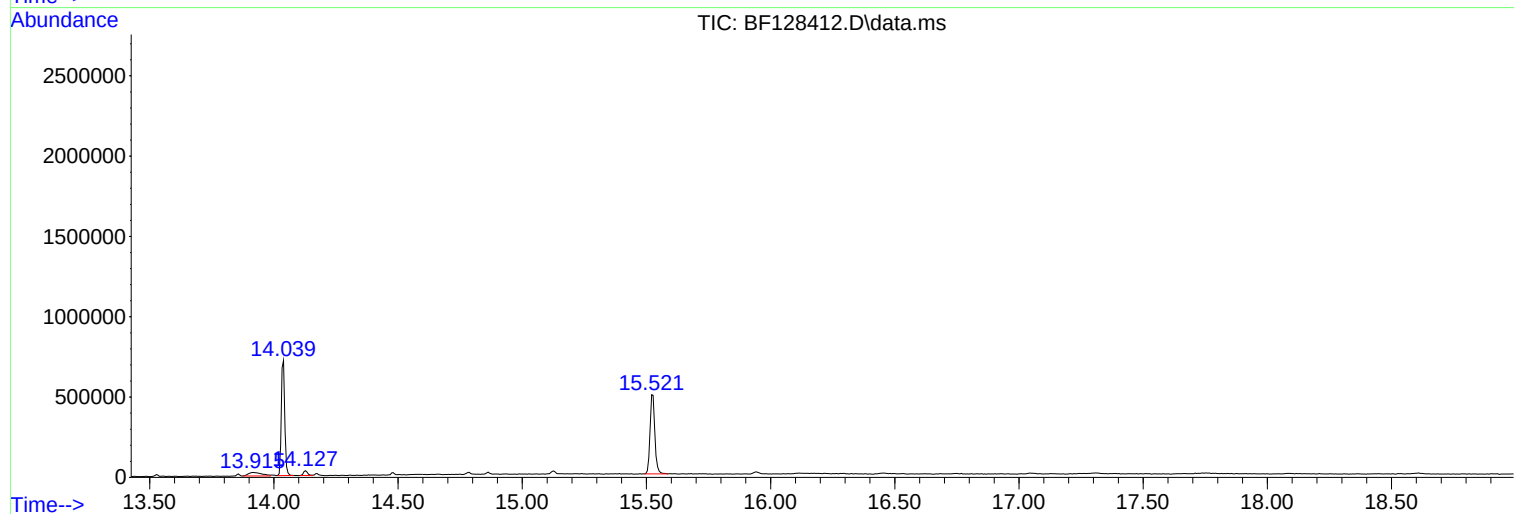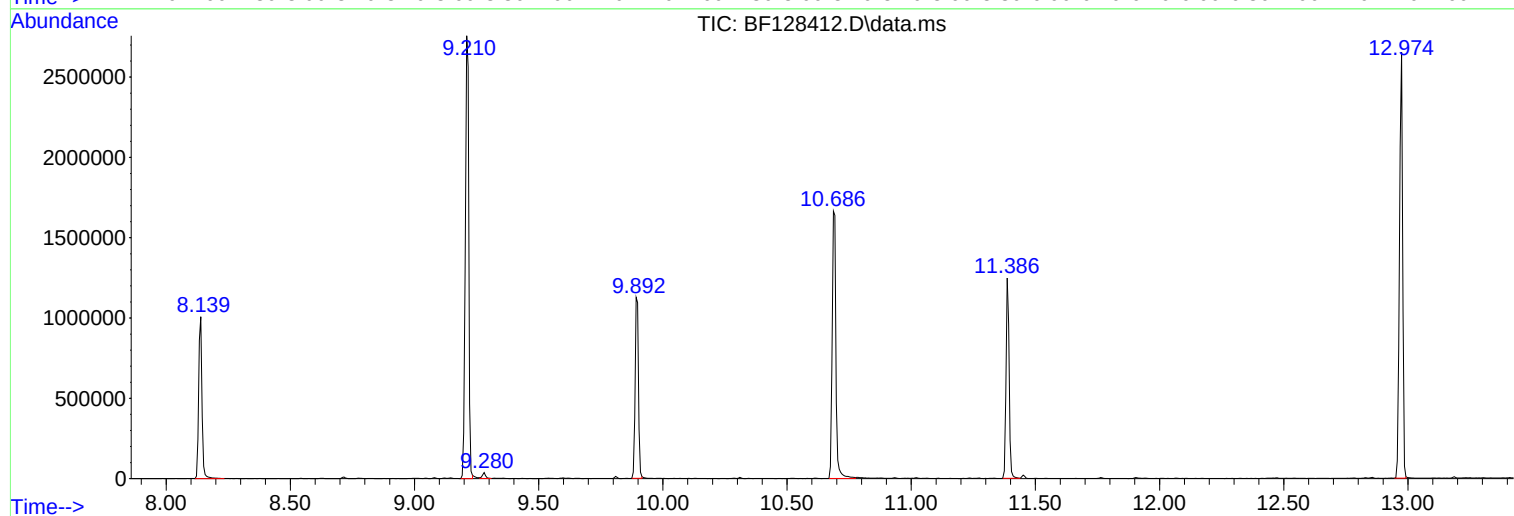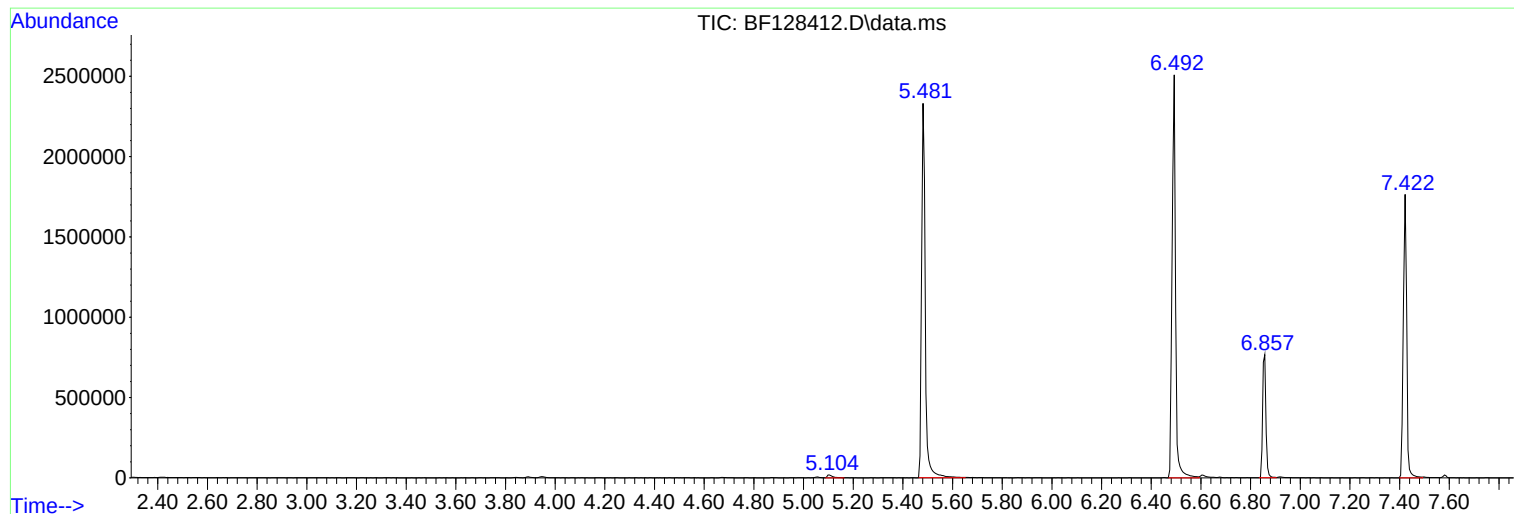

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052322\
Data File : BF128412.D
Acq On : 23 May 2022 21:10
Operator : CG\JU
Sample : N2873-06
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P031-SS001-0612-01










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 3-Chloropropionic acid, hep... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.916	2.49 ng	85416	Chrysene-d12	14.039

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			3-Chloropropionic acid, heptadec...	346	C20H39ClO2	1000283-05-1	94
2			Trichloroacetic acid, tridecyl e...	344	C15H27Cl3O2	074339-51-8	91
3			Trichloroacetic acid, pentadecyl...	372	C17H31Cl3O2	074339-53-0	91
4			1-Heptadecene	238	C17H34	006765-39-5	91
5			1-Nonadecene	266	C19H38	018435-45-5	91

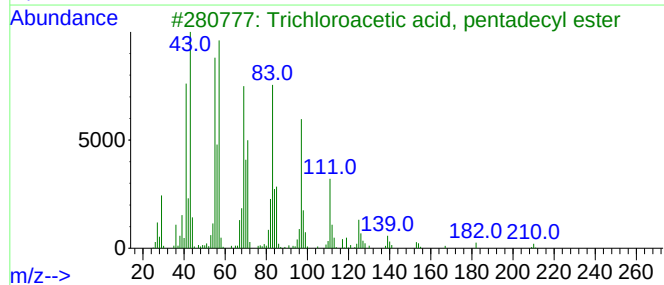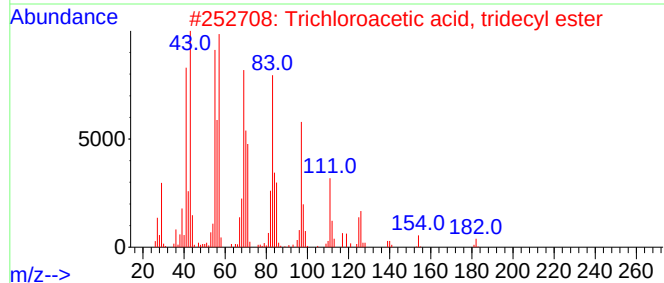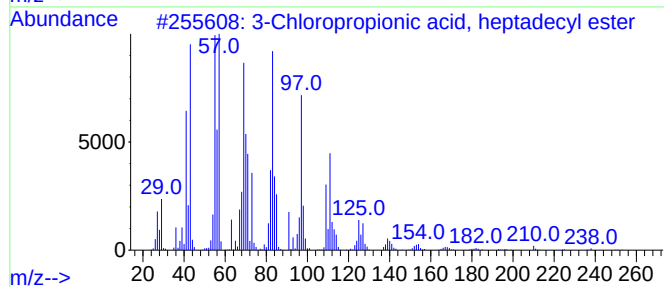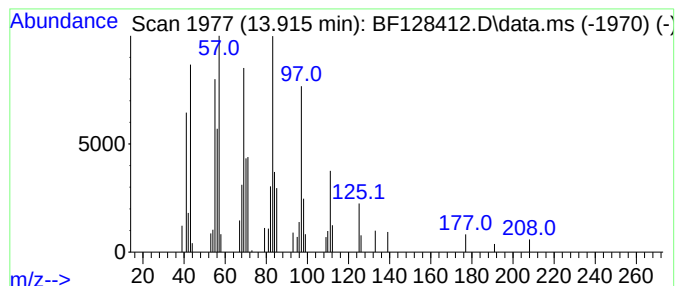

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052322\
Data File : BF128412.D
Acq On : 23 May 2022 21:10
Operator : CG\JU
Sample : N2873-06
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P031-SS001-0612-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
3-Chloropropion...	13.916	2.5	ng	85416	5	14.039	685330	20.0