

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052322\
 Data File : BF128417.D
 Acq On : 23 May 2022 23:38
 Operator : CG\JU
 Sample : N2875-06
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 P007-SS007-0006-01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128417.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.098	475	478	491	rBV	27053	38341	1.55%	0.228%
2	5.481	540	543	571	rBV	2198266	2301468	92.93%	13.658%
3	6.493	711	715	734	rBV	2430258	2308146	93.20%	13.698%
4	6.851	773	776	786	rBV	744122	678233	27.39%	4.025%
5	7.422	869	873	876	rBV	1713501	1524159	61.54%	9.045%
6	8.139	991	995	1014	rBV	915546	887710	35.85%	5.268%
7	9.210	1173	1177	1181	rBV	2613490	2476509	100.00%	14.697%
8	9.892	1290	1293	1297	rBV	1082181	971007	39.21%	5.762%
9	10.686	1425	1428	1442	rBV	1539951	1473340	59.49%	8.744%
10	11.386	1544	1547	1556	rBV	1093890	927764	37.46%	5.506%
11	12.969	1812	1816	1820	rBV	1985516	1911218	77.17%	11.342%
12	13.916	1970	1977	1989	rBV8	17052	69890	2.82%	0.415%
13	14.033	1994	1997	2007	rBV	593627	595617	24.05%	3.535%
14	14.127	2009	2013	2018	rBV	30111	34261	1.38%	0.203%
15	15.521	2245	2250	2264	rVB2	482868	653006	26.37%	3.875%




Sum of corrected areas: 16850669

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052322\
Data File : BF128417.D
Acq On : 23 May 2022 23:38
Operator : CG\JU
Sample : N2875-06
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P007-SS007-0006-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

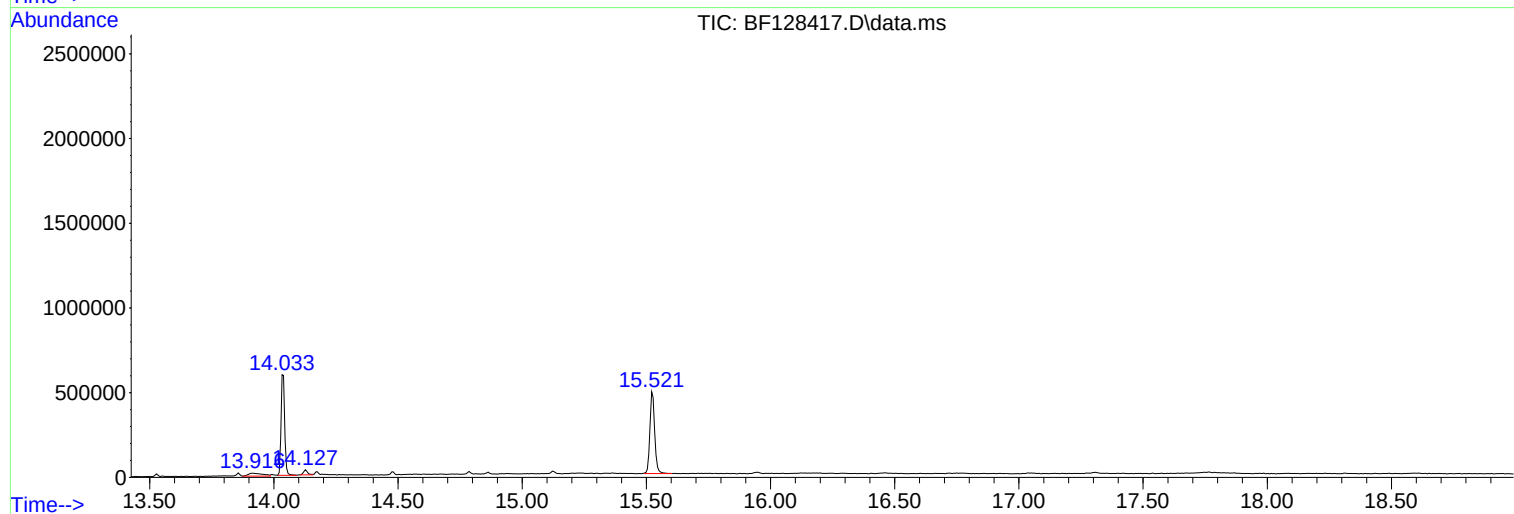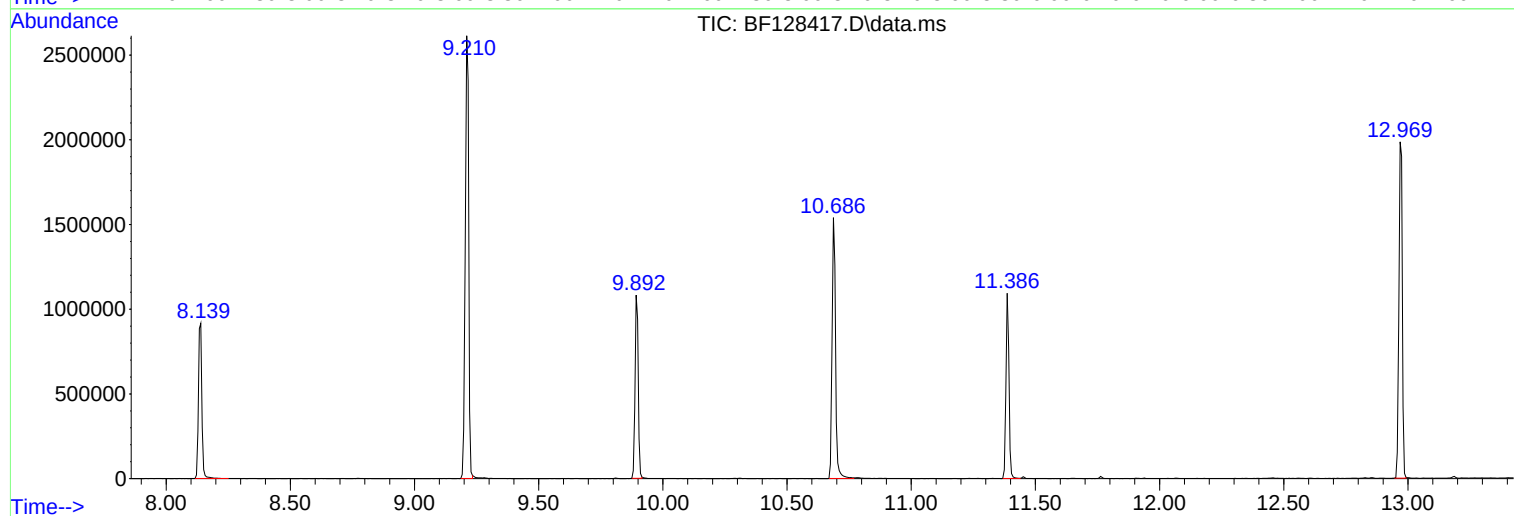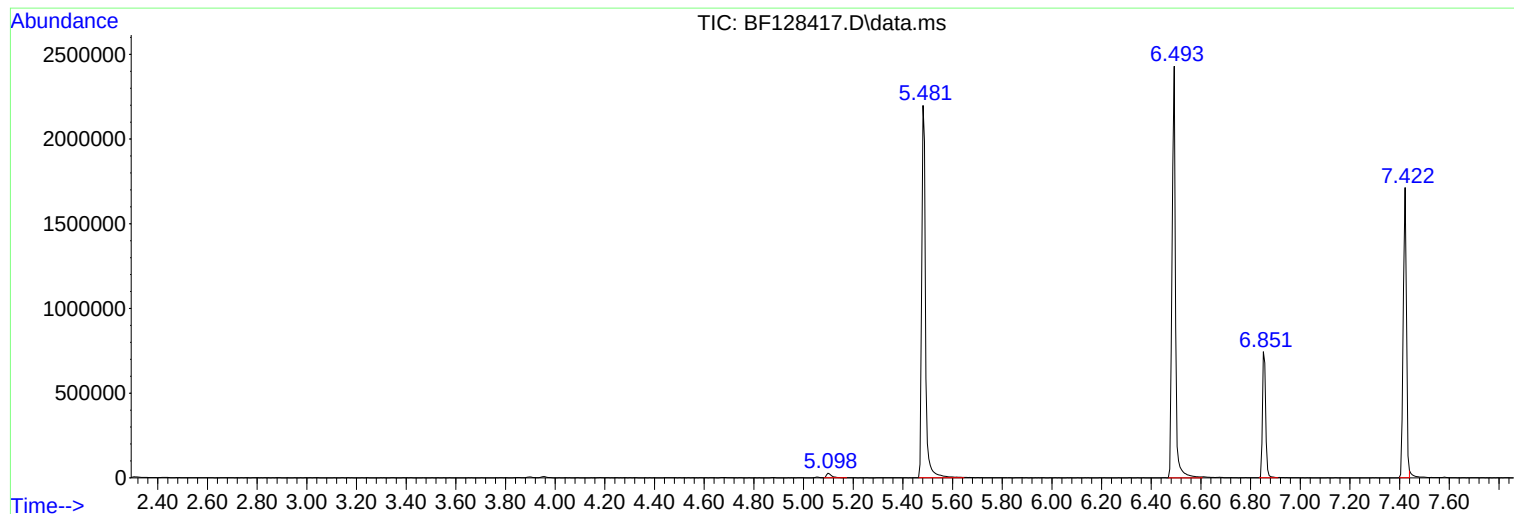

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052322\
Data File : BF128417.D
Acq On : 23 May 2022 23:38
Operator : CG\JU
Sample : N2875-06
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P007-SS007-0006-01










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 1-Eicosanol Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.916	2.35 ng	69890	Chrysene-d12	14.039

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			1-Eicosanol	298	C20H42O	000629-96-9	81
2			Carbonic acid, octadecyl 2,2,2-t...	444	C21H39Cl3O3	1000314-56-3	76
3			Dichloroacetic acid, heptadecyl ...	366	C19H36Cl2O2	1000282-98-2	76
4			1-Octadecanol	270	C18H38O	000112-92-5	76
5			Eicosyl methyl ether	312	C21H44O	1000406-29-4	76

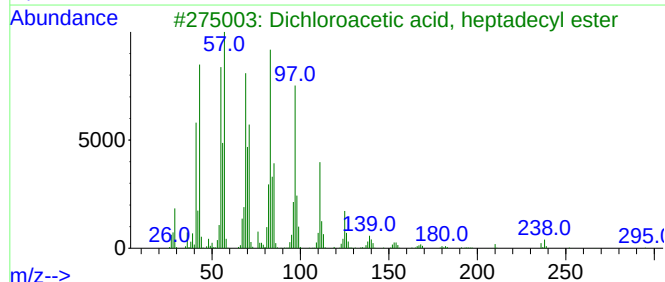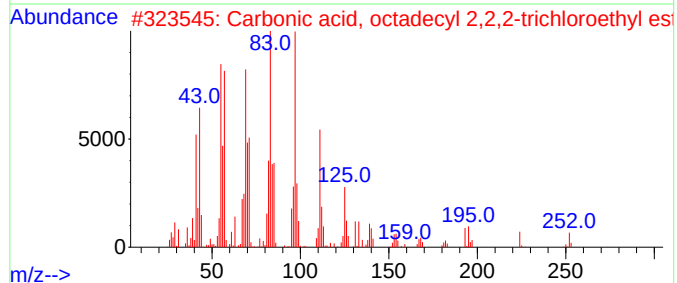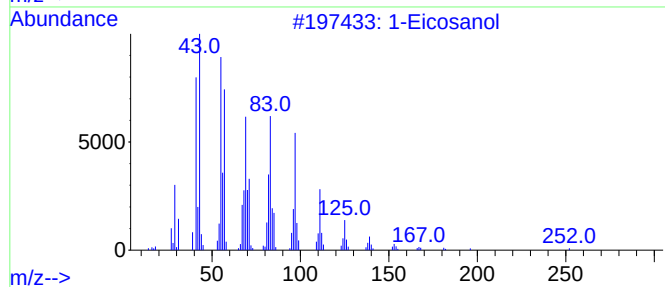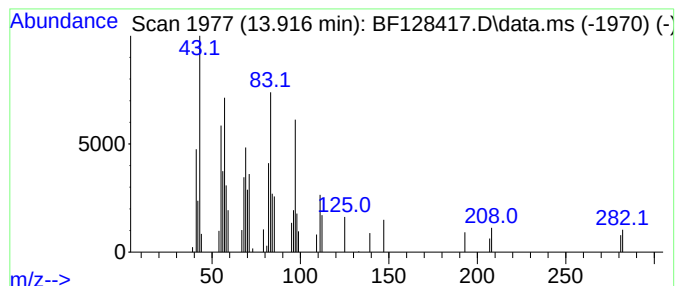

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052322\
Data File : BF128417.D
Acq On : 23 May 2022 23:38
Operator : CG\JU
Sample : N2875-06
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P007-SS007-0006-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
1-Eicosanol	13.916	2.4	ng	69890	5	14.039	595617	20.0