

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052322\
 Data File : BF128421.D
 Acq On : 24 May 2022 01:35
 Operator : CG\JU
 Sample : N2873-10
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 P032-SS001-0006-01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128421.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.099	475	478	488	rBV	21876	31062	1.26%	0.181%
2	5.481	540	543	566	rBV	2151194	2282989	92.33%	13.281%
3	6.493	711	715	732	rBV	2353114	2293616	92.76%	13.343%
4	6.851	773	776	786	rBV	761809	711324	28.77%	4.138%
5	7.422	869	873	876	rBV	1694727	1518765	61.42%	8.835%
6	8.140	991	995	998	rBV	991212	885891	35.83%	5.153%
7	9.210	1173	1177	1181	rBV	2633167	2472666	100.00%	14.384%
8	9.281	1186	1189	1195	rVB	32130	26972	1.09%	0.157%
9	9.892	1290	1293	1297	rBV	1040337	913053	36.93%	5.311%
10	10.686	1424	1428	1442	rBV	1341353	1248487	50.49%	7.263%
11	11.386	1543	1547	1556	rBV	910639	766841	31.01%	4.461%
12	12.969	1812	1816	1820	rBV	1862868	1701710	68.82%	9.899%
13	13.916	1971	1977	1986	rBV6	34572	121181	4.90%	0.705%
14	14.033	1994	1997	2008	rVB	688376	663632	26.84%	3.861%
15	14.127	2010	2013	2016	rVV	26993	29210	1.18%	0.170%
16	14.480	2070	2073	2077	rBV	38847	39865	1.61%	0.232%
17	14.786	2121	2125	2130	rBV2	28557	31281	1.27%	0.182%
18	15.121	2179	2182	2190	rVB	61762	77901	3.15%	0.453%
19	15.521	2244	2250	2258	rBV2	499426	663233	26.82%	3.858%
20	15.715	2280	2283	2290	rVB7	18433	27758	1.12%	0.161%
21	15.945	2318	2322	2327	rVB	50136	73833	2.99%	0.430%
22	16.751	2454	2459	2466	rVB3	62683	118675	4.80%	0.690%
23	17.309	2548	2554	2567	rVB3	133481	320174	12.95%	1.863%
24	18.086	2681	2686	2693	rBV10	30026	71896	2.91%	0.418%
25	18.609	2769	2775	2785	rVB7	36439	98155	3.97%	0.571%




Sum of corrected areas: 17190170

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052322\
Data File : BF128421.D
Acq On : 24 May 2022 01:35
Operator : CG\JU
Sample : N2873-10
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P032-SS001-0006-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

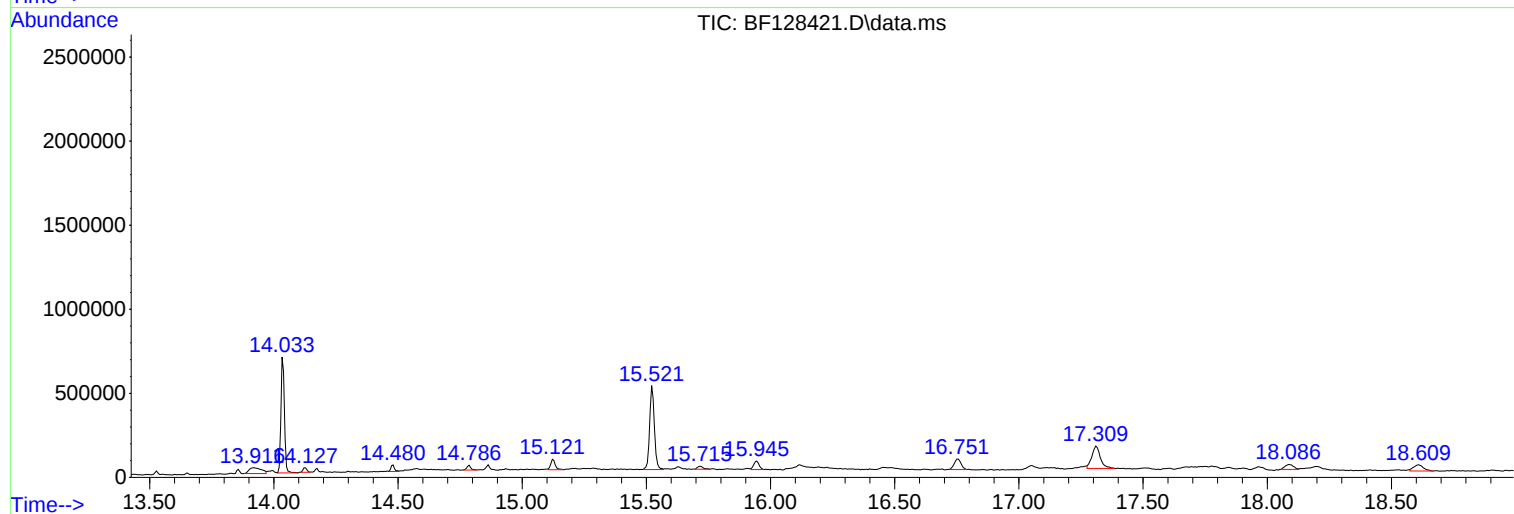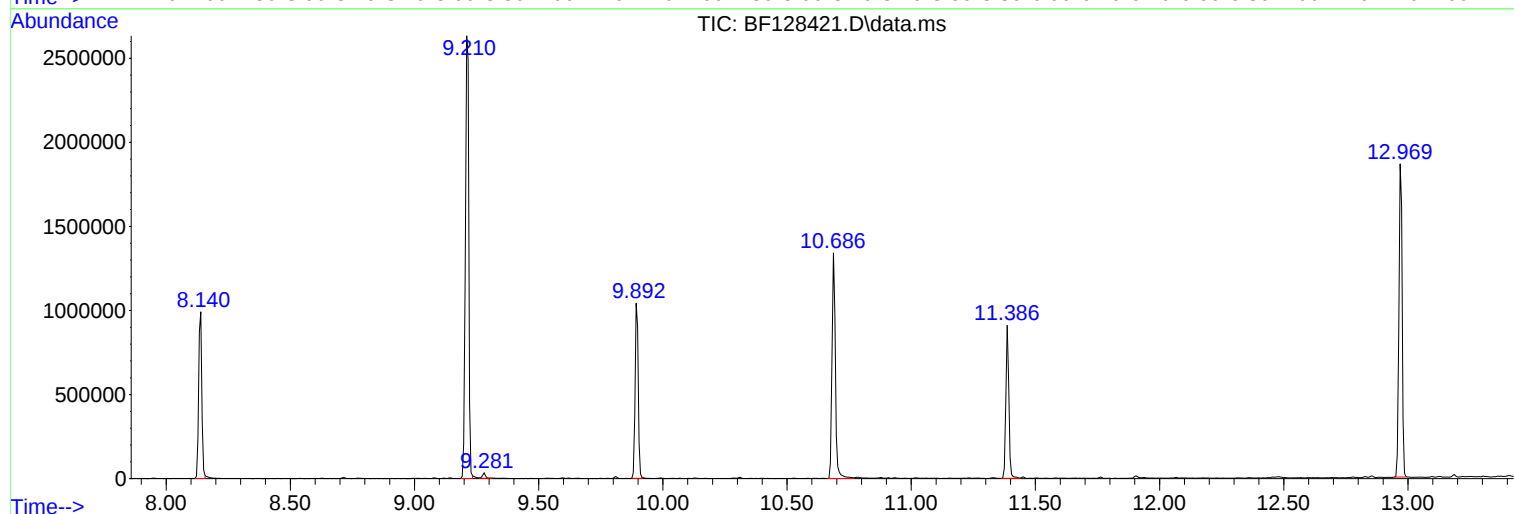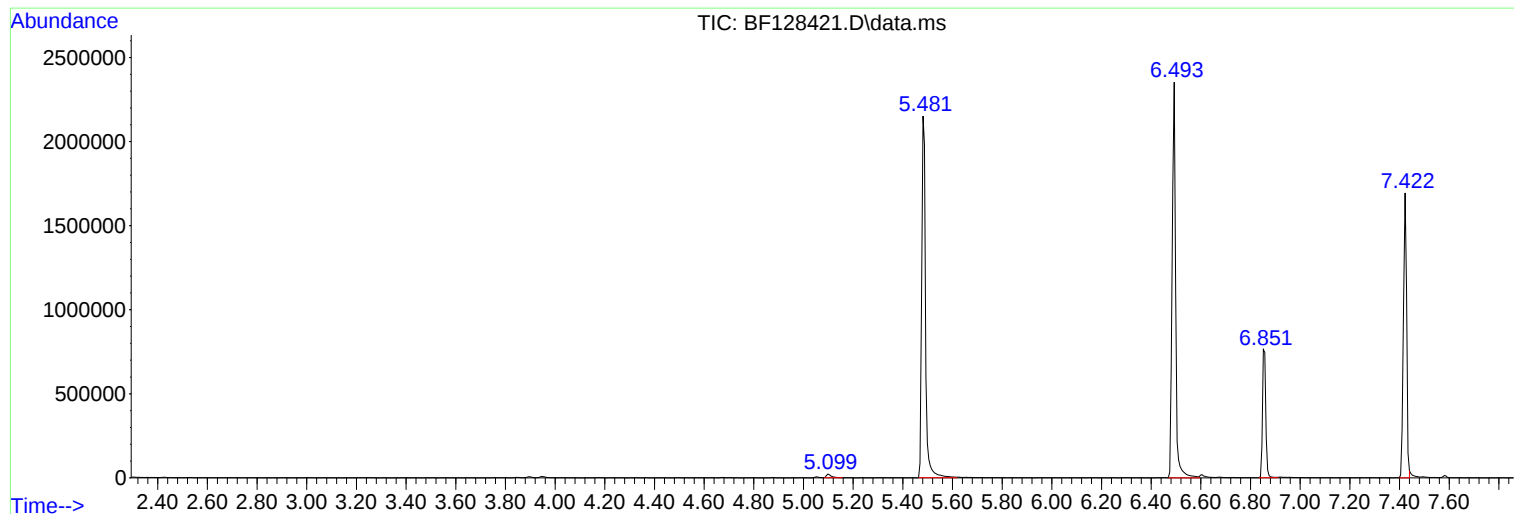

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052322\
Data File : BF128421.D
Acq On : 24 May 2022 01:35
Operator : CG\JU
Sample : N2873-10
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P032-SS001-0006-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052322\
Data File : BF128421.D
Acq On : 24 May 2022 01:35
Operator : CG\JU
Sample : N2873-10
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P032-SS001-0006-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------