

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052322\
 Data File : BF128422.D
 Acq On : 24 May 2022 02:04
 Operator : CG\JU
 Sample : N2875-11
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 P007-SS008-0006-01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128422.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.481	539	543	569	rBV	1950199	2049437	96.02%	14.140%
2	6.493	711	715	733	rBV	2175087	2022692	94.77%	13.956%
3	6.857	773	777	789	rBV	742177	691165	32.38%	4.769%
4	7.422	869	873	876	rBV	1571890	1337874	62.68%	9.231%
5	8.139	991	995	1008	rBV	997317	860065	40.30%	5.934%
6	9.210	1173	1177	1181	rBV	2423729	2134281	100.00%	14.725%
7	9.892	1290	1293	1297	rBV	937220	830924	38.93%	5.733%
8	10.686	1425	1428	1442	rBV	1125830	1019361	47.76%	7.033%
9	11.386	1543	1547	1551	rBV	854040	712578	33.39%	4.916%
10	12.969	1812	1816	1820	rBV	1780992	1625213	76.15%	11.213%
11	14.039	1994	1998	2002	rBV	657051	650214	30.47%	4.486%
12	14.127	2010	2013	2016	rBV	32240	32921	1.54%	0.227%
13	15.521	2246	2250	2255	rVB	408786	527127	24.70%	3.637%




Sum of corrected areas: 14493852

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052322\
Data File : BF128422.D
Acq On : 24 May 2022 02:04
Operator : CG\JU
Sample : N2875-11
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P007-SS008-0006-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

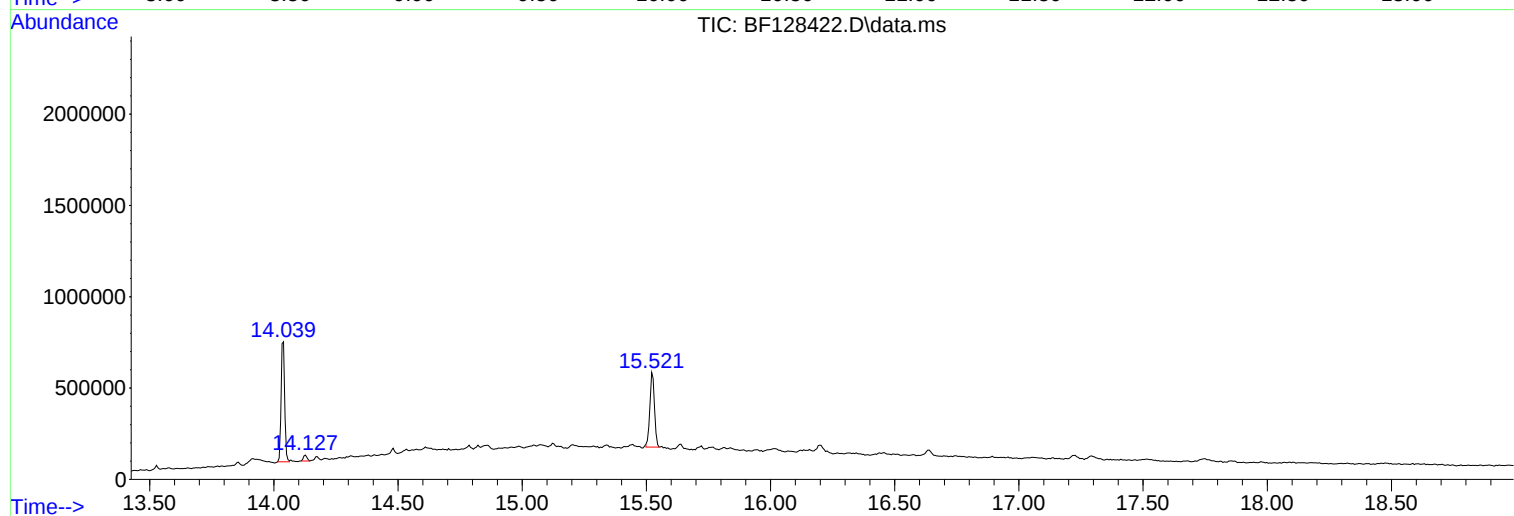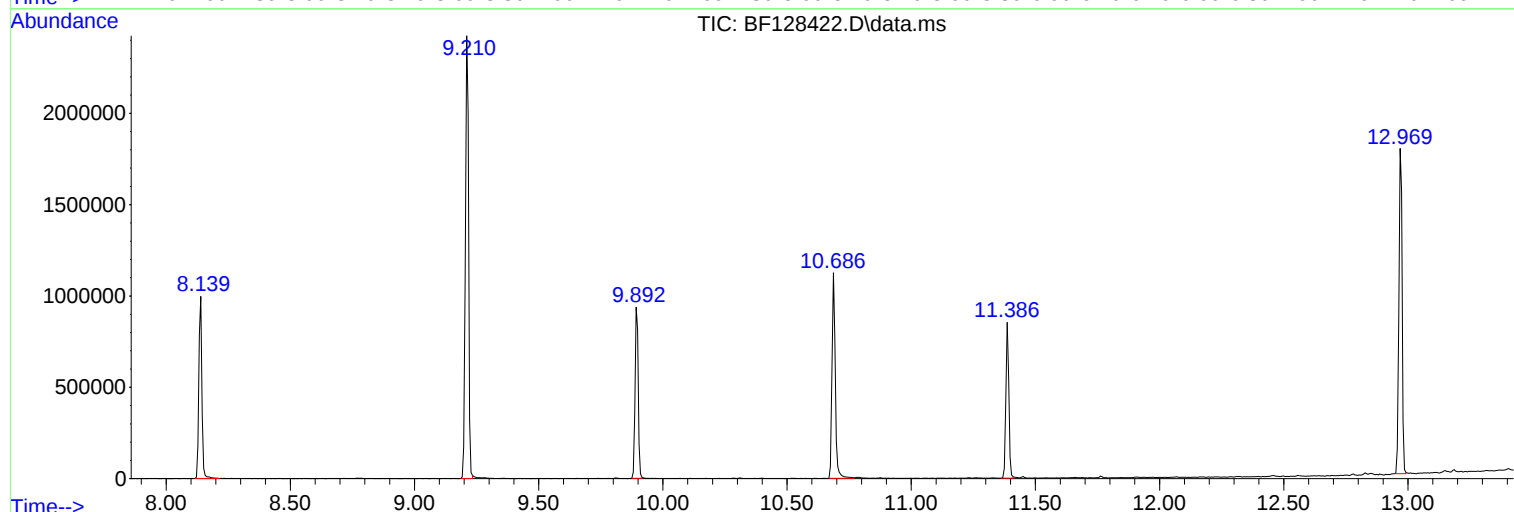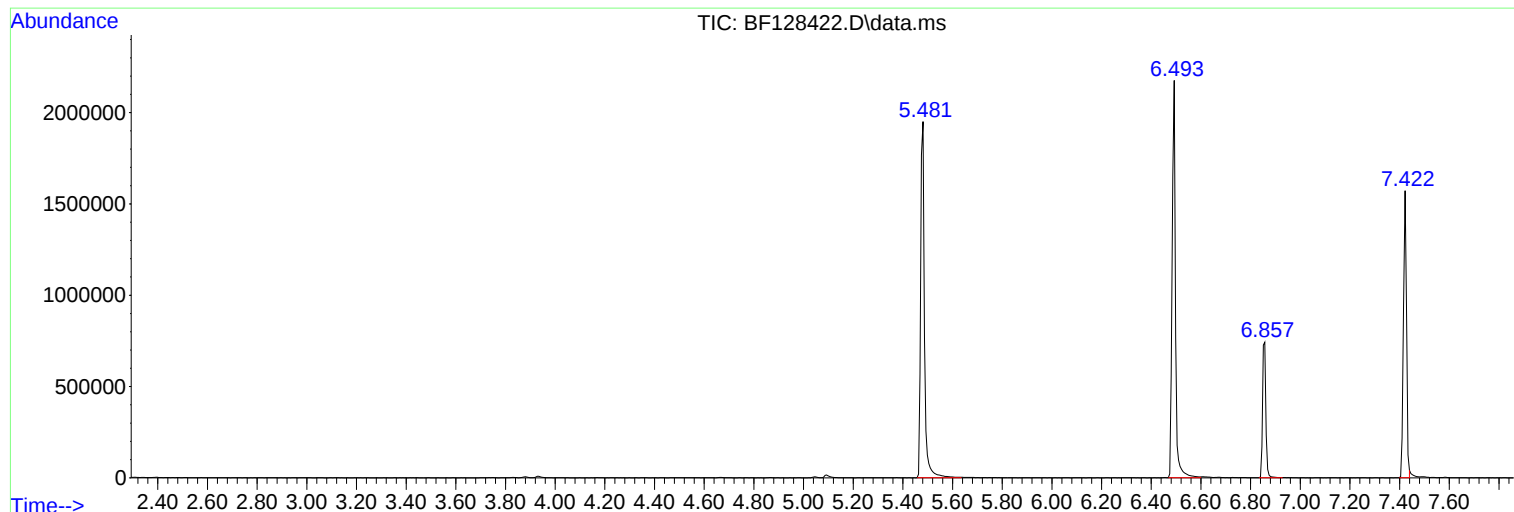

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052322\
Data File : BF128422.D
Acq On : 24 May 2022 02:04
Operator : CG\JU
Sample : N2875-11
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P007-SS008-0006-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052322\
Data File : BF128422.D
Acq On : 24 May 2022 02:04
Operator : CG\JU
Sample : N2875-11
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P007-SS008-0006-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------