

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052322\
 Data File : BF128424.D
 Acq On : 24 May 2022 03:03
 Operator : CG\JU
 Sample : N2875-19 2X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 P007-SS010-0006-01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128424.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.475	539	542	560	rBV	1298157	1275414	96.43%	11.884%
2	6.493	711	715	730	rBV	1227418	1264417	95.60%	11.782%
3	6.857	773	777	791	rVB	801803	746230	56.42%	6.953%
4	7.422	869	873	883	rBV	959366	810016	61.24%	7.548%
5	8.139	991	995	999	rBV	1072640	891470	67.40%	8.307%
6	9.210	1173	1177	1181	rBV	1624086	1322653	100.00%	12.324%
7	9.892	1290	1293	1297	rBV	959687	860283	65.04%	8.016%
8	10.686	1425	1428	1438	rBV	710285	642955	48.61%	5.991%
9	11.386	1544	1547	1551	rBV	915729	784352	59.30%	7.309%
10	12.969	1813	1816	1820	rBV	1184690	1056596	79.88%	9.845%
11	14.039	1994	1998	2003	rBV	709482	633545	47.90%	5.903%
12	15.527	2247	2251	2256	rVB	356834	444113	33.58%	4.138%




Sum of corrected areas: 10732044

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052322\
Data File : BF128424.D
Acq On : 24 May 2022 03:03
Operator : CG\JU
Sample : N2875-19 2X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P007-SS010-0006-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

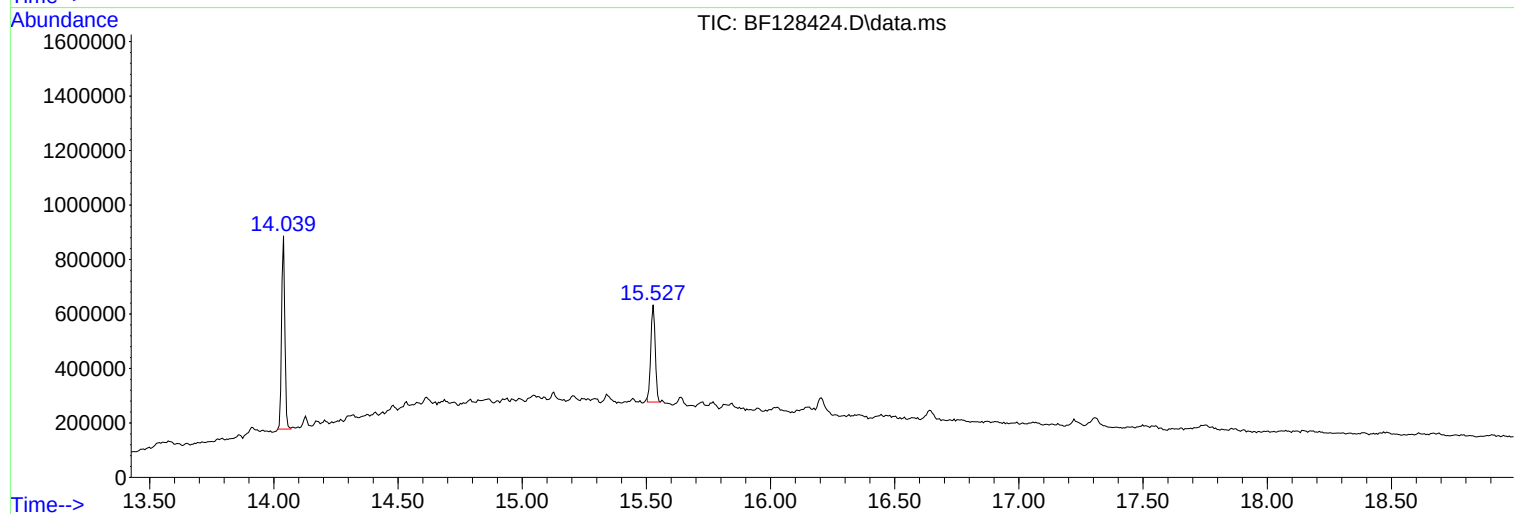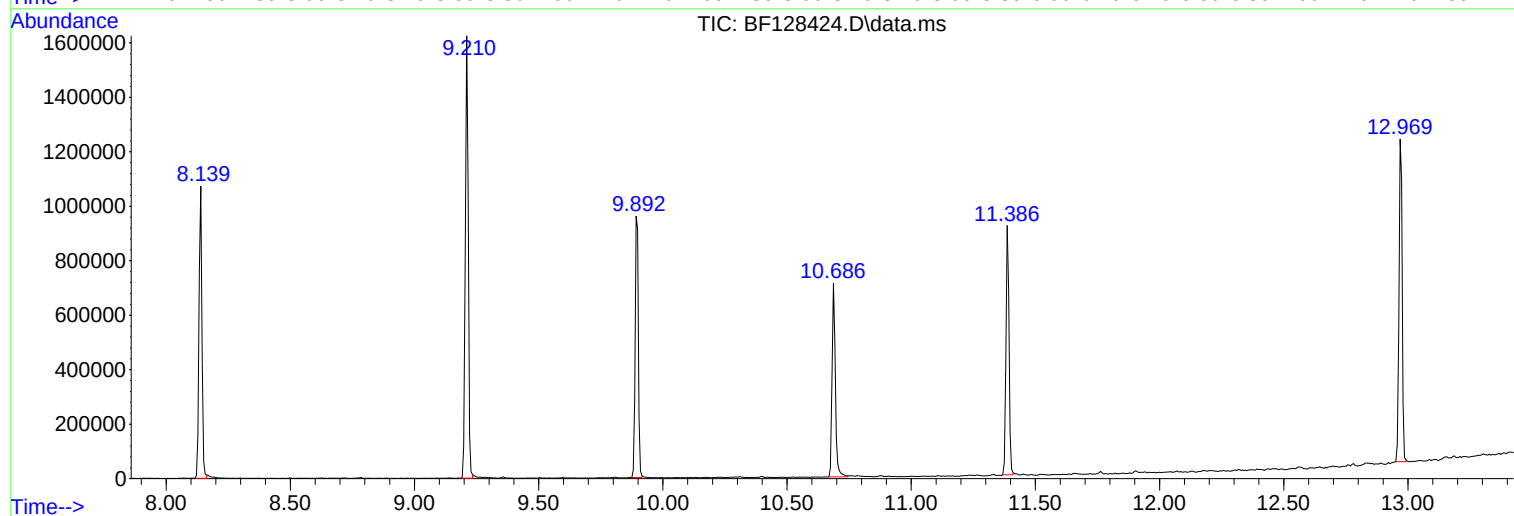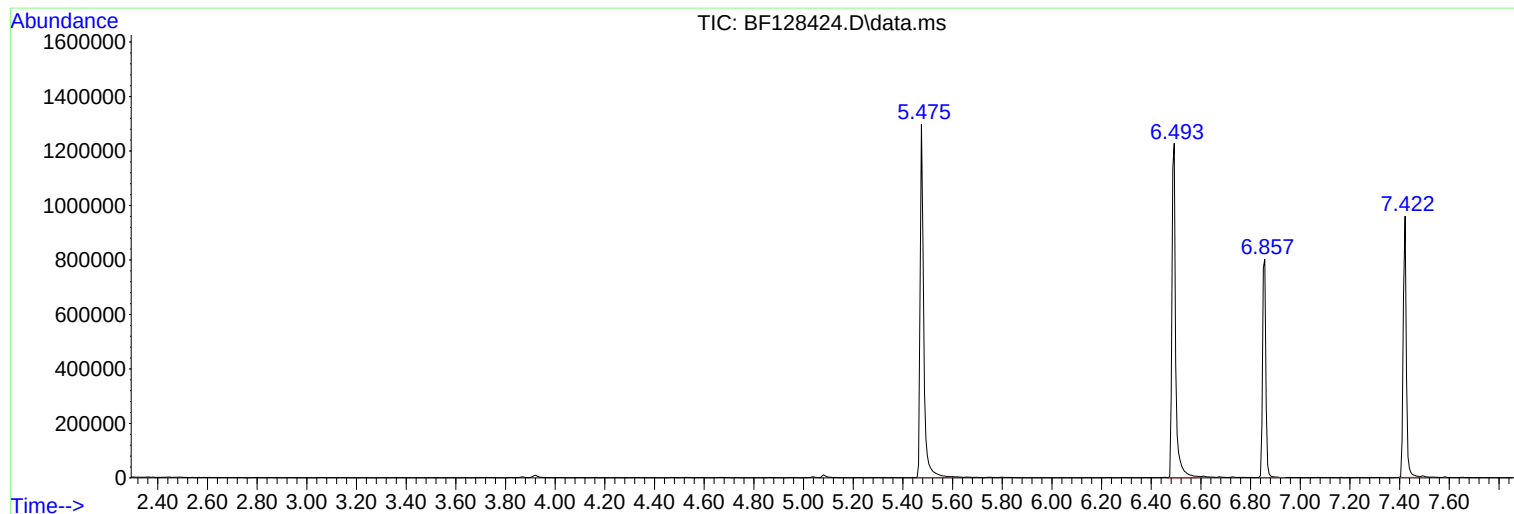

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052322\
Data File : BF128424.D
Acq On : 24 May 2022 03:03
Operator : CG\JU
Sample : N2875-19 2X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P007-SS010-0006-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052322\
Data File : BF128424.D
Acq On : 24 May 2022 03:03
Operator : CG\JU
Sample : N2875-19 2X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P007-SS010-0006-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------