

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052322\
 Data File : BF128425.D
 Acq On : 24 May 2022 03:32
 Operator : CG\JU
 Sample : N2875-16 5X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 P007-SS009-0006-01

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128425.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.910	272	276	285	rBV2	7881	11474	1.52%	0.208%
2	5.481	540	543	558	rBV	251691	315743	41.85%	5.732%
3	6.492	712	715	728	rBV	281001	312672	41.45%	5.676%
4	6.857	773	777	785	rBV	741822	646968	85.76%	11.744%
5	7.422	870	873	883	rBV	206322	187393	24.84%	3.402%
6	8.139	991	995	1015	rBV	912966	754411	100.00%	13.695%
7	9.210	1174	1177	1184	rBV	424551	331576	43.95%	6.019%
8	9.892	1290	1293	1297	rBV	753455	689289	91.37%	12.513%
9	10.692	1425	1429	1438	rBV	135964	145083	19.23%	2.634%
10	11.386	1544	1547	1556	rBV	739363	669736	88.78%	12.158%
11	12.780	1782	1784	1788	rBV5	7148	9797	1.30%	0.178%
12	12.968	1813	1816	1820	rBV	387525	326798	43.32%	5.932%
13	14.039	1994	1998	2003	rBV	681646	638828	84.68%	11.597%
14	14.127	2011	2013	2016	rVB	26406	22440	2.97%	0.407%
15	15.527	2246	2251	2257	rBV	366871	446571	59.19%	8.107%




Sum of corrected areas: 5508779

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052322\
Data File : BF128425.D
Acq On : 24 May 2022 03:32
Operator : CG\JU
Sample : N2875-16 5X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P007-SS009-0006-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

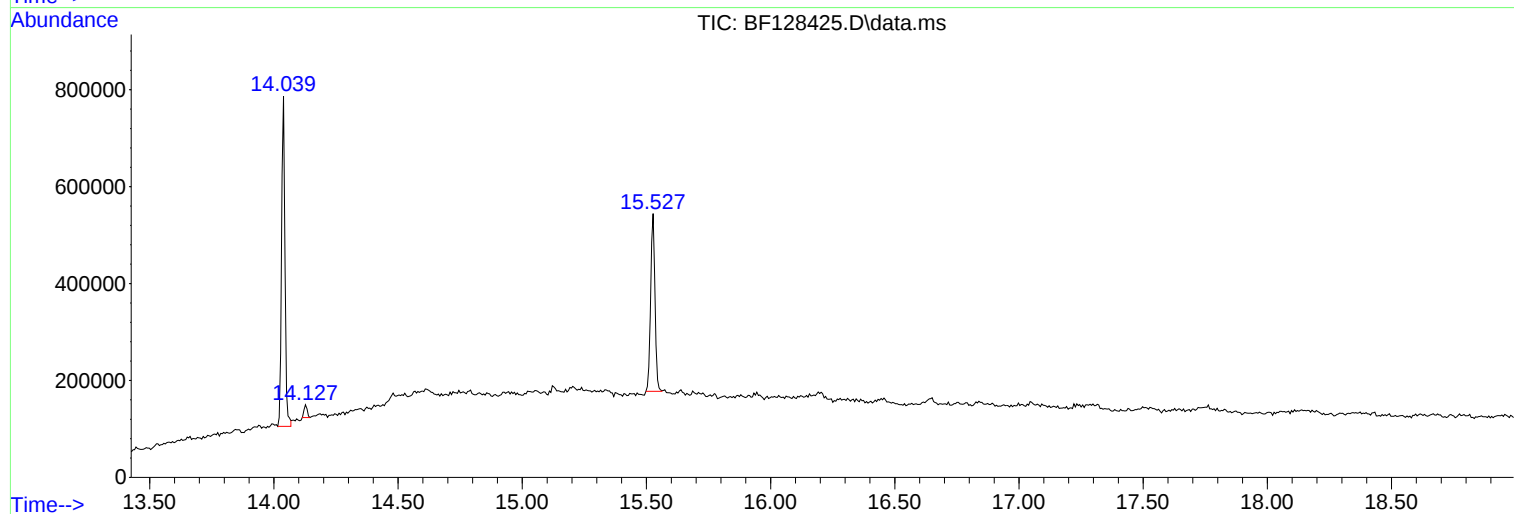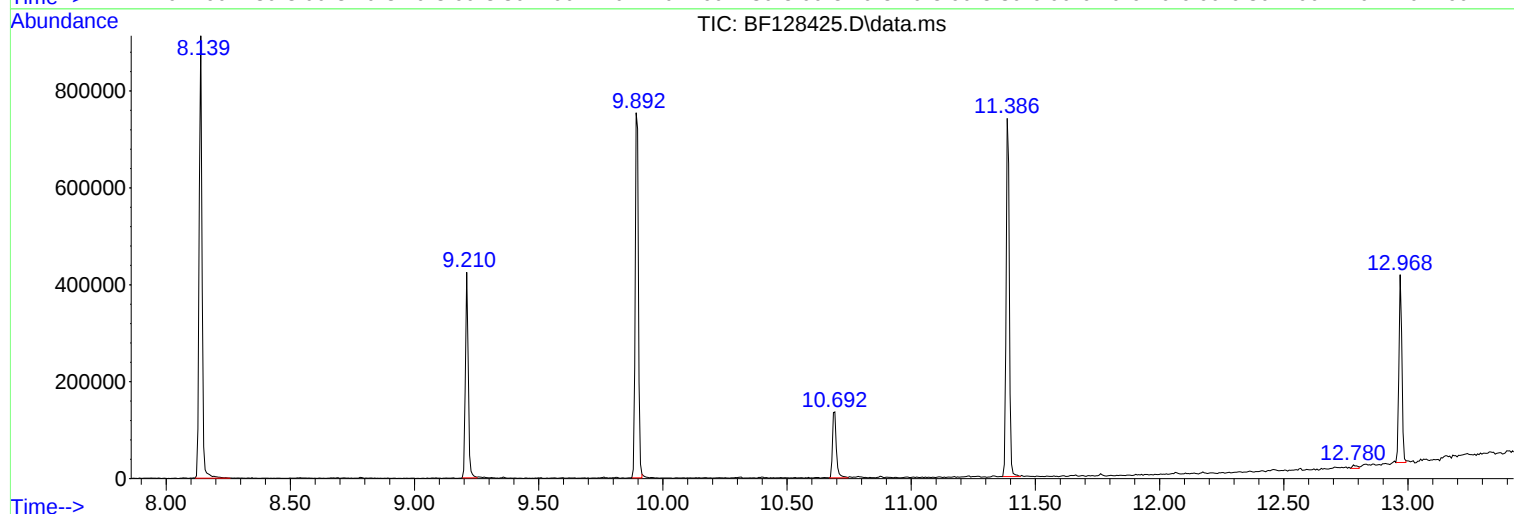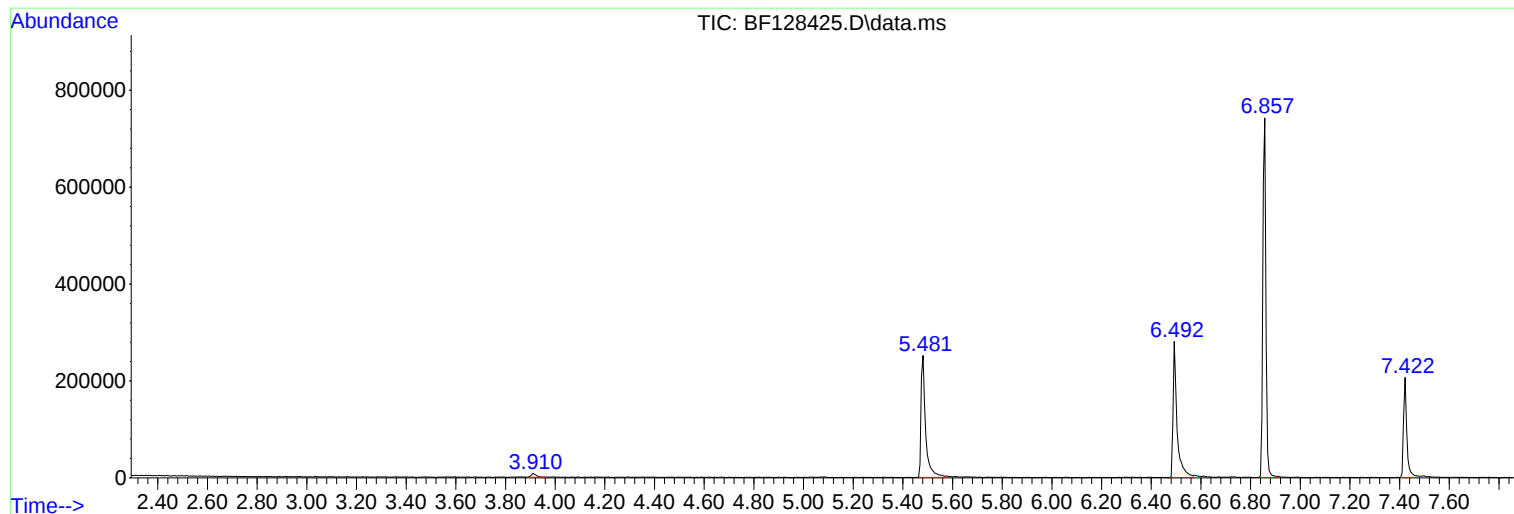

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052322\
Data File : BF128425.D
Acq On : 24 May 2022 03:32
Operator : CG\JU
Sample : N2875-16 5X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P007-SS009-0006-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052322\
Data File : BF128425.D
Acq On : 24 May 2022 03:32
Operator : CG\JU
Sample : N2875-16 5X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P007-SS009-0006-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------