

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052322\
 Data File : BF128426.D
 Acq On : 24 May 2022 04:01
 Operator : CG\JU
 Sample : N2876-04 10X
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 P007-SS011-0006-01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128426.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.916	272	277	283	rBV2	7315	12296	1.56%	0.246%
2	5.481	540	543	556	rBV	113711	155422	19.66%	3.107%
3	6.451	705	708	713	rVB	48465	39322	4.97%	0.786%
4	6.498	713	716	733	rBV	126127	166575	21.07%	3.330%
5	6.857	773	777	789	rBV	732208	671544	84.95%	13.423%
6	7.422	870	873	883	rBV	100724	101177	12.80%	2.022%
7	7.586	896	901	903	rVB	23522	21525	2.72%	0.430%
8	8.139	991	995	999	rBV	963275	790530	100.00%	15.801%
9	9.210	1174	1177	1184	rBV	238638	192899	24.40%	3.856%
10	9.898	1290	1294	1297	rBV	906661	790132	99.95%	15.793%
11	10.692	1425	1429	1436	rBV	81506	81537	10.31%	1.630%
12	11.386	1544	1547	1551	rBV	856651	766093	96.91%	15.313%
13	11.763	1609	1611	1615	rVB5	14532	13006	1.65%	0.260%
14	12.474	1730	1732	1735	rVB3	14025	10417	1.32%	0.208%
15	12.557	1744	1746	1751	rVB6	15823	18581	2.35%	0.371%
16	12.833	1791	1793	1798	rBV3	17847	20701	2.62%	0.414%
17	12.968	1813	1816	1820	rBV	199463	174022	22.01%	3.478%
18	14.039	1995	1998	2002	rBV	669293	567677	71.81%	11.347%
19	15.533	2248	2252	2256	rVB	324095	409505	51.80%	8.185%




Sum of corrected areas: 5002961

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052322\
Data File : BF128426.D
Acq On : 24 May 2022 04:01
Operator : CG\JU
Sample : N2876-04 10X
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P007-SS011-0006-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

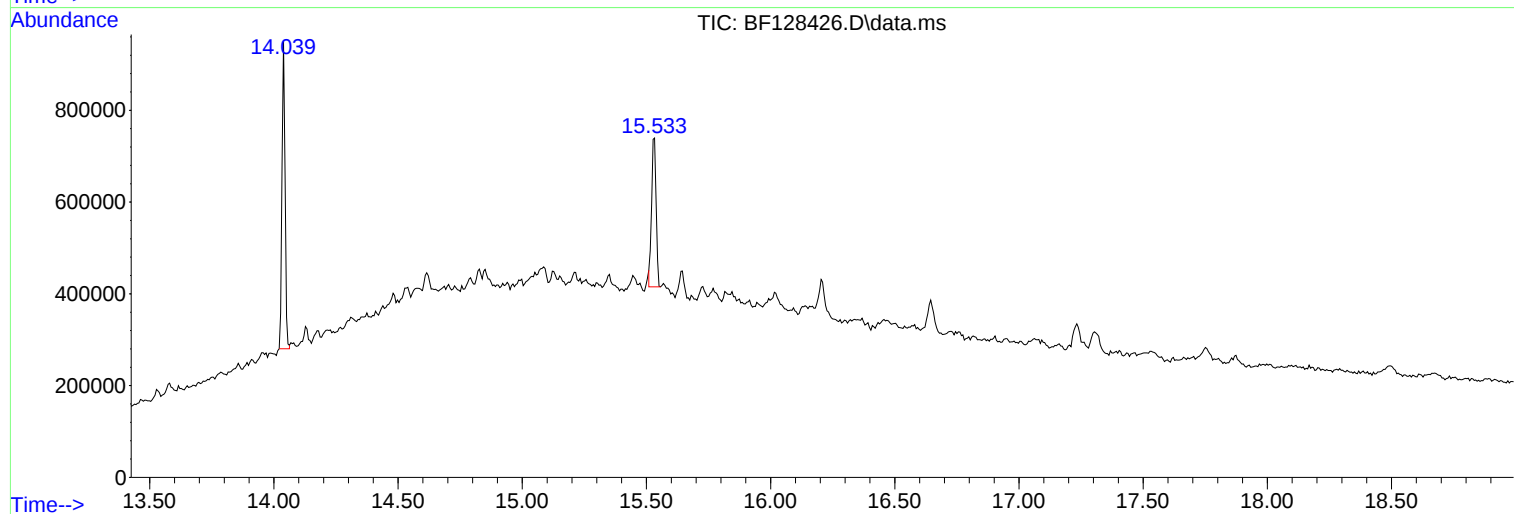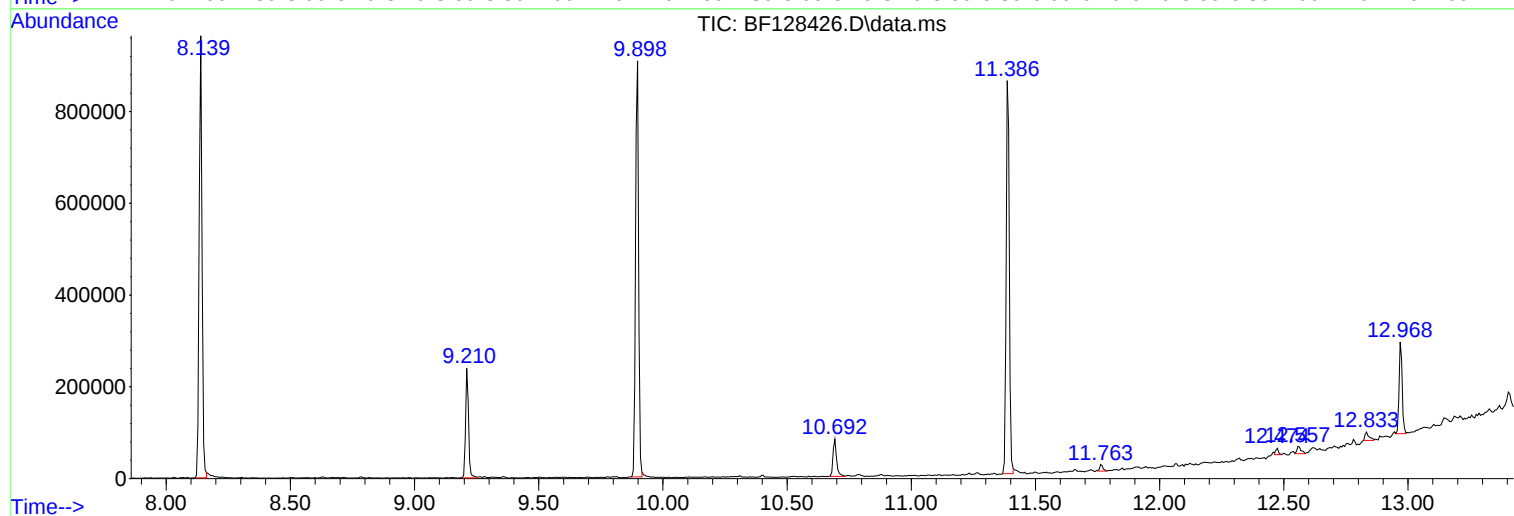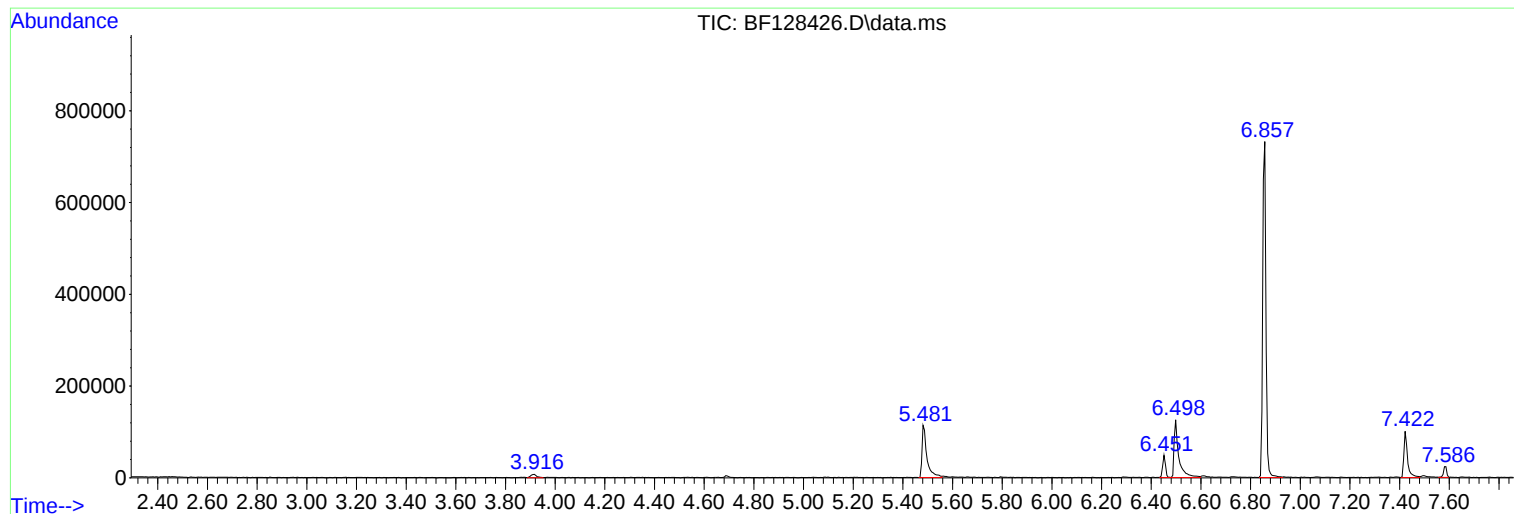

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052322\
Data File : BF128426.D
Acq On : 24 May 2022 04:01
Operator : CG\JU
Sample : N2876-04 10X
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P007-SS011-0006-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052322\
Data File : BF128426.D
Acq On : 24 May 2022 04:01
Operator : CG\JU
Sample : N2876-04 10X
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P007-SS011-0006-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------