
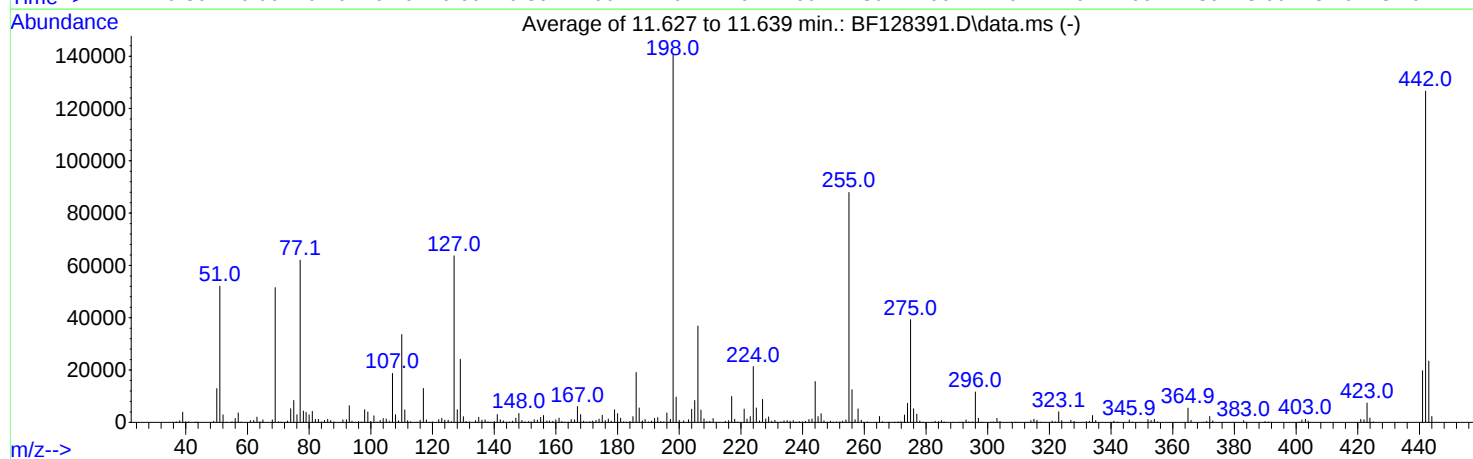


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052322\
 Data File : BF128391.D
 Acq On : 23 May 2022 10:01
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat May 21 05:28:09 2022

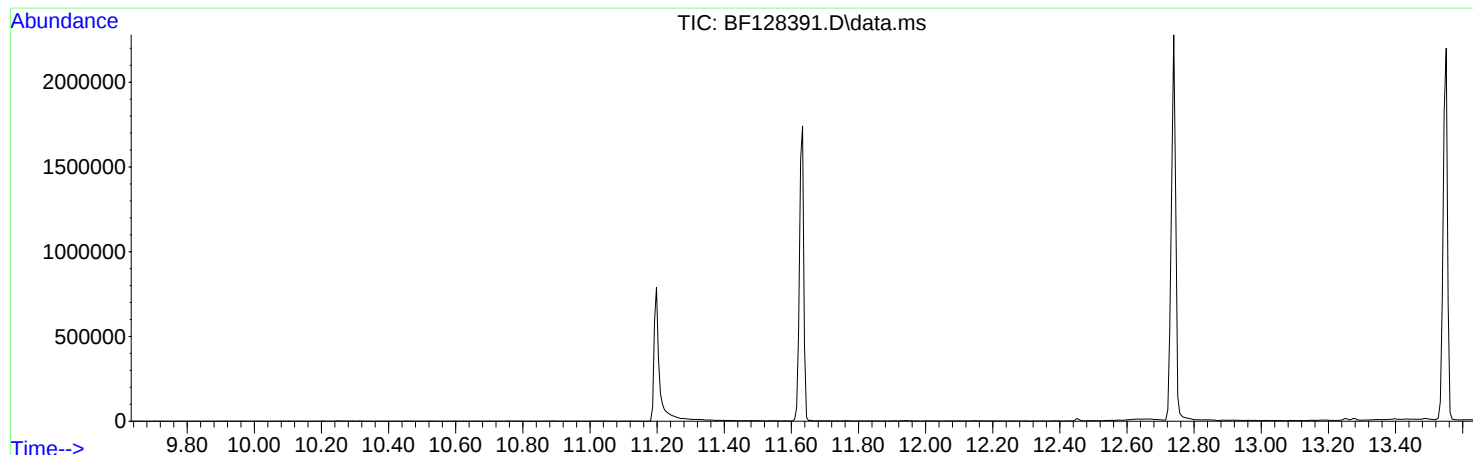




AutoFind: Scans 1588, 1589, 1590; Background Corrected with Scan 1581

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.0	52060	PASS
68	69	0.00	2	1.9	995	PASS
69	198	0.00	100	36.6	51537	PASS
70	69	0.00	2	0.4	227	PASS
127	198	10	80	45.3	63709	PASS
197	198	0.00	2	0.8	1187	PASS
198	198	100	100	100.0	140651	PASS
199	198	5	9	6.9	9641	PASS
275	198	10	60	27.9	39277	PASS
365	198	1	100	3.9	5464	PASS
441	198	0.01	100	14.1	19766	PASS
442	442	50	100	100.0	126645	PASS
443	442	15	24	18.5	23424	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052322\
Data File : BF128391.D
Acq On : 23 May 2022 10:01
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 24 08:31:12 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 21 05:28:09 2022
Response via : Initial Calibration

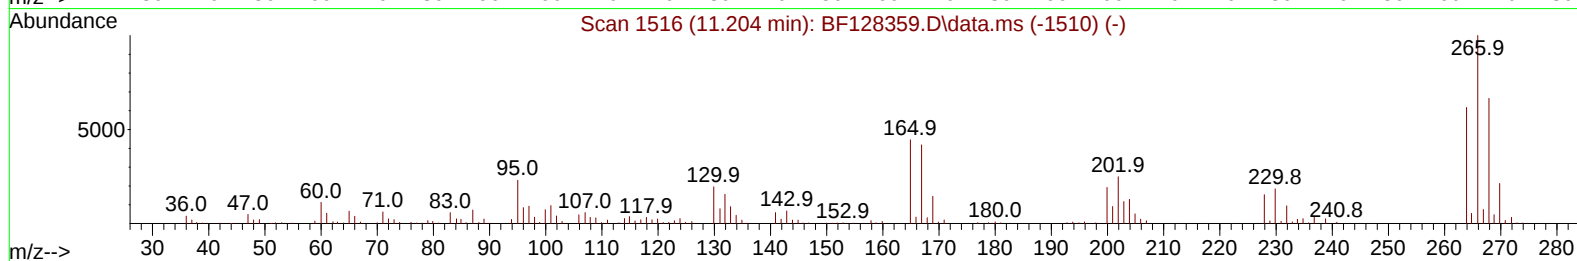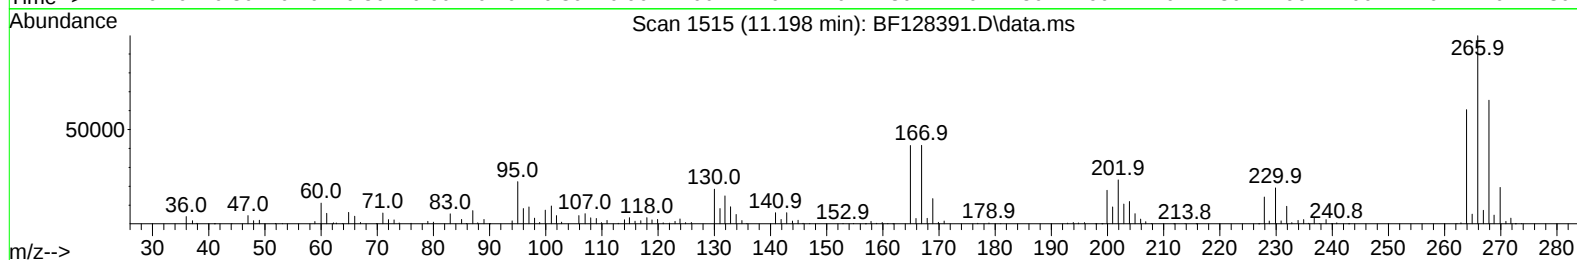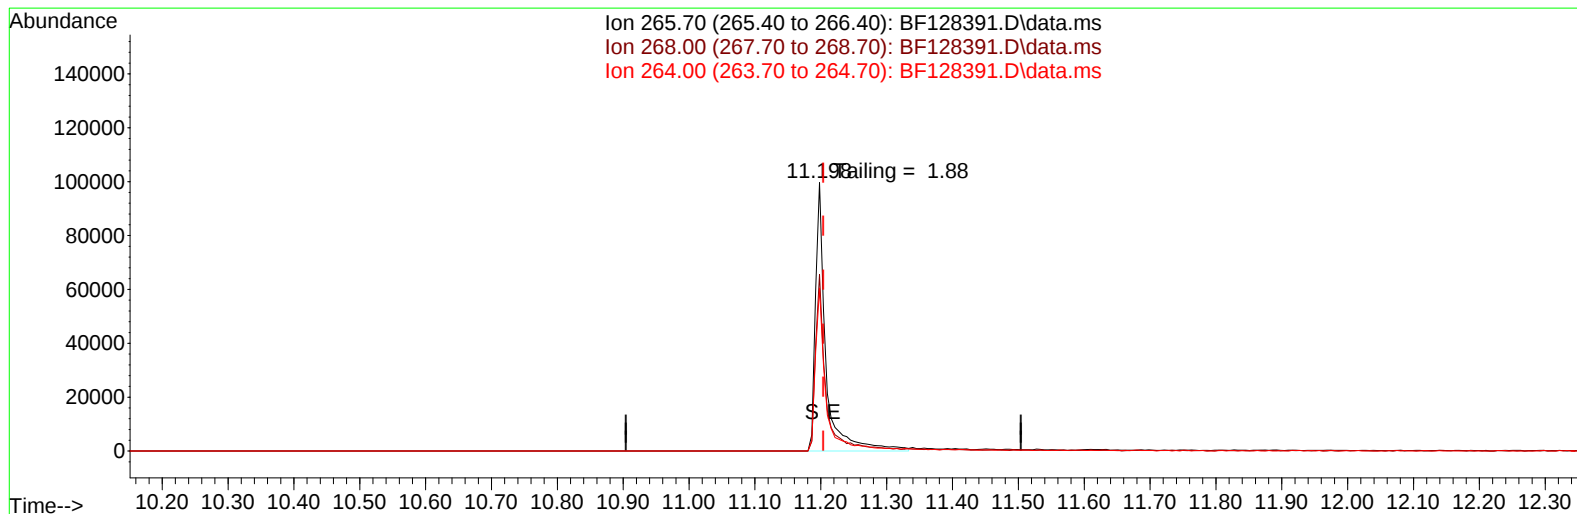

TIC: BF128391.D\data.ms

(70) Pentachlorophenol (C)

11.198min (-0.006) 167898.05 ng




response 111331

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.30	65.75
264.00	66.40	60.72
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052322\
 Data File : BF128391.D
 Acq On : 23 May 2022 10:01
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: May 24 08:31:12 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat May 21 05:28:09 2022
 Response via : Initial Calibration

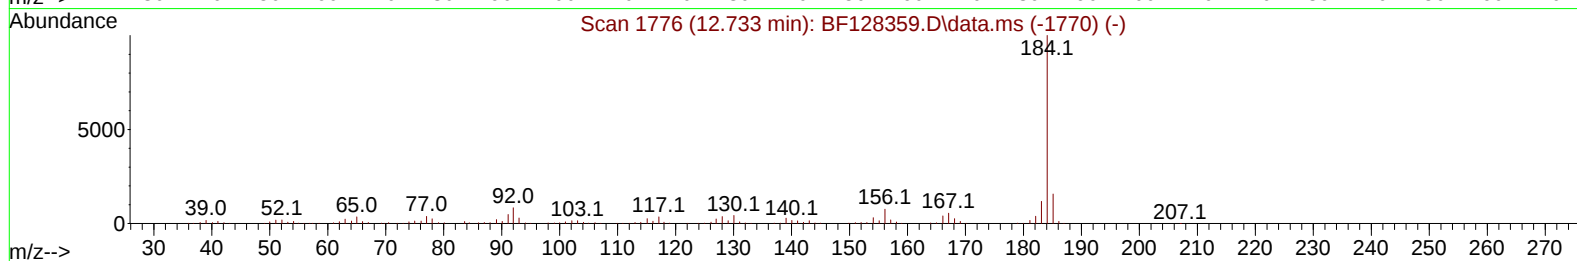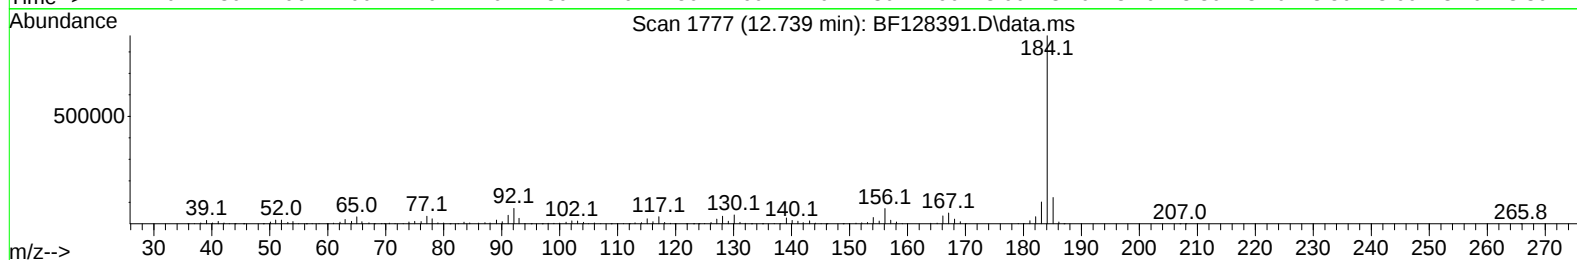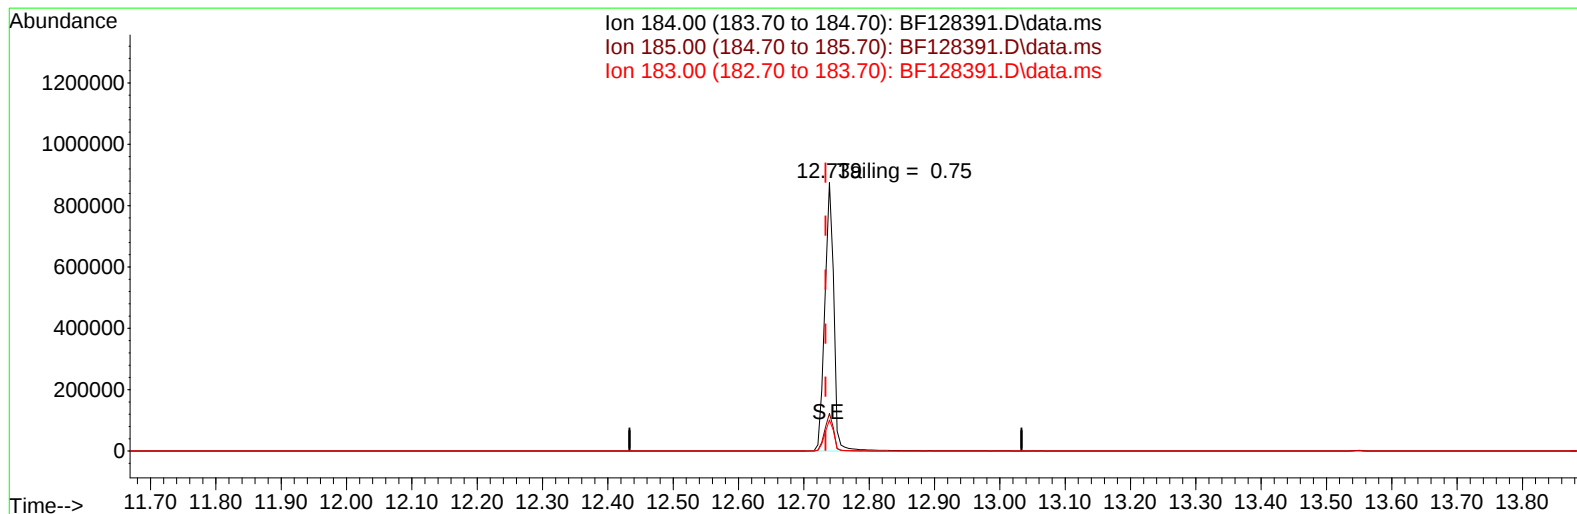

TIC: BF128391.D\data.ms

(77) Benzidine

12.739min (+ 0.006) 526465.04 ng

response 843132

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	14.01
183.00	11.20	11.58
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/23/2022	BNA_F	<u>BF128391.D</u>
Compound Name	Response	Retention Time
DDT	379790	13.551
DDD	5060	13.251
DDE	767	12.916
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5827	385617	1.51

Instrument :
BNA_F
ClientSampleId :
DFTPP