


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052322\
 Data File : BF128403.D
 Acq On : 23 May 2022 16:37
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat May 21 05:28:09 2022

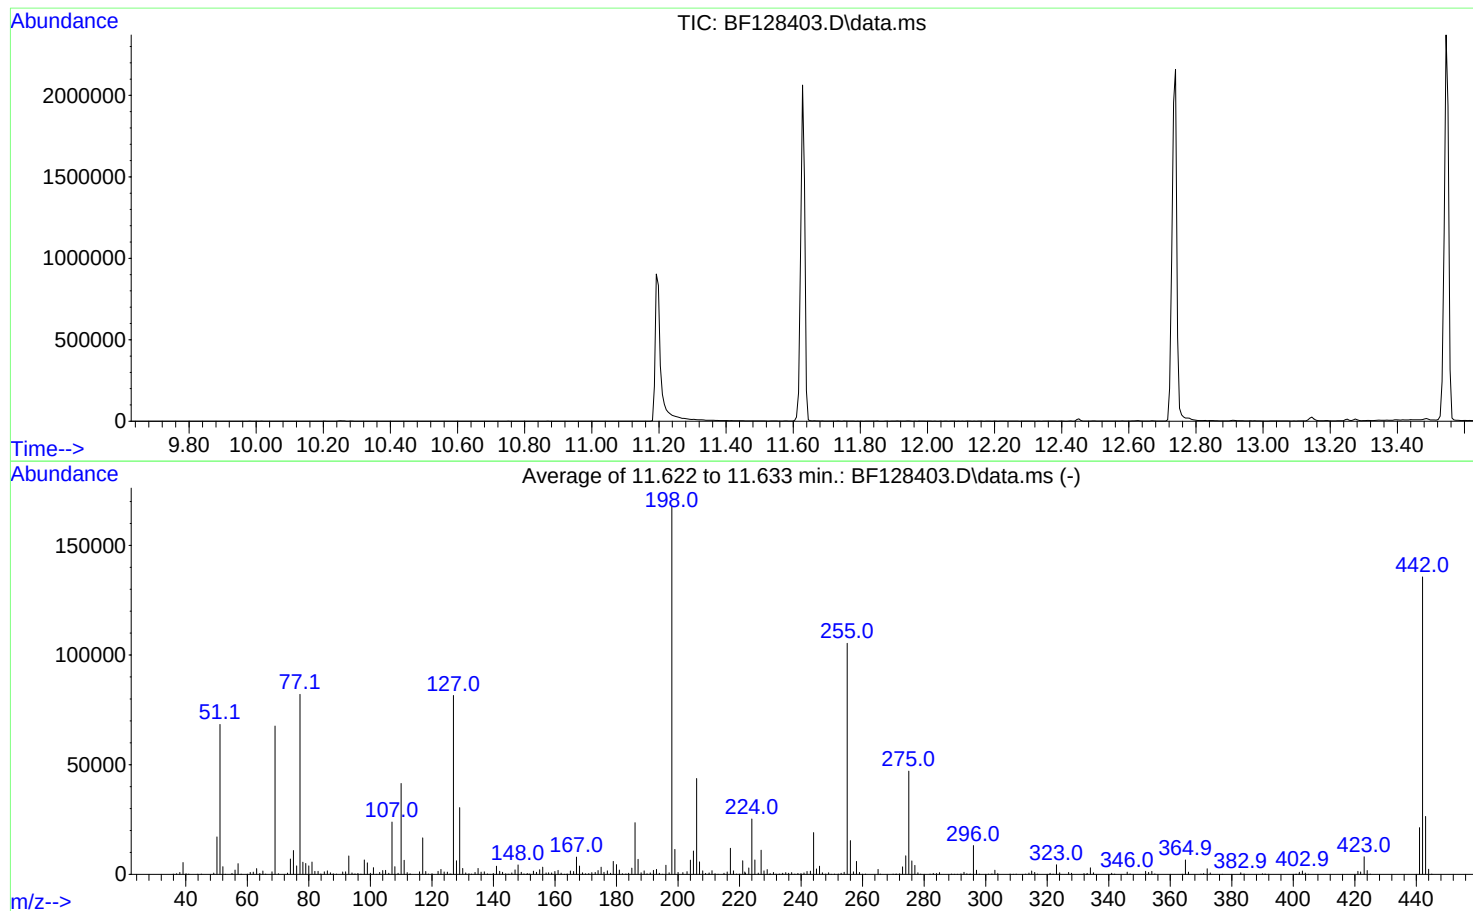




AutoFind: Scans 1587, 1588, 1589; Background Corrected with Scan 1581

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.8	68400	PASS
68	69	0.00	2	1.8	1206	PASS
69	198	0.00	100	40.3	67616	PASS
70	69	0.00	2	0.5	322	PASS
127	198	10	80	48.6	81565	PASS
197	198	0.00	2	0.5	768	PASS
198	198	100	100	100.0	167739	PASS
199	198	5	9	6.8	11389	PASS
275	198	10	60	28.1	47080	PASS
365	198	1	100	3.9	6584	PASS
441	198	0.01	100	12.7	21325	PASS
442	442	50	100	100.0	135664	PASS
443	442	15	24	19.5	26395	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052322\
Data File : BF128403.D
Acq On : 23 May 2022 16:37
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 24 08:33:45 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 21 05:28:09 2022
Response via : Initial Calibration

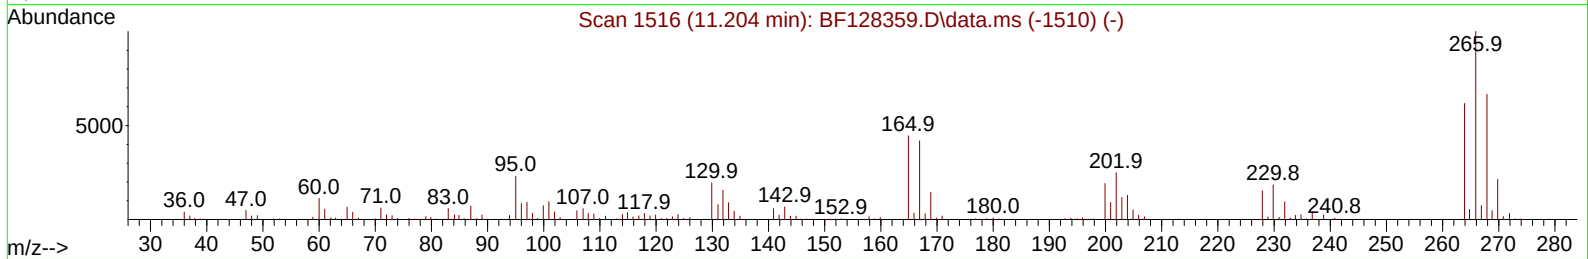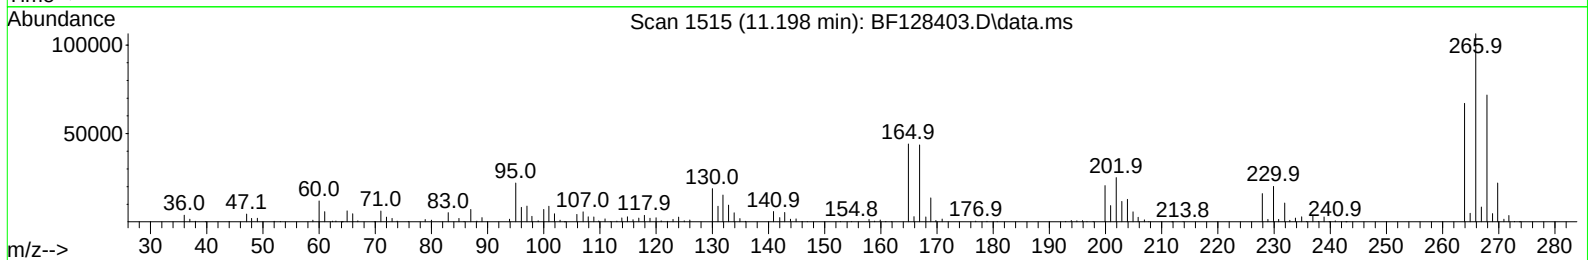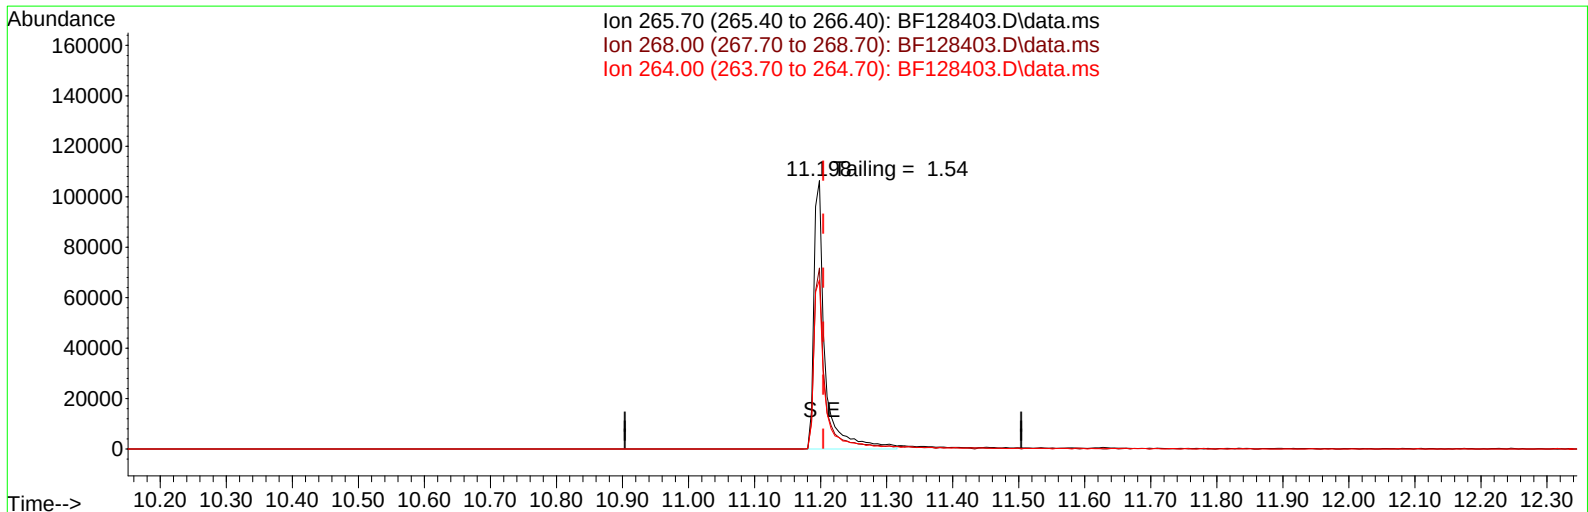

TIC: BF128403.D\data.ms

(70) Pentachlorophenol (C)

11.198min (-0.006) 192327.72 ng

response 127530

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.30	67.43
264.00	66.40	63.04
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/23/2022	BNA_F	<u>BF128403.D</u>
Compound Name	Response	Retention Time
DDT	412288	13.545
DDD	4677	13.251
DDE	1008	12.91
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5685	417973	1.36

Instrument :
BNA_F
ClientSampleId :
DFTPP