


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052323\
Data File : BF133450.D
Acq On : 23 May 2023 11:03
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052323.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed May 24 02:41:39 2023

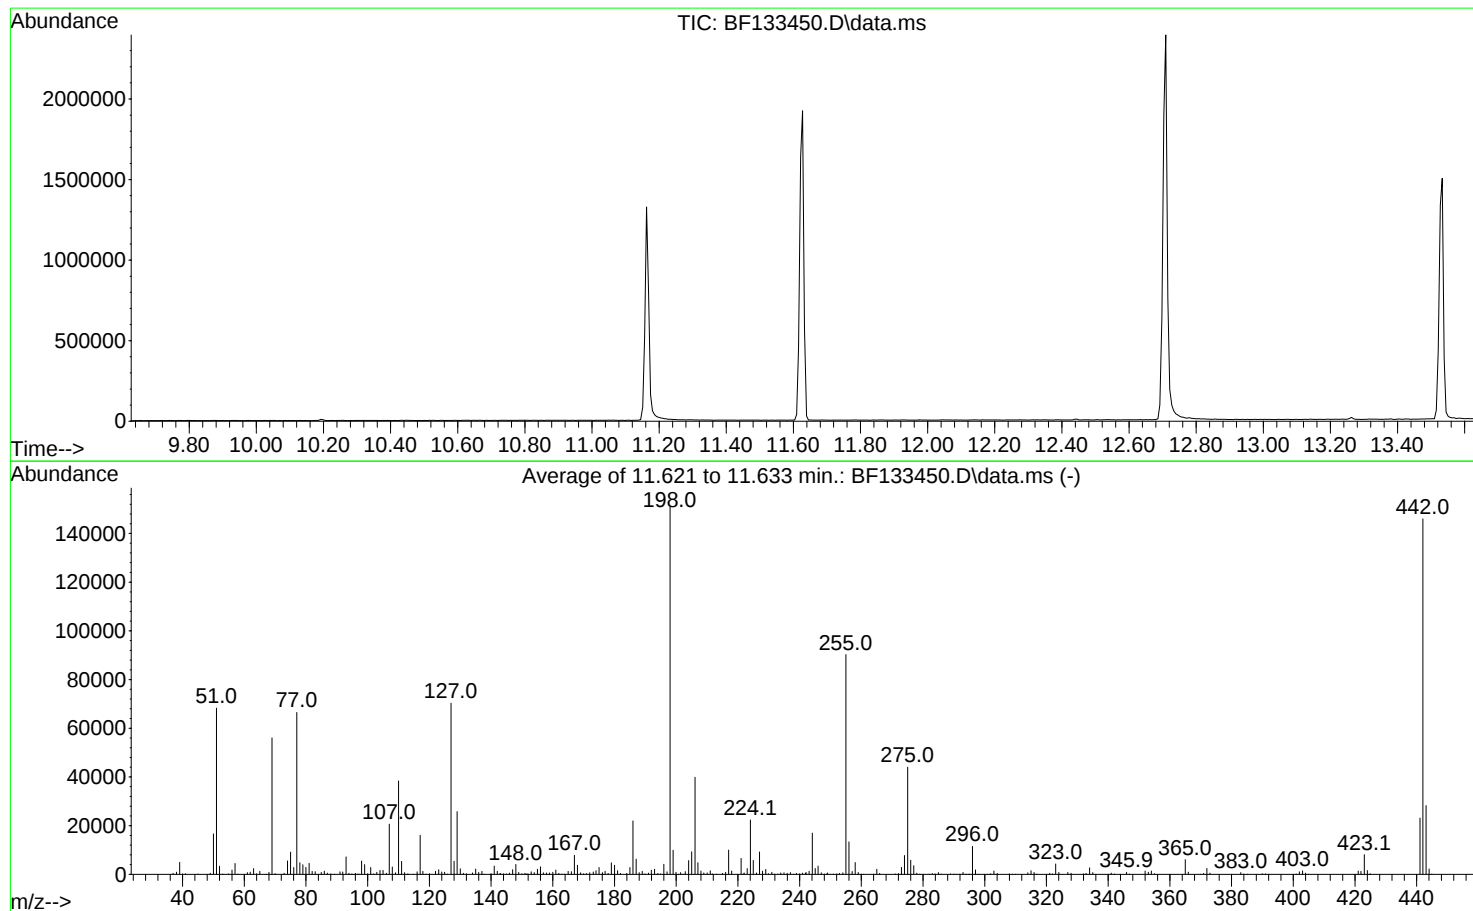

AutoFind: Scans 1621, 1622, 1623; Background Corrected with Scan 1615

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.2	68308	PASS
68	69	0.00	2	1.5	858	PASS
69	198	0.00	100	37.1	56055	PASS
70	69	0.00	2	0.4	229	PASS
127	198	10	80	46.5	70312	PASS
197	198	0.00	2	0.7	1033	PASS
198	198	100	100	100.0	151075	PASS
199	198	5	9	6.6	9956	PASS
275	198	10	60	29.1	44021	PASS
365	198	1	100	4.0	6060	PASS
441	198	0.01	100	15.3	23107	PASS
442	442	50	100	100.0	146016	PASS
443	442	15	24	19.4	28285	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/23/2023	BNA_F	<u>BF133450.D</u>
Compound Name	Response	Retention Time
DDT	197162	13.533
DDD	1549	13.263
DDE	0	12.896
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1549	198711	0.78

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052323\
Data File : BF133450.D
Acq On : 23 May 2023 11:03
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 24 06:55:23 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 24 02:41:39 2023
Response via : Initial Calibration

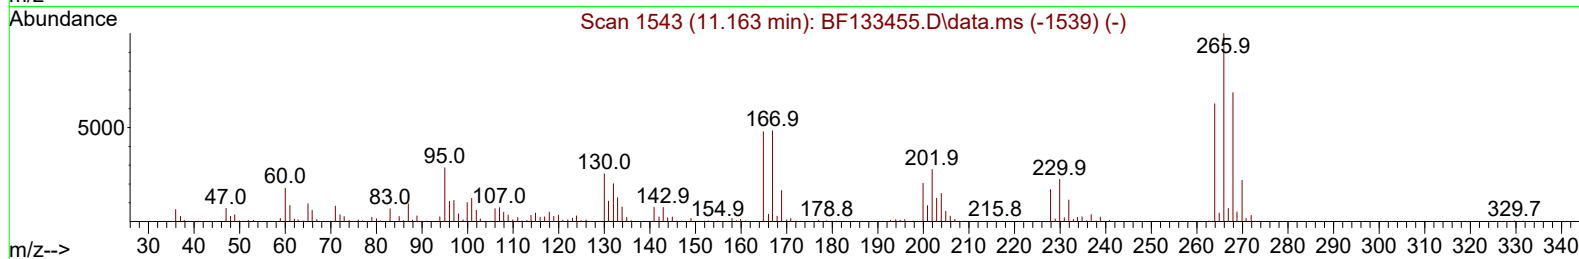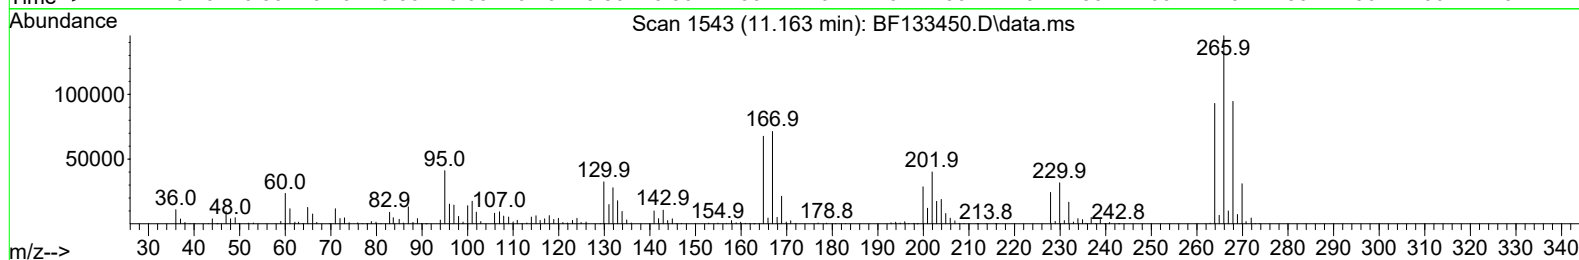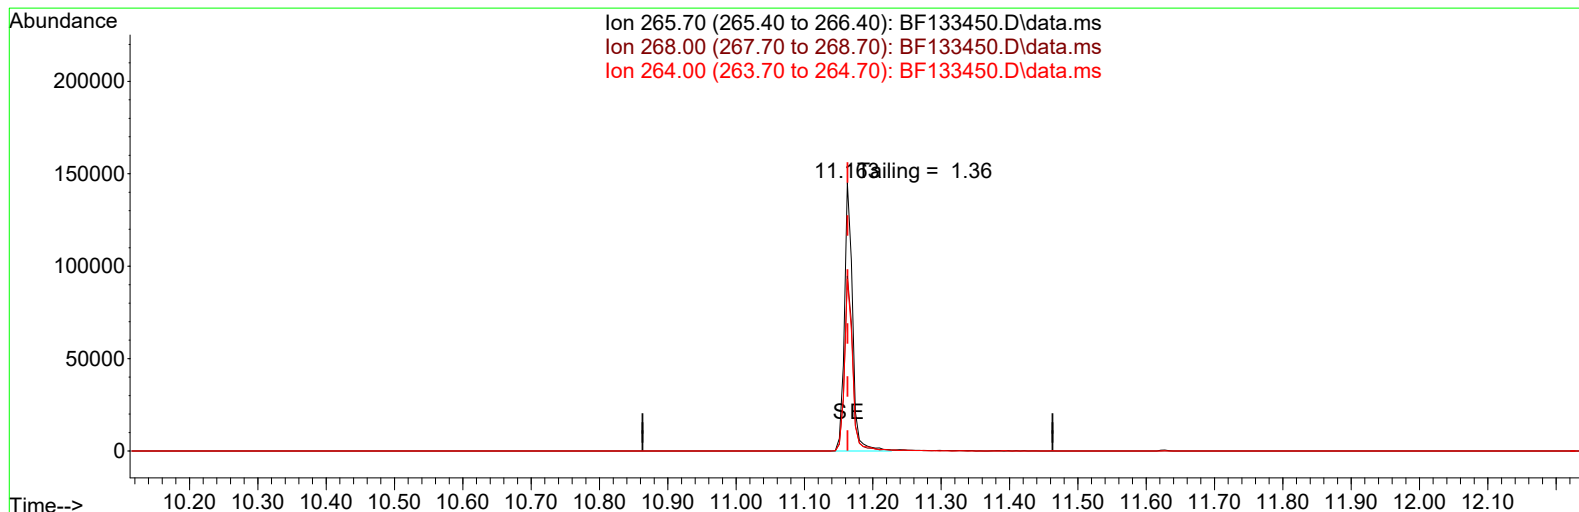

TIC: BF133450.D\data.ms

(70) Pentachlorophenol (C)

11.163min (-0.000) 22758.08 ng




response 121249

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	68.50	65.18
264.00	62.70	64.01
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052323\
 Data File : BF133450.D
 Acq On : 23 May 2023 11:03
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: May 24 06:55:23 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 24 02:41:39 2023
 Response via : Initial Calibration

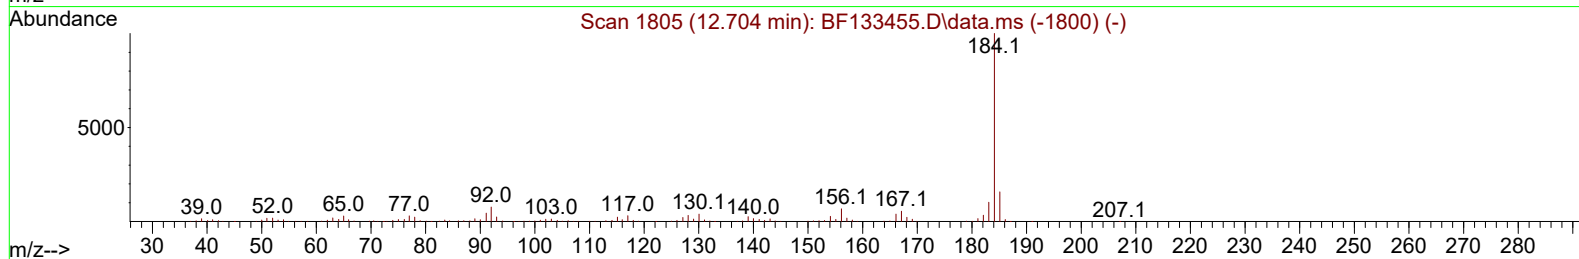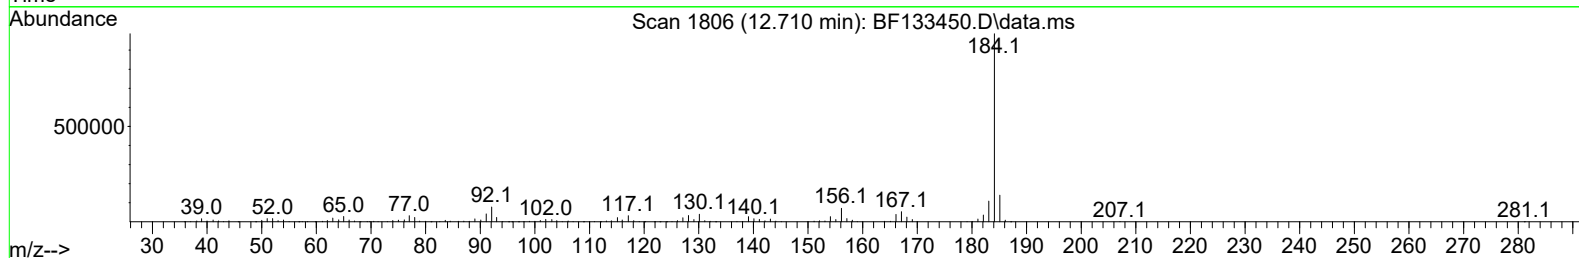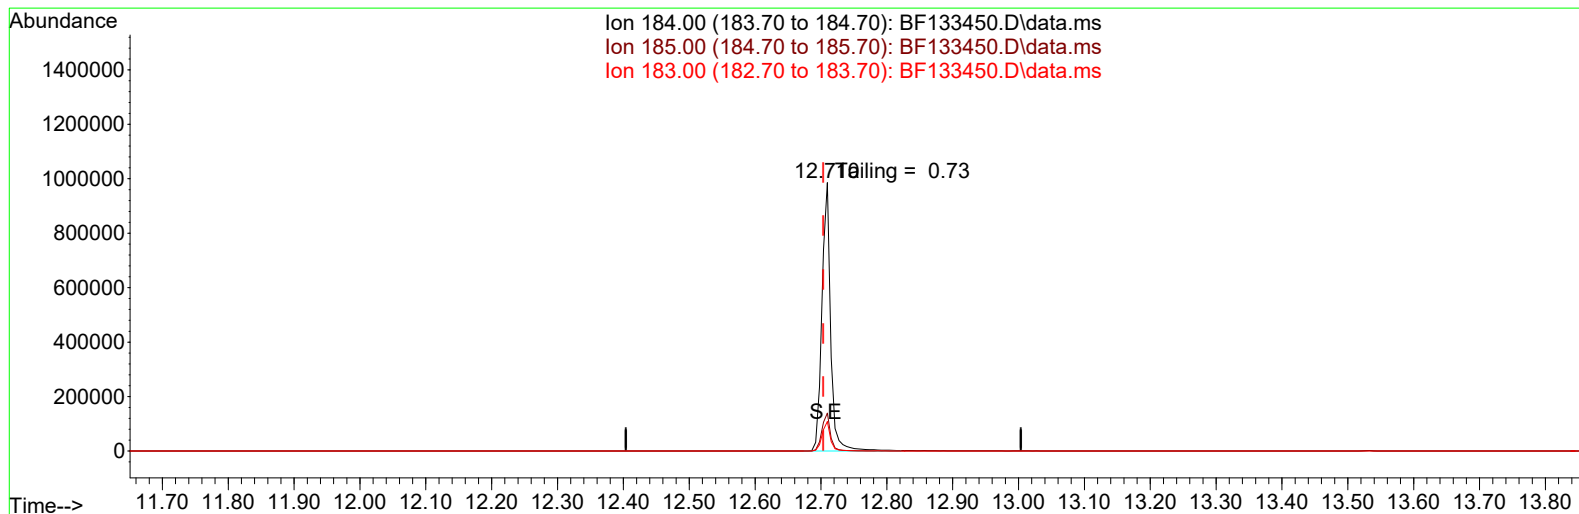

TIC: BF133450.D\data.ms

(77) Benzidine

12.710min (+ 0.006) 0.00 ng

response 910461

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.80	14.17
183.00	10.20	10.96
0.00	0.00	0.00