
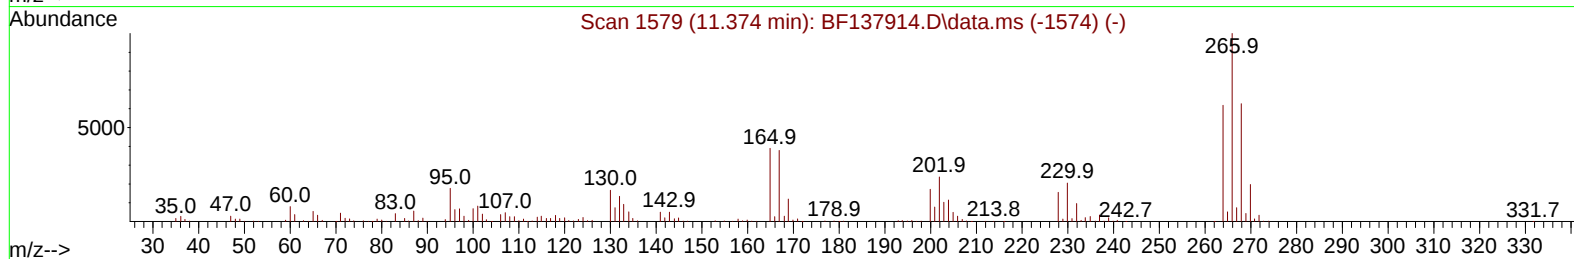
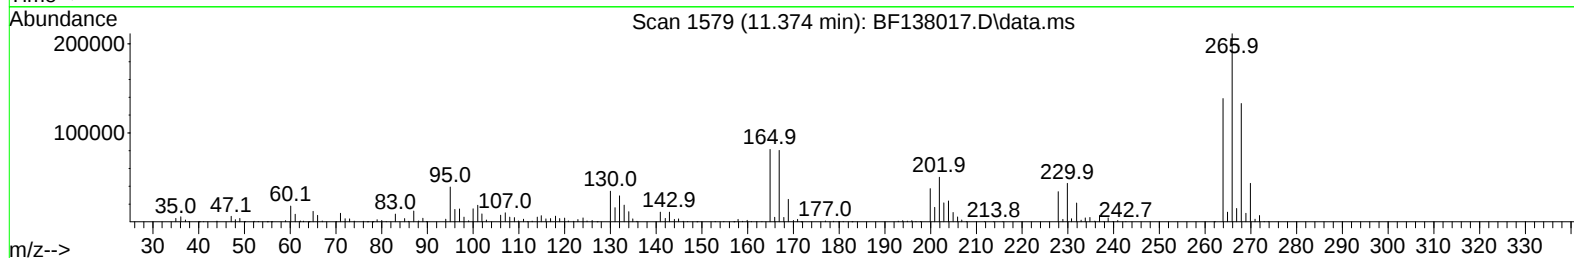


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052324\
Data File : BF138017.D
Acq On : 23 May 2024 09:47
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 23 11:02:56 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF051424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 15 04:12:16 2024
Response via : Initial Calibration

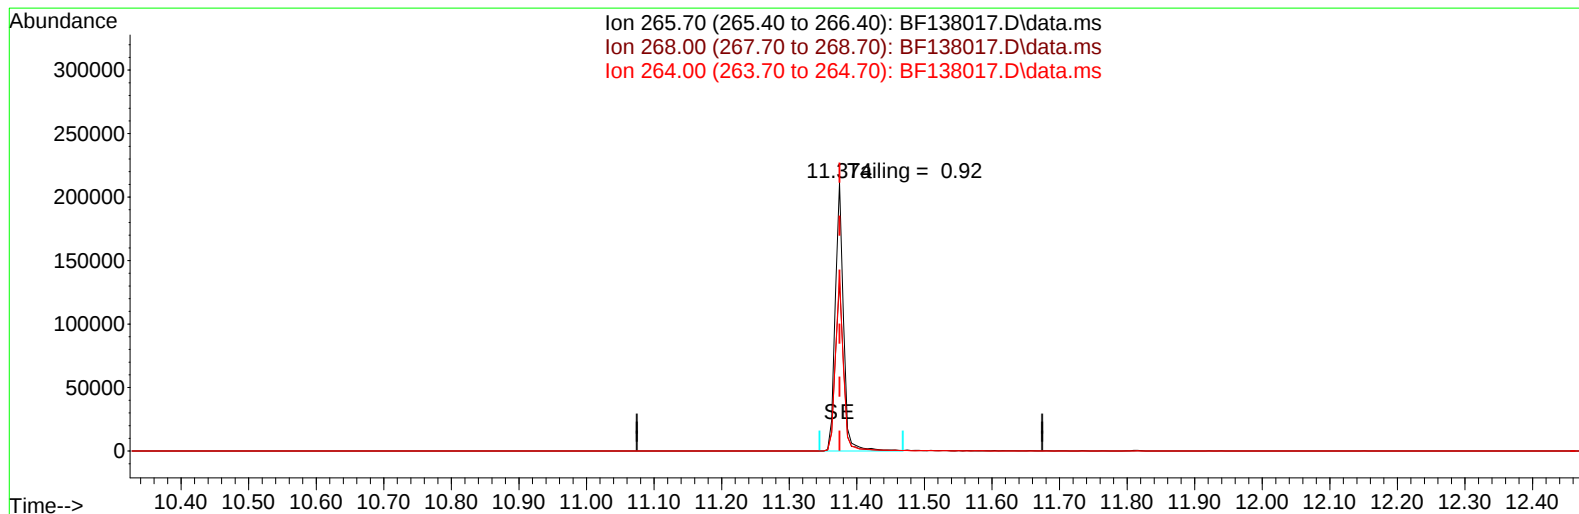

TIC: BF138017.D\data.ms

(70) Pentachlorophenol (C)




11.374min (-0.000) 27966.53 ng

response 179262

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	62.91
264.00	61.80	65.58
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052324\
Data File : BF138017.D
Acq On : 23 May 2024 09:47
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 23 11:02:56 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF051424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 15 04:12:16 2024
Response via : Initial Calibration

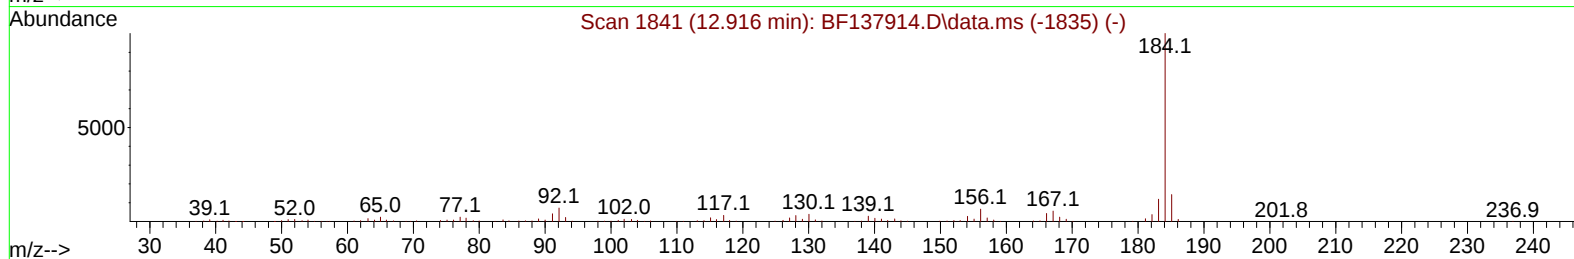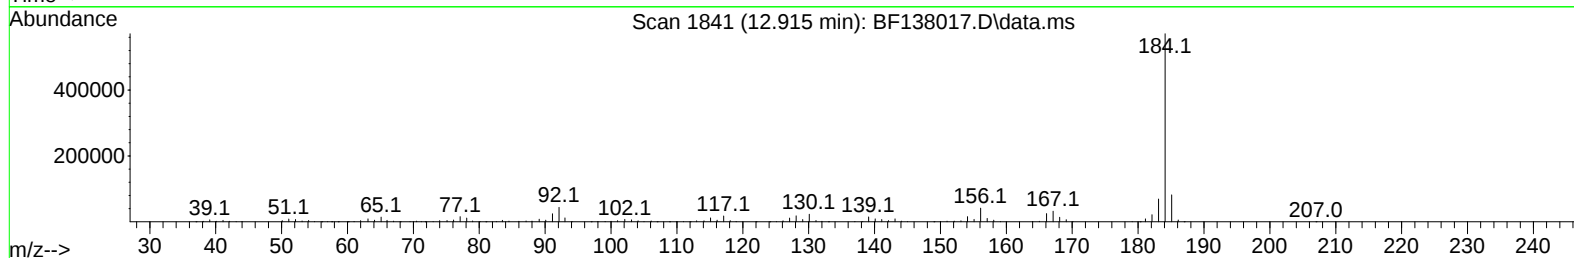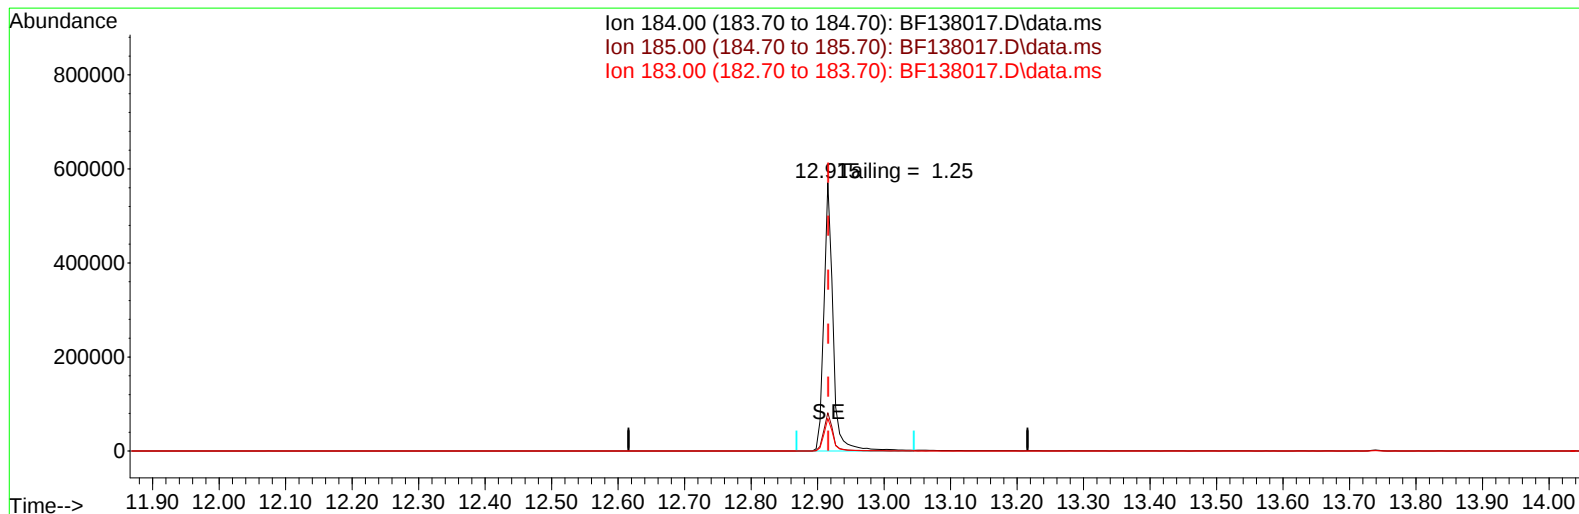

TIC: BF138017.D\data.ms

(77) Benzidine**12.915min (-0.001) 635082.55 ng****response 547789**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	14.29
183.00	11.90	12.13
0.00	0.00	0.00