

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052324\
Data File : BF138026.D
Acq On : 23 May 2024 14:20
Operator : CG\JU
Sample : PB161081BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB161081BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF051424.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF138026.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.128	3	7	11	rVB	5976654	8181014	100.00%	23.092%
2	2.475	51	66	71	rVB	54951	83579	1.02%	0.236%
3	5.669	604	609	612	rBV	3387442	3462966	42.33%	9.775%
4	6.651	770	776	779	rBV	3017520	3378735	41.30%	9.537%
5	7.034	837	841	844	rBV	977493	770726	9.42%	2.175%
6	7.598	930	937	940	rBV	2020461	2258452	27.61%	6.375%
7	8.316	1054	1059	1062	rBV	1224544	1042739	12.75%	2.943%
8	9.392	1236	1242	1245	rBV	4898026	4712357	57.60%	13.301%
9	10.081	1353	1359	1362	rBV	1506220	1234278	15.09%	3.484%
10	10.875	1489	1494	1497	rBV	3160883	2739897	33.49%	7.734%
11	11.575	1609	1613	1629	rVB	1518267	1253161	15.32%	3.537%
12	13.163	1878	1883	1886	rBV	4914274	4818668	58.90%	13.601%
13	14.227	2060	2064	2079	rBV	812579	831122	10.16%	2.346%
14	15.792	2324	2330	2344	rBV	416340	660866	8.08%	1.865%




Sum of corrected areas: 35428560

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052324\
Data File : BF138026.D
Acq On : 23 May 2024 14:20
Operator : CG\JU
Sample : PB161081BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB161081BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF051424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

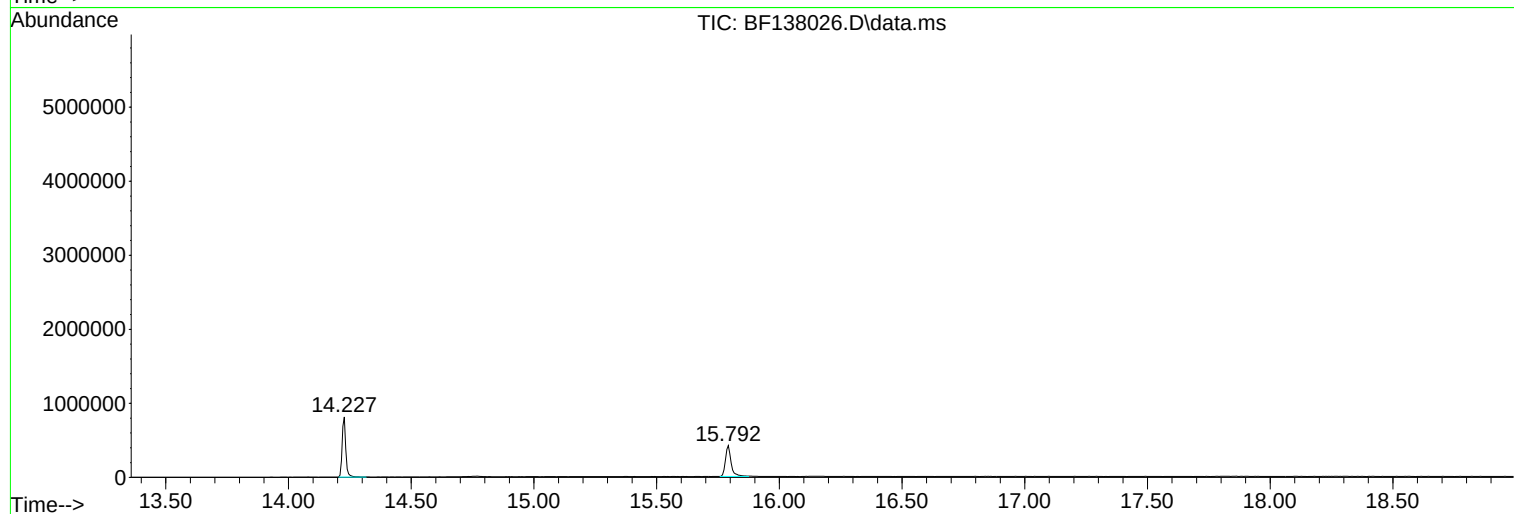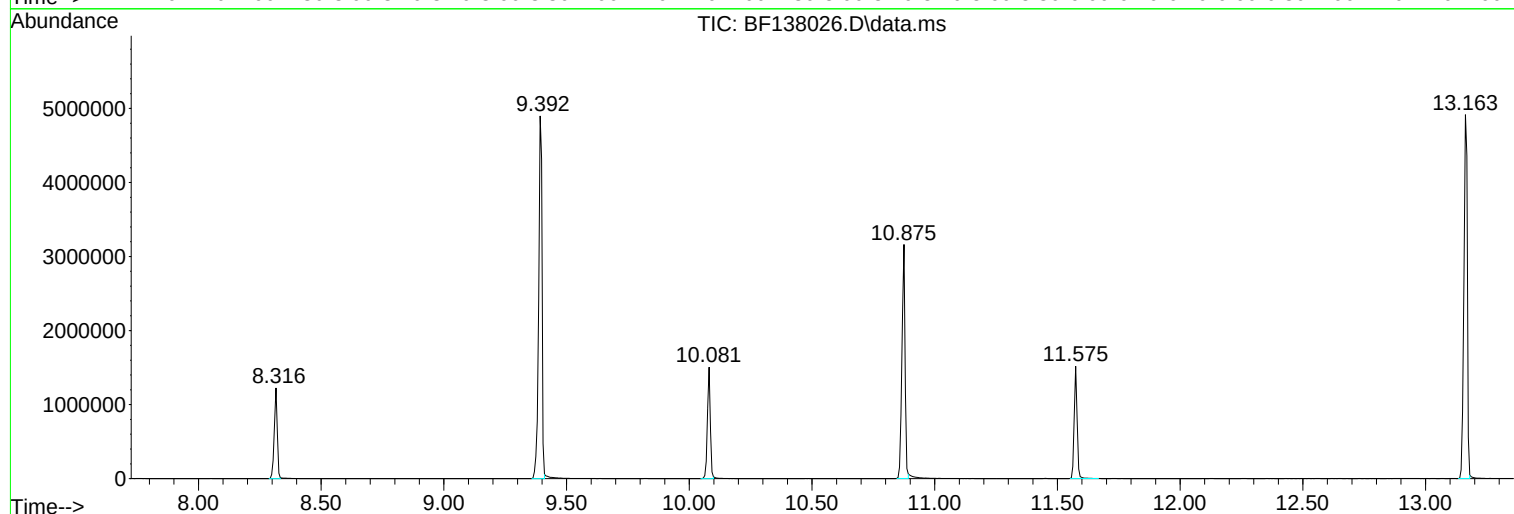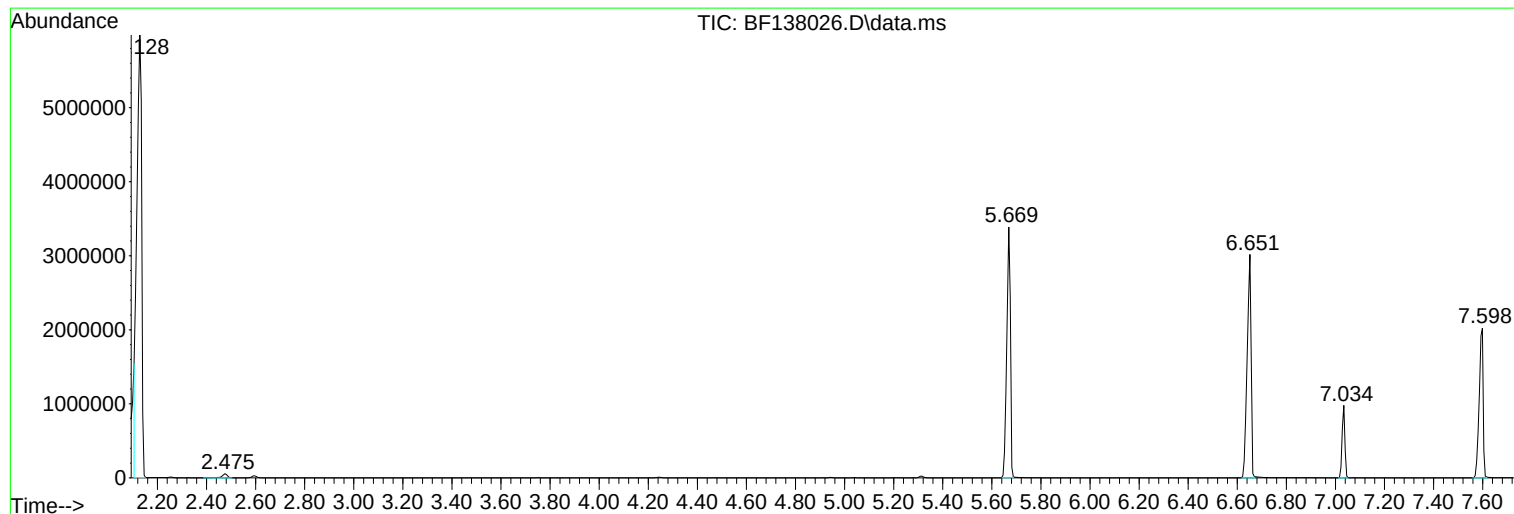

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052324\
Data File : BF138026.D
Acq On : 23 May 2024 14:20
Operator : CG\JU
Sample : PB161081BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB161081BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF051424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052324\
Data File : BF138026.D
Acq On : 23 May 2024 14:20
Operator : CG\JU
Sample : PB161081BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB161081BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF051424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------