


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052324\
Data File : BF138017.D
Acq On : 23 May 2024 09:47
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF051424.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed May 15 04:12:16 2024

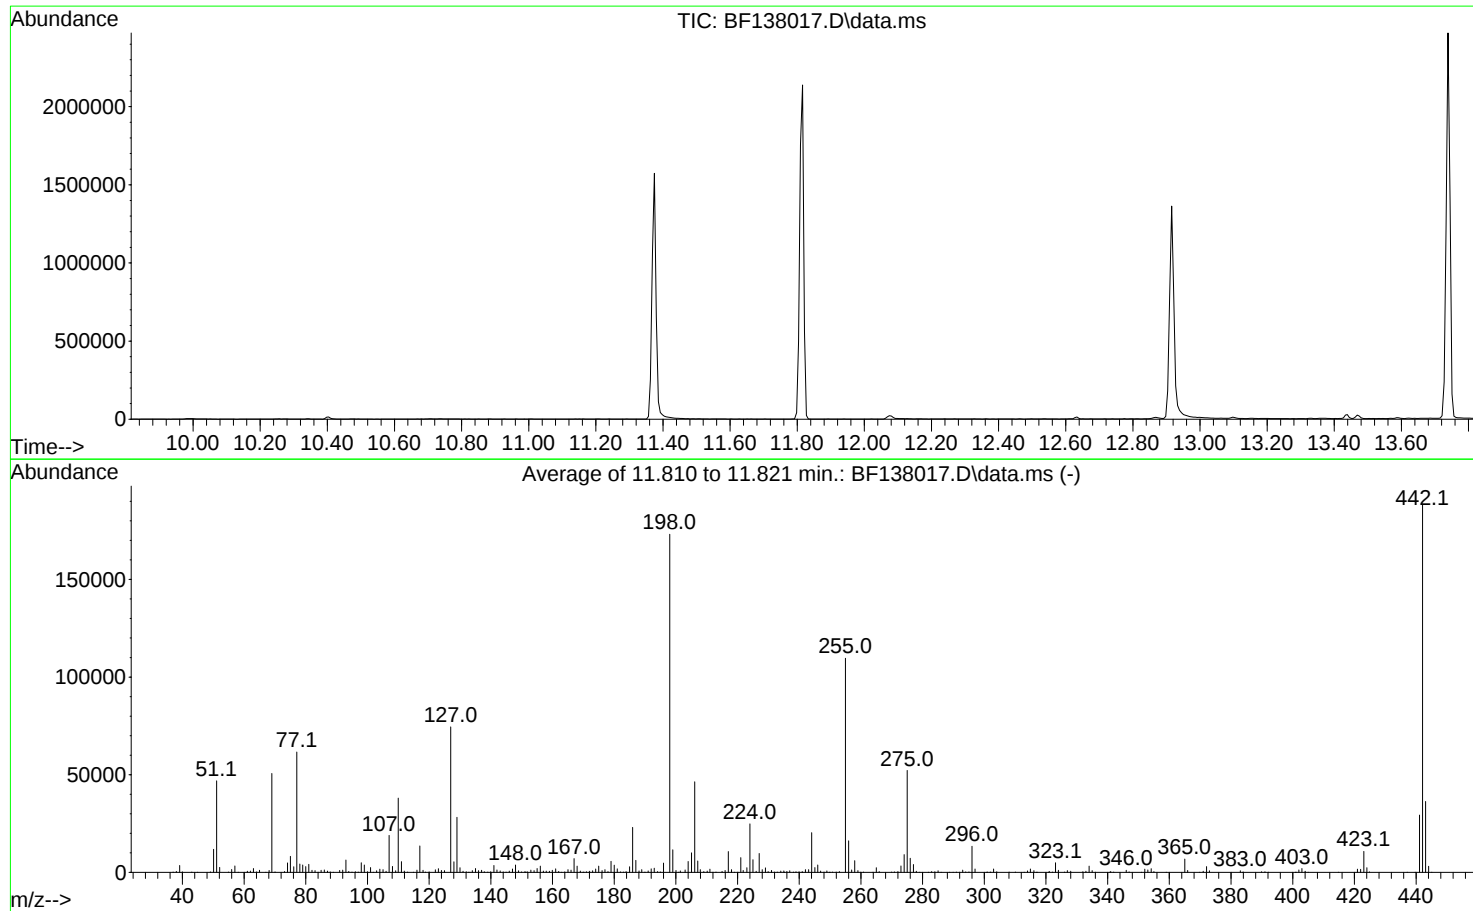




AutoFind: Scans 1653, 1654, 1655; Background Corrected with Scan 1647

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.1	46847	PASS
68	69	0.00	2	1.9	982	PASS
69	198	0.00	100	29.2	50620	PASS
70	69	0.00	2	0.6	286	PASS
127	198	10	80	43.0	74499	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	173099	PASS
199	198	5	9	6.7	11568	PASS
275	198	10	60	30.1	52168	PASS
365	198	1	100	3.9	6779	PASS
441	198	0.01	100	16.9	29304	PASS
442	442	50	100	100.0	188373	PASS
443	442	15	24	19.3	36320	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052324\
Data File : BF138017.D
Acq On : 23 May 2024 09:47
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 23 11:02:56 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF051424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 15 04:12:16 2024
Response via : Initial Calibration

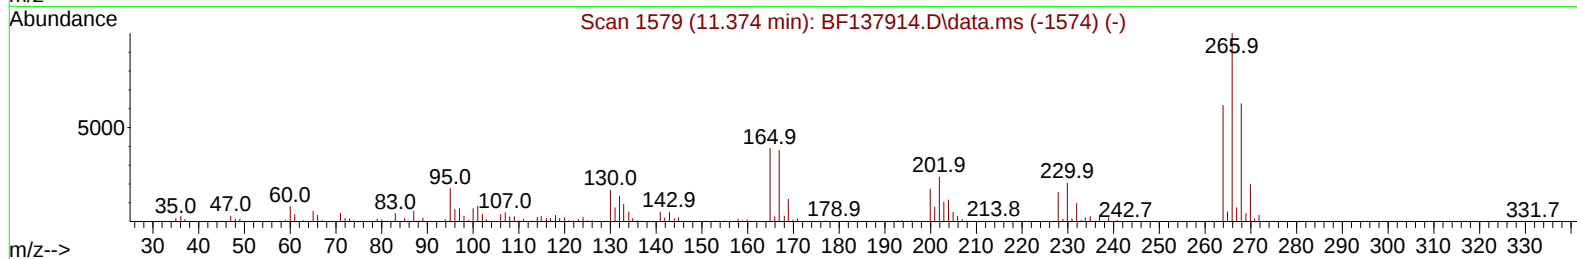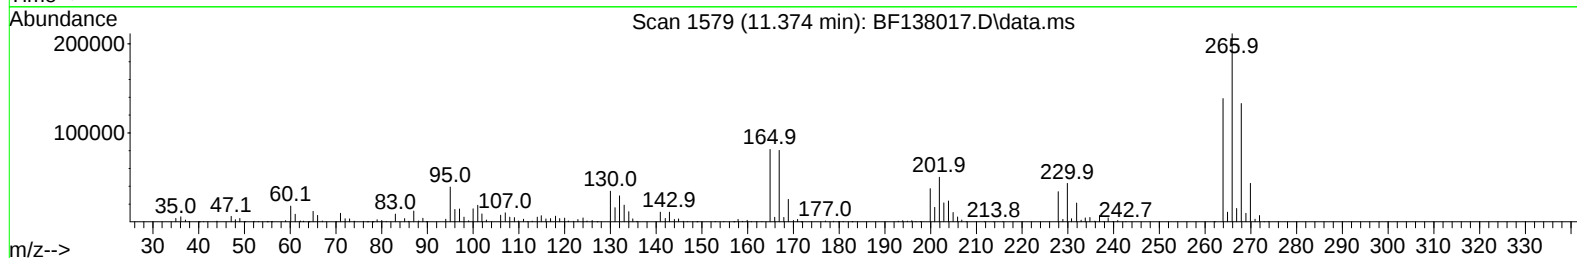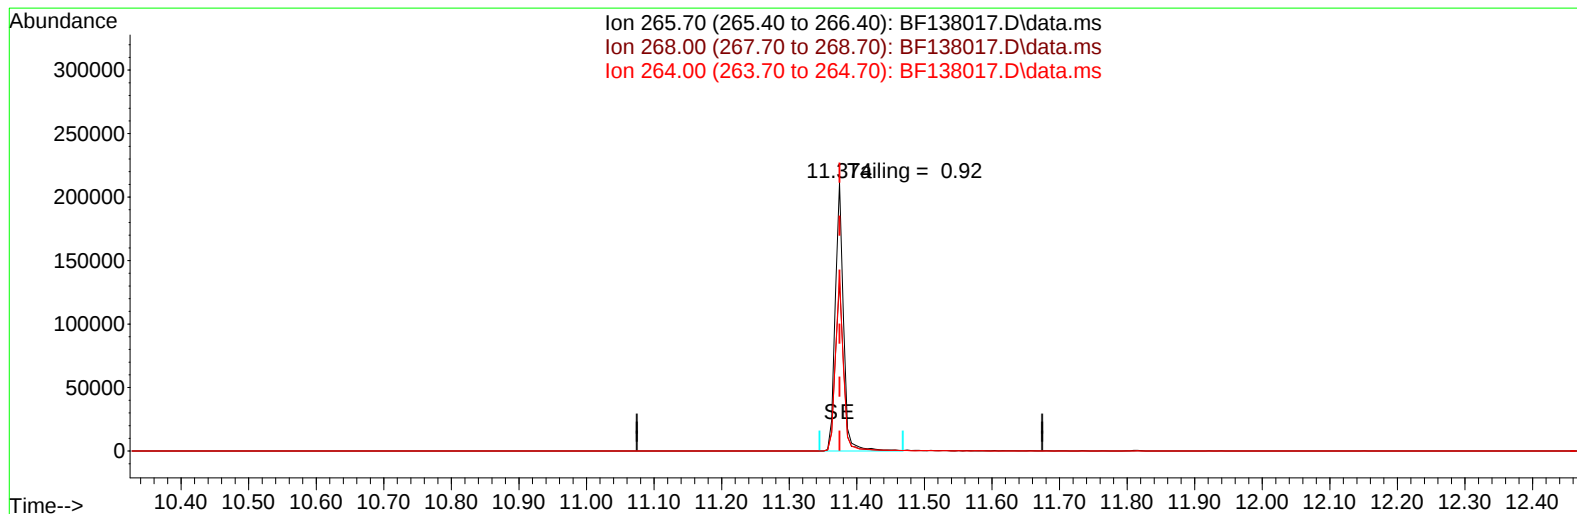

TIC: BF138017.D\data.ms

(70) Pentachlorophenol (C)

11.374min (-0.000) 27966.53 ng




response 179262

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	62.91
264.00	61.80	65.58
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052324\
Data File : BF138017.D
Acq On : 23 May 2024 09:47
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 23 11:02:56 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF051424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 15 04:12:16 2024
Response via : Initial Calibration

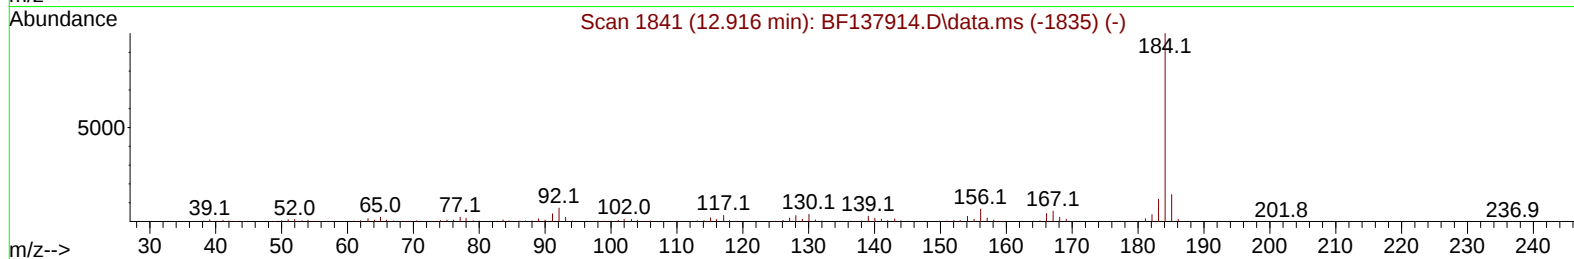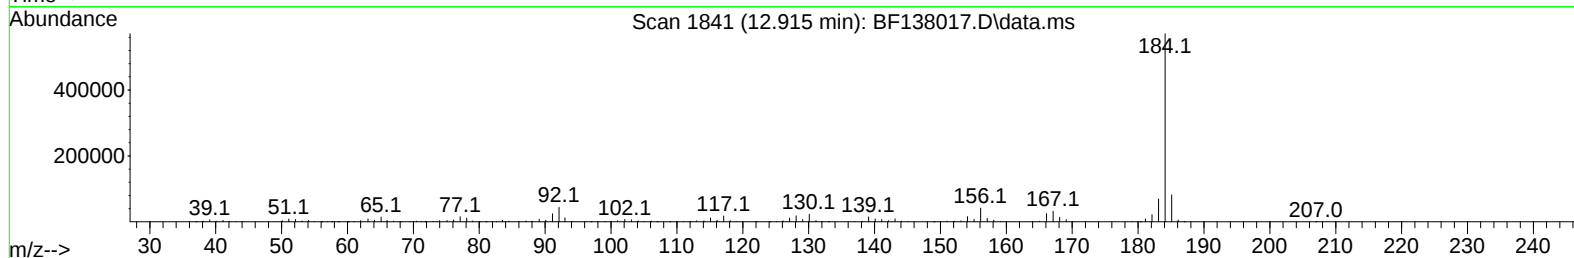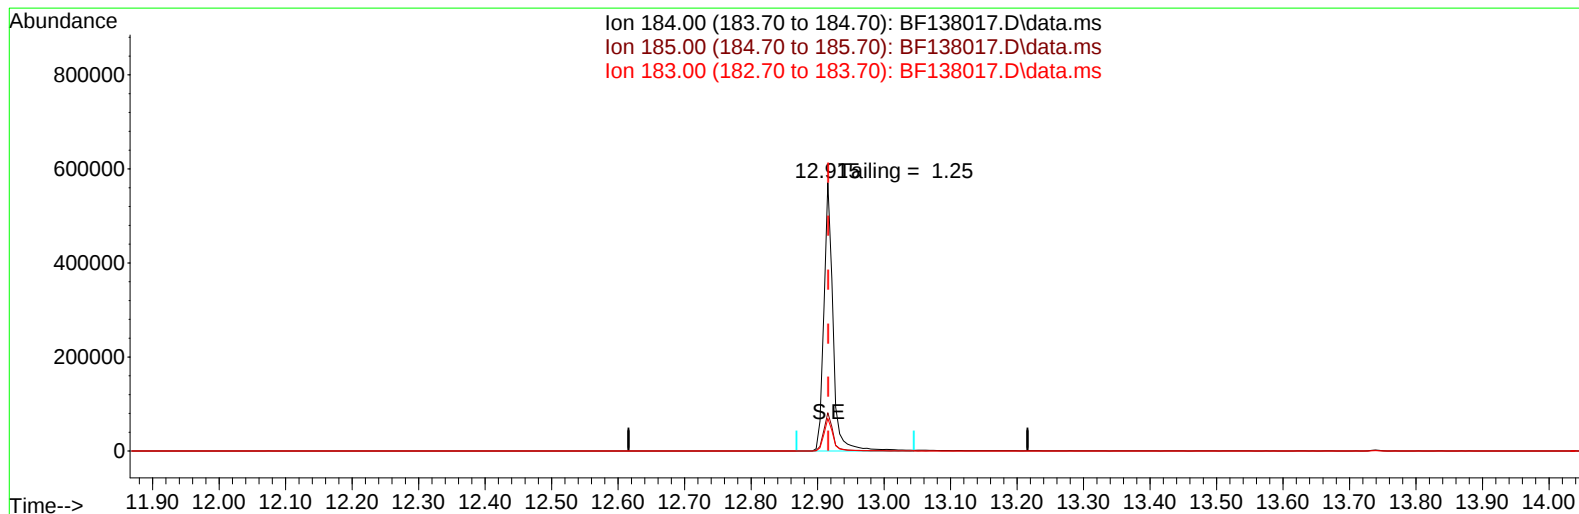

TIC: BF138017.D\data.ms

(77) Benzidine

12.915min (-0.001) 635082.55 ng

response 547789

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	14.29
183.00	11.90	12.13
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/23/2024	BNA_F	<u>BF138017.D</u>
Compound Name	Response	Retention Time
DDT	405953	13.739
DDD	9236	13.439
DDE	1282	13.098
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10518	416471	2.53

Instrument :
BNA_F
ClientSampleId :
DFTPP