
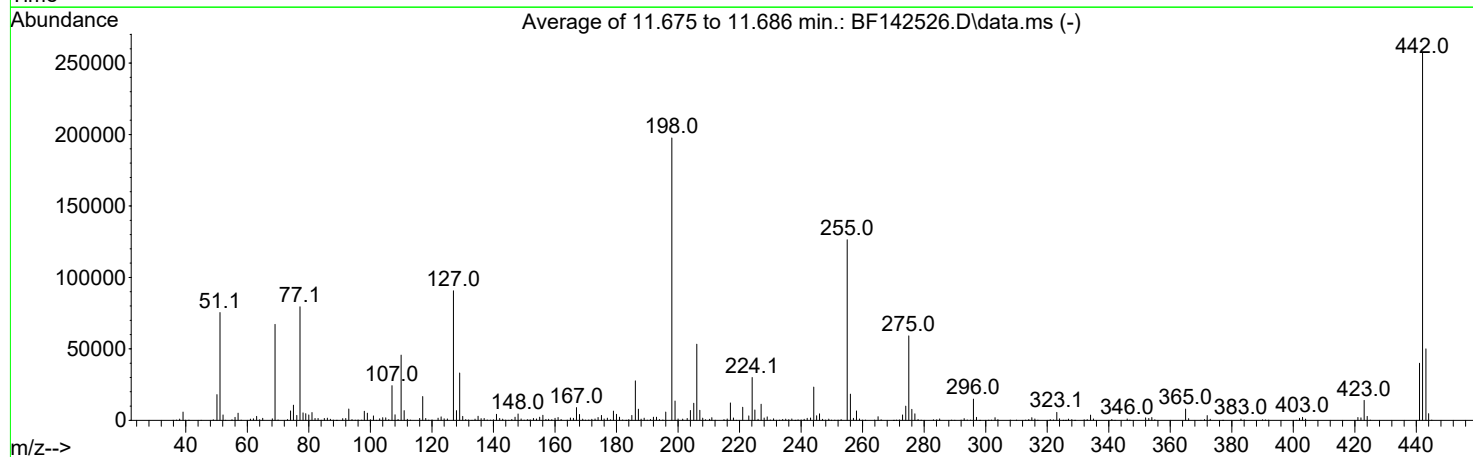


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052325\
Data File : BF142526.D
Acq On : 23 May 2025 10:43
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052025.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue May 20 16:26:47 2025

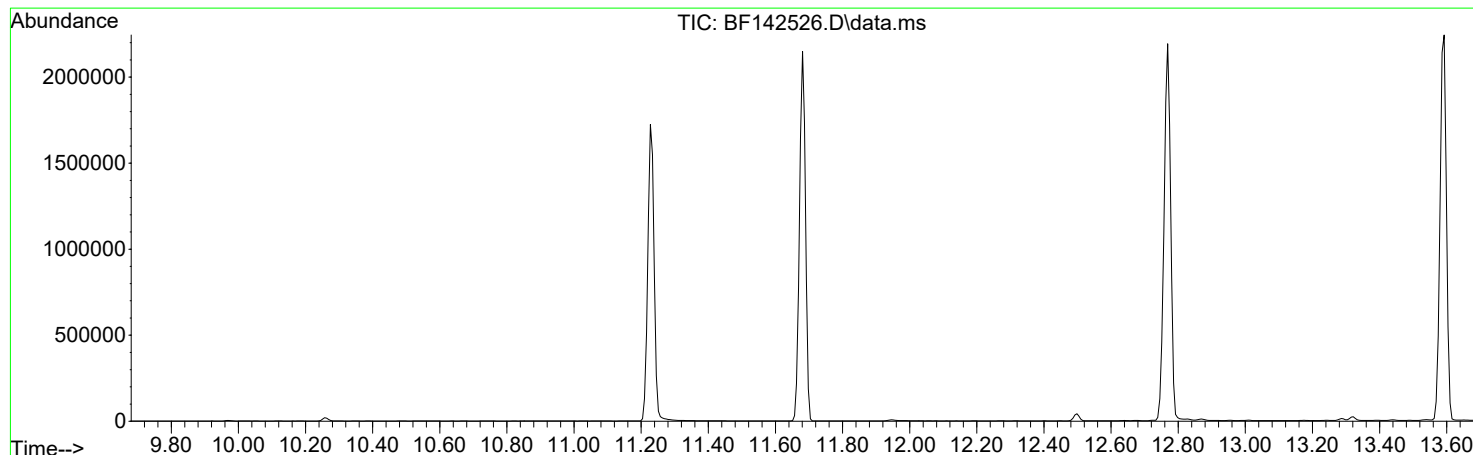

AutoFind: Scans 1612, 1613, 1614; Background Corrected with Scan 1605

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.2	75485	PASS
68	69	0.00	2	1.7	1160	PASS
69	198	0.00	100	34.0	67144	PASS
70	69	0.00	2	0.5	354	PASS
127	198	10	80	45.9	90704	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	197568	PASS
199	198	5	9	6.8	13522	PASS
275	198	10	60	29.9	59096	PASS
365	198	1	100	4.1	8009	PASS
441	198	0.01	100	20.2	39968	PASS
442	442	50	100	100.0	257387	PASS
443	442	15	24	19.5	50077	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/23/2025	BNA_F	<u>BF142526.D</u>
Compound Name	Response	Retention Time
DDT	607232	13.592
DDD	10711	13.322
DDE	553	12.951
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11264	618496	1.82

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052325\
Data File : BF142526.D
Acq On : 23 May 2025 10:43
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 23 11:43:30 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 20 16:26:47 2025
Response via : Initial Calibration

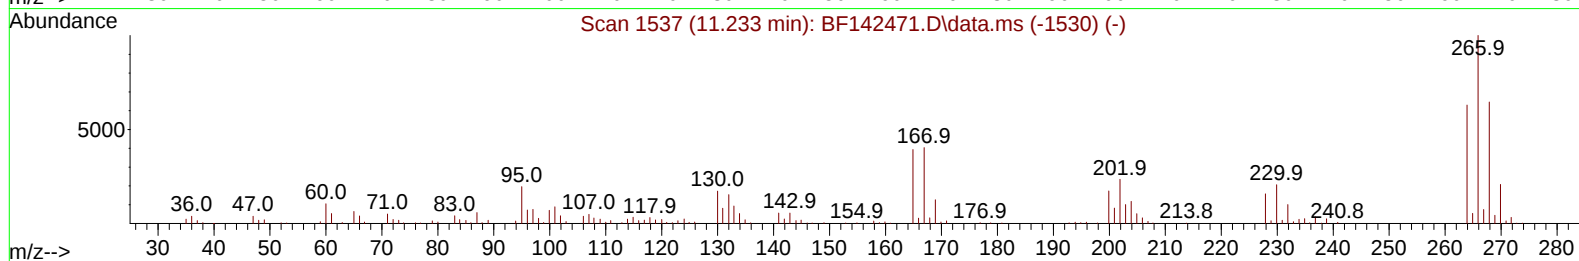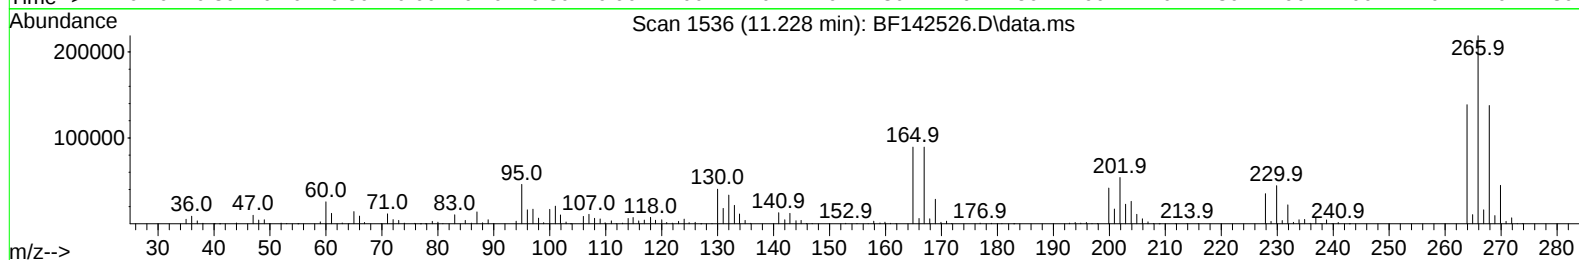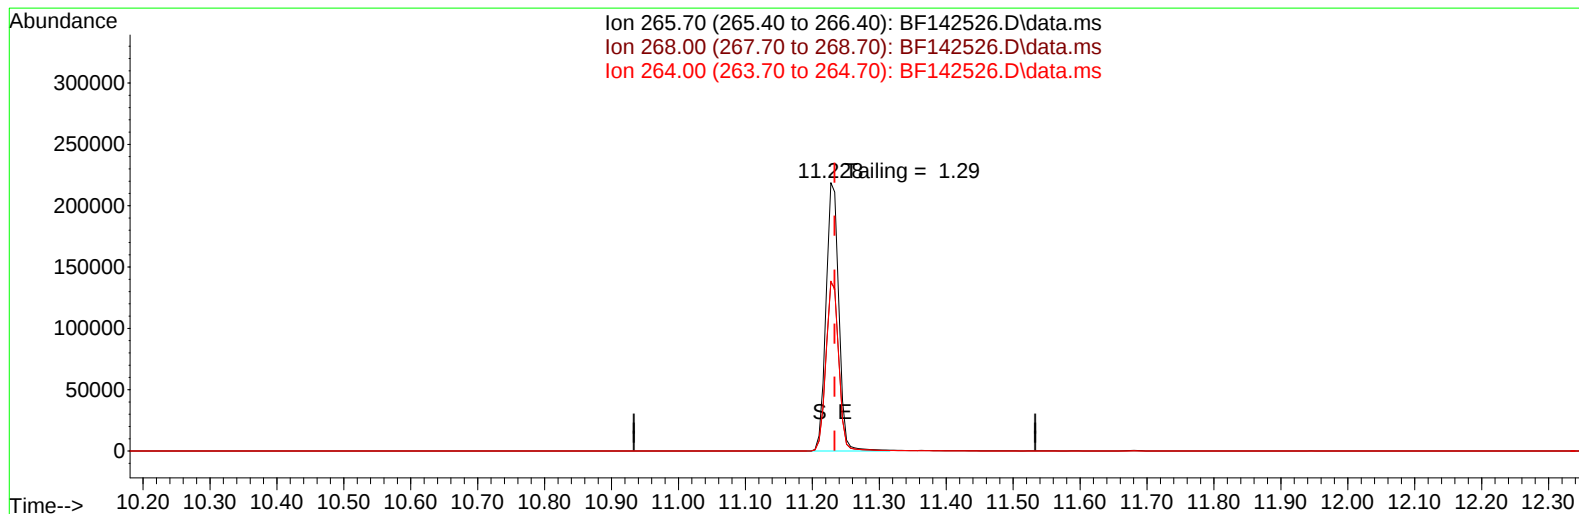

TIC: BF142526.D\data.ms

(70) Pentachlorophenol (C)

11.228min (-0.006) 71983.90 ng




response 293388

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.60	62.88
264.00	63.00	63.32
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052325\
Data File : BF142526.D
Acq On : 23 May 2025 10:43
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 23 11:43:30 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 20 16:26:47 2025
Response via : Initial Calibration

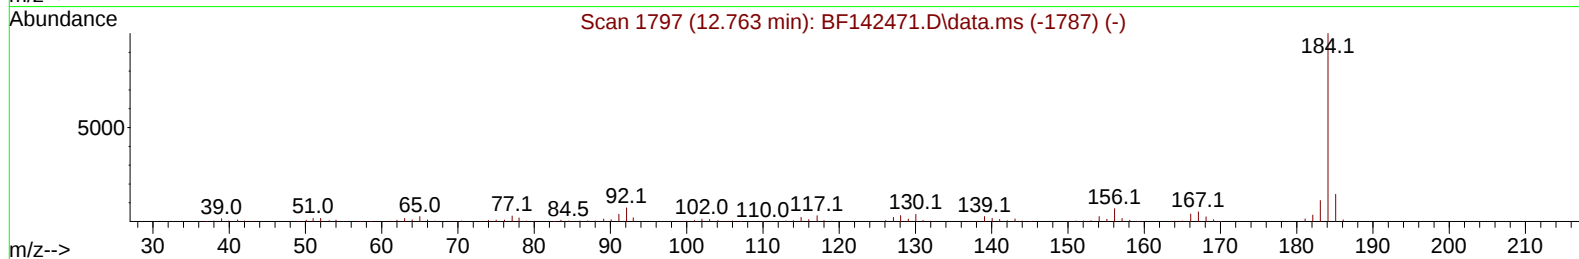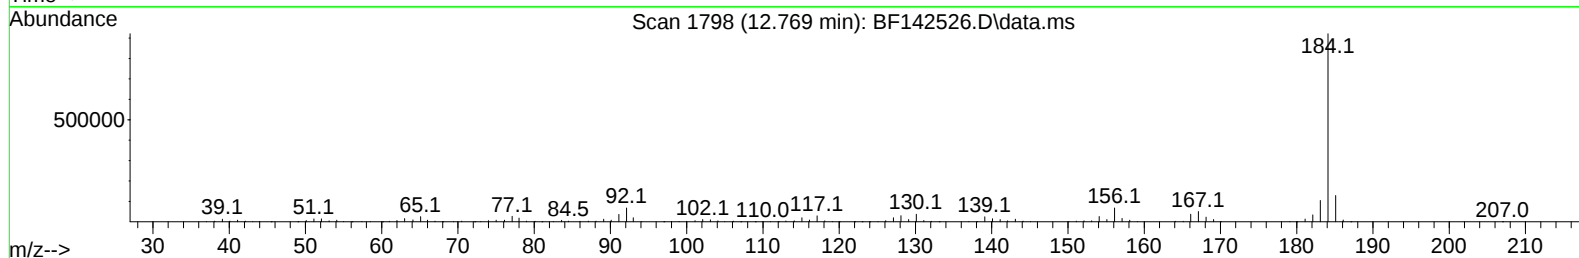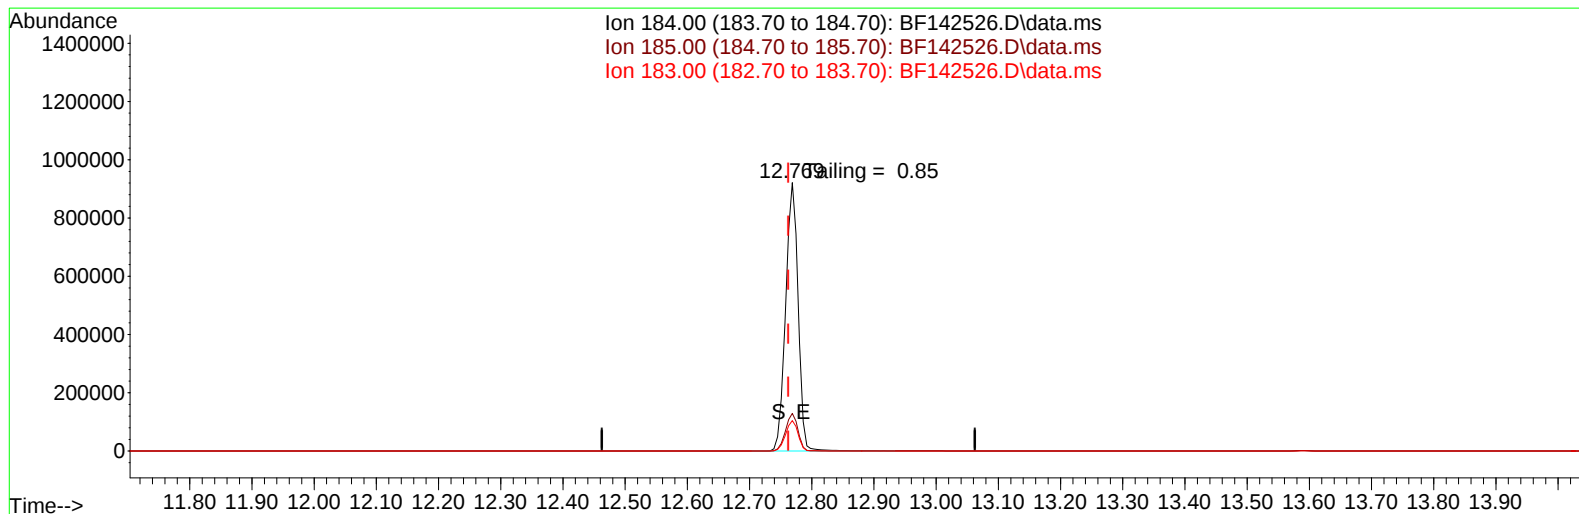

TIC: BF142526.D\data.ms

(77) Benzidine

12.769min (+ 0.006) 73026.94 ng

response 1290837

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.00
183.00	11.20	11.37
0.00	0.00	0.00